

CE Diameter Report - Number Distribution



Measurement Details

Sample Name: Tylose MH100001 P6 DEAT135417

SOP Name: MATERIE PRIME.vsop

Edited: True

User Name: Russo

Edited On: 12 March 2014 10:02:11

Date: 12 March 2014 09:51:06

Analysis

SOP Analysis: 3.0

SOP Fill Holes: True

SOP Segmentation: None

SOP Trash Size: 10

SOP Optic(s) used: 50x

Particles Counted: 3399

Result

CE Diameter Minimum (μm): 0.22

CE Diameter D[n, 0.1] (μm): 0.23

CE Diameter Maximum (μm): 74.80

CE Diameter D[n, 0.5] (μm): 0.38


CE Diameter Mean (μm): 1.68

CE Diameter D[n, 0.9] (μm): 3.11

CE Diameter STDV (μm): 5.22

CE Diameter RSD (%): 311.36

CE Diameter (μm) smoothed over 11 points

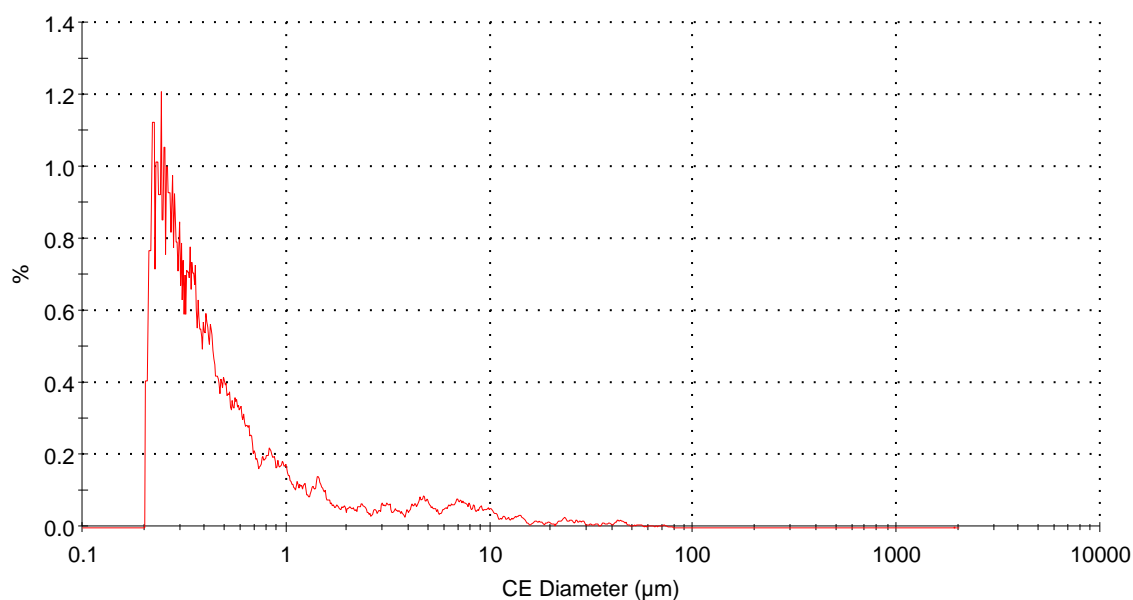

Record 163: Tylose MH100001 P6 DEAT135417

Comments:

Morphologi

Malvern Instruments Worldwide

www.malvern.com