

Intensity Mean Report - Number Distribution



Measurement Details

Sample Name: MP 2080

SOP Name: MATERIE PRIME.vsop

Edited: True

User Name: Morphologi

Edited On: 11 April 2014 15:58:56

Date: 11 April 2014 14:01:45

Analysis

SOP Analysis: 3.0

SOP Fill Holes: True

SOP Segmentation: None

SOP Trash Size: 10

SOP Optic(s) used: 20x, 50x

Result

Mean Intensity Minimum: 27

Mean Intensity D[n, 0.1]: 168

Mean Intensity Maximum: 171

Mean Intensity D[n, 0.5]: 169

Mean Intensity Mean: 169


Mean Intensity D[n, 0.9]: 170

Particles Counted: 8872

Mean Intensity STDV: 6

Mean Intensity RSD (%): 3.37

Intensity Mean smoothed over 11 points

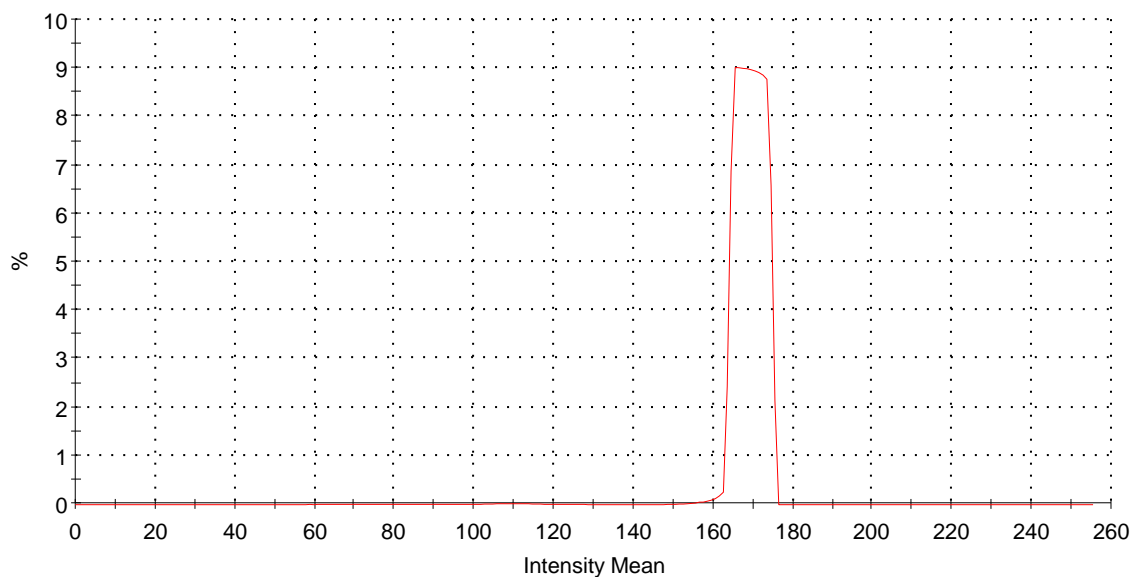

Record 582: MP 2080

Comments:

Morphologi

Malvern Instruments Worldwide

www.malvern.com