

# Intensity Mean Report - Number Distribution



## Measurement Details

**Sample Name:** E-Spheres SLG

**SOP Name:** MATERIE PRIME.vsop

**Edited:** False

**User Name:** Morphologi

**Edited On:** 24 April 2014 17:52:44

**Date:** 24 April 2014 17:52:44

## Analysis

**SOP Analysis:** 3.0

**SOP Fill Holes:** True

**SOP Segmentation:** None

**SOP Trash Size:** 10

**SOP Optic(s) used:** 10x

## Result

**Mean Intensity Minimum:** 25

**Mean Intensity D[n, 0.1]:** 97

**Mean Intensity Maximum:** 146

**Mean Intensity D[n, 0.5]:** 126

**Mean Intensity Mean:** 122


**Mean Intensity D[n, 0.9]:** 139

**Particles Counted:** 3132

**Mean Intensity STDV:** 21

**Mean Intensity RSD (%):** 16.79

Intensity Mean smoothed over 11 points

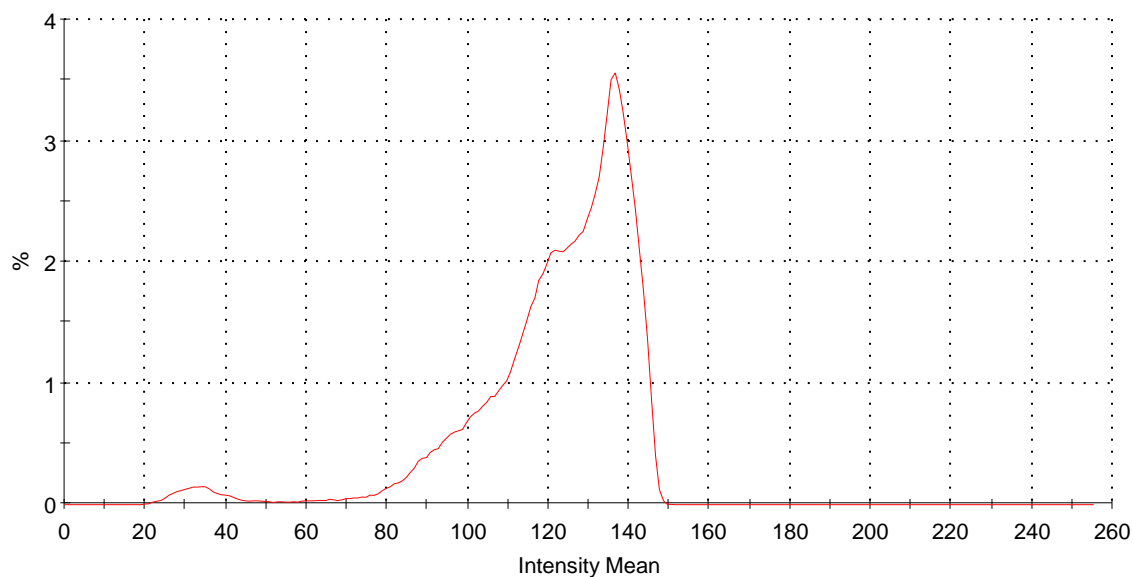

Record 71: E-Spheres SLG

## Comments:

Morphologi

Malvern Instruments Worldwide

[www.malvern.com](http://www.malvern.com)