

HS Circularity - Number Distribution



Measurement Details

Sample Name: HD 1500

SOP Name: MATERIE PRIME.vsop

User Name: Morphologi

Date: 10 April 2014 18:02:39

Edited: False

Edited On: 10 April 2014 18:02:39

Analysis

SOP Analysis: 3.0

SOP Fill Holes: True

SOP Segmentation: None

SOP Trash Size: 10

SOP Optic(s) used: 20x

Result

HS Circularity Minimum: 0.051

HS Circularity D[n, 0.1]: 0.683

HS Circularity Maximum: 1.000

HS Circularity D[n, 0.5]: 0.923

HS Circularity Mean: 0.877


HS Circularity D[n, 0.9]: 0.981

Particles Counted: 10591

HS Circularity STDV: 0.142

HS Circularity RSD (%): 16.131

HS Circularity smoothed over 11 points

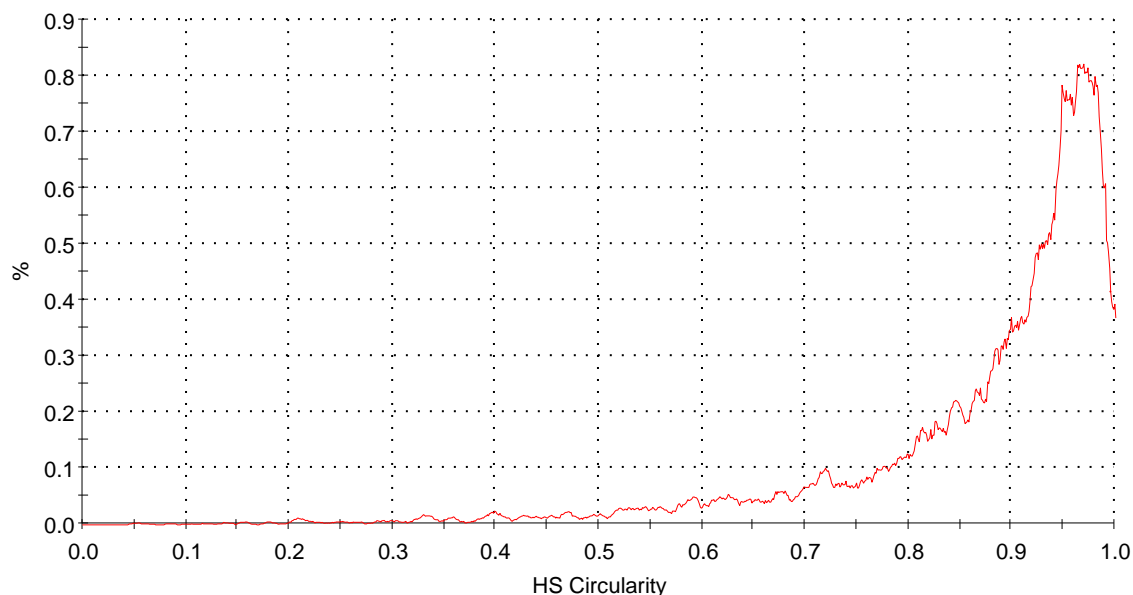

Record 573: HD 1500

Comments:

Morphologi

Malvern Instruments Worldwide

www.malvern.com