

Scattergram CE Diameter VS HS Circularity



Measurement Details

Sample Name: MP 2080

SOP Name: MATERIE PRIME.vsop

Edited: True

User Name: Morphologi

Edited On: 11 April 2014 15:58:56

Date: 11 April 2014 14:01:45

Analysis


SOP Analysis: 3.0

SOP Fill Holes: True

SOP Segmentation: None

SOP Trash Size: 10

SOP Optic(s) used: 20x, 50x

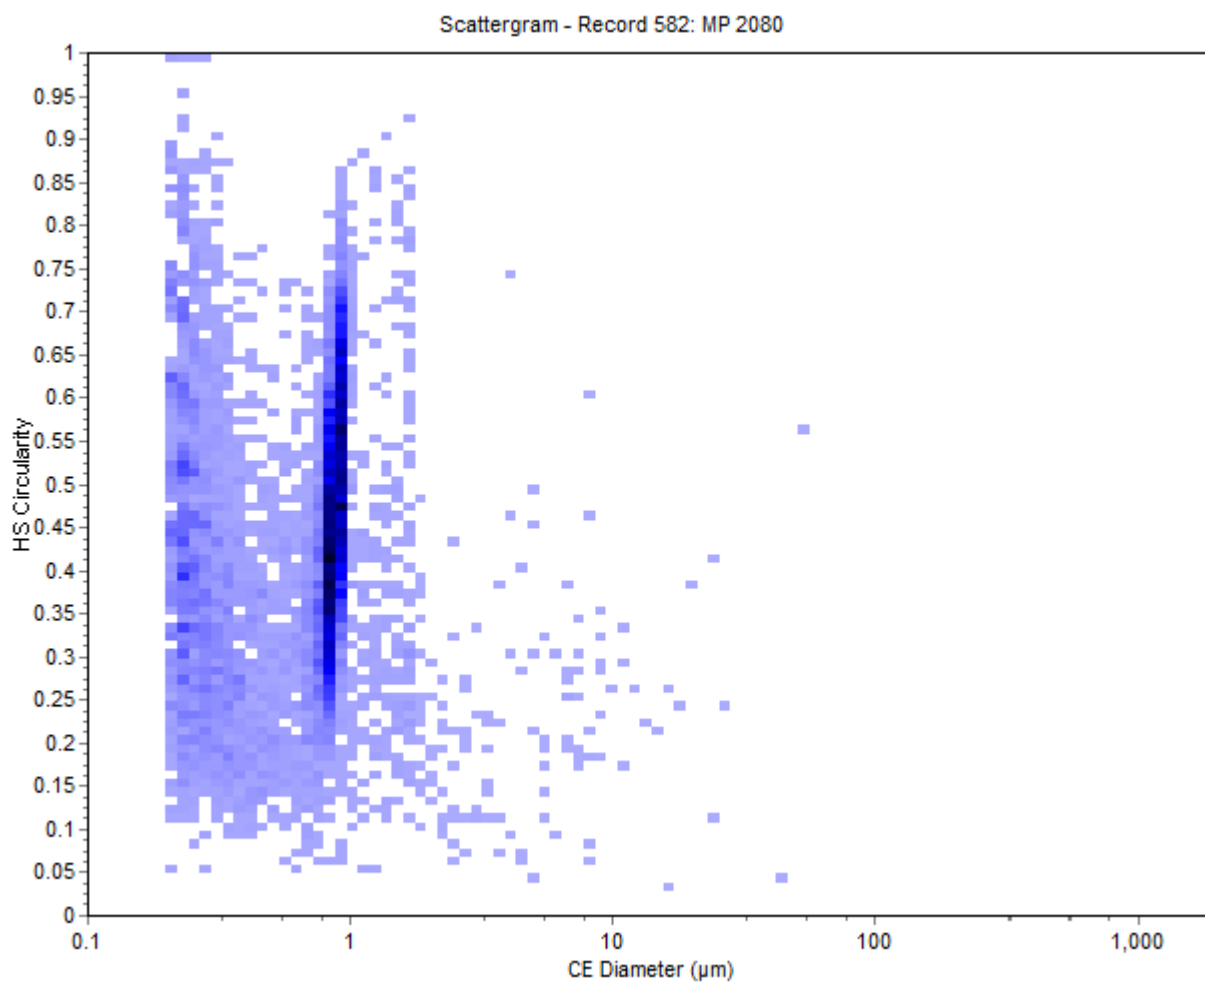

Comments:

Morphologi

Malvern Instruments Worldwide

www.malvern.com