Intensity Mean Report - Number Distribution

Malvern

Measurement Details

Sample Name: Alabastrino

SOP Name: GESSI.vsop

User Name: roberto antonio

Date: 13 June 2014 12:39:52

Edited: False

Edited On: 13 June 2014 12:39:52

Analysis

SOP Analysis: 3.0

SOP Segmentation: None

SOP Optic(s) used: 50x

SOP Fill Holes: True

SOP Trash Size: 10

Result

Mean Intensity Minimum: 51

Mean Intensity Maximum: 151

Mean Intensity Mean: 128

Particles Counted: 30025

Mean Intensity D[n, 0.1]: 98

Mean Intensity D[n, 0.5]: 137
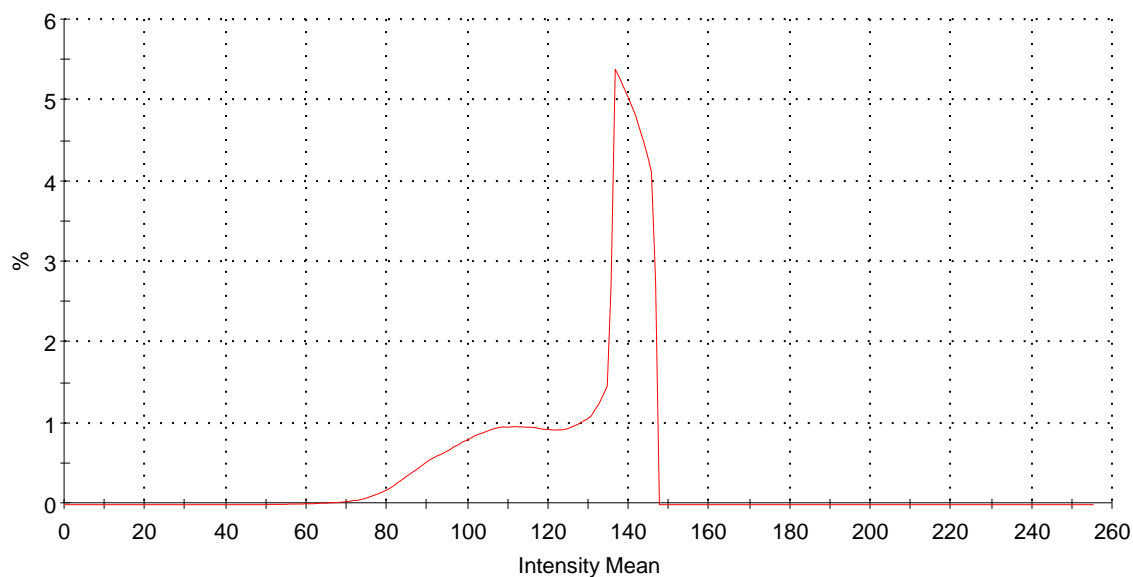
Mean Intensity D[n, 0.9]: 141

Mean Intensity STDV: 18

Mean Intensity RSD (%): 14.09

Intensity Mean smoothed over 11 points

Record 85: Alabastrino

Comments:

Morphologi

Malvern Instruments Worldwide

www.malvern.com