

HS Circularity - Number Distribution



Measurement Details

Sample Name: FX 2300

SOP Name: MATERIE PRIME.vsop

User Name: Morphologi

Date: 10 April 2014 11:44:50

Edited: False

Edited On: 10 April 2014 11:44:50

Analysis

SOP Analysis: 3.0

SOP Fill Holes: True

SOP Segmentation: None

SOP Trash Size: 10

SOP Optic(s) used: 20x

Result

HS Circularity Minimum: 0.046

HS Circularity Maximum: 1.000

HS Circularity Mean: 0.777

Particles Counted: 4932


HS Circularity D[n, 0.1]: 0.466

HS Circularity D[n, 0.5]: 0.844

HS Circularity D[n, 0.9]: 0.956

HS Circularity STDV: 0.195

HS Circularity RSD (%): 25.114

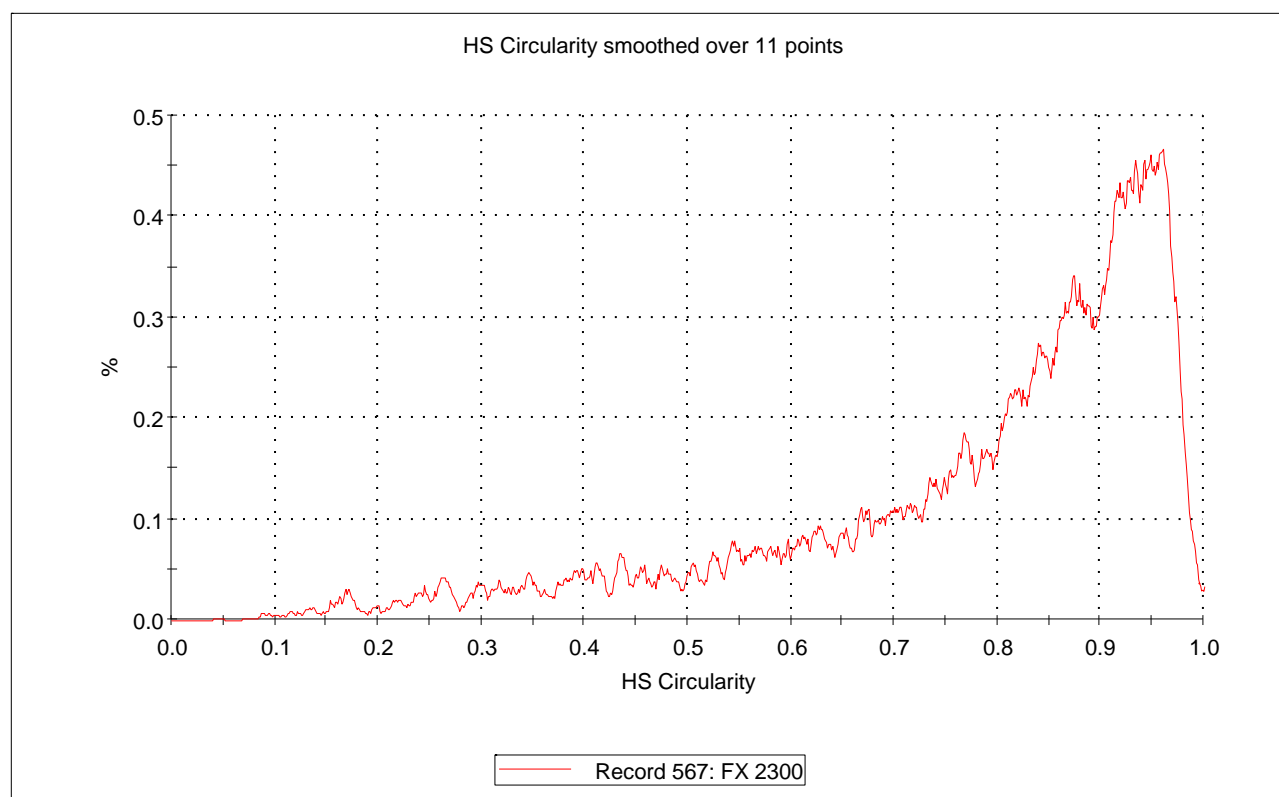

Comments: