

Scattergram CE Diameter VS HS Circularity



Measurement Details

Sample Name: FLEX 8310

SOP Name: MATERIE PRIME.vsop

Edited: True

User Name: Morphologi

Edited On: 16 April 2014 09:54:11

Date: 16 April 2014 09:46:23

Analysis


SOP Analysis: 3.0

SOP Fill Holes: True

SOP Segmentation: None

SOP Trash Size: 10

SOP Optic(s) used: 20x

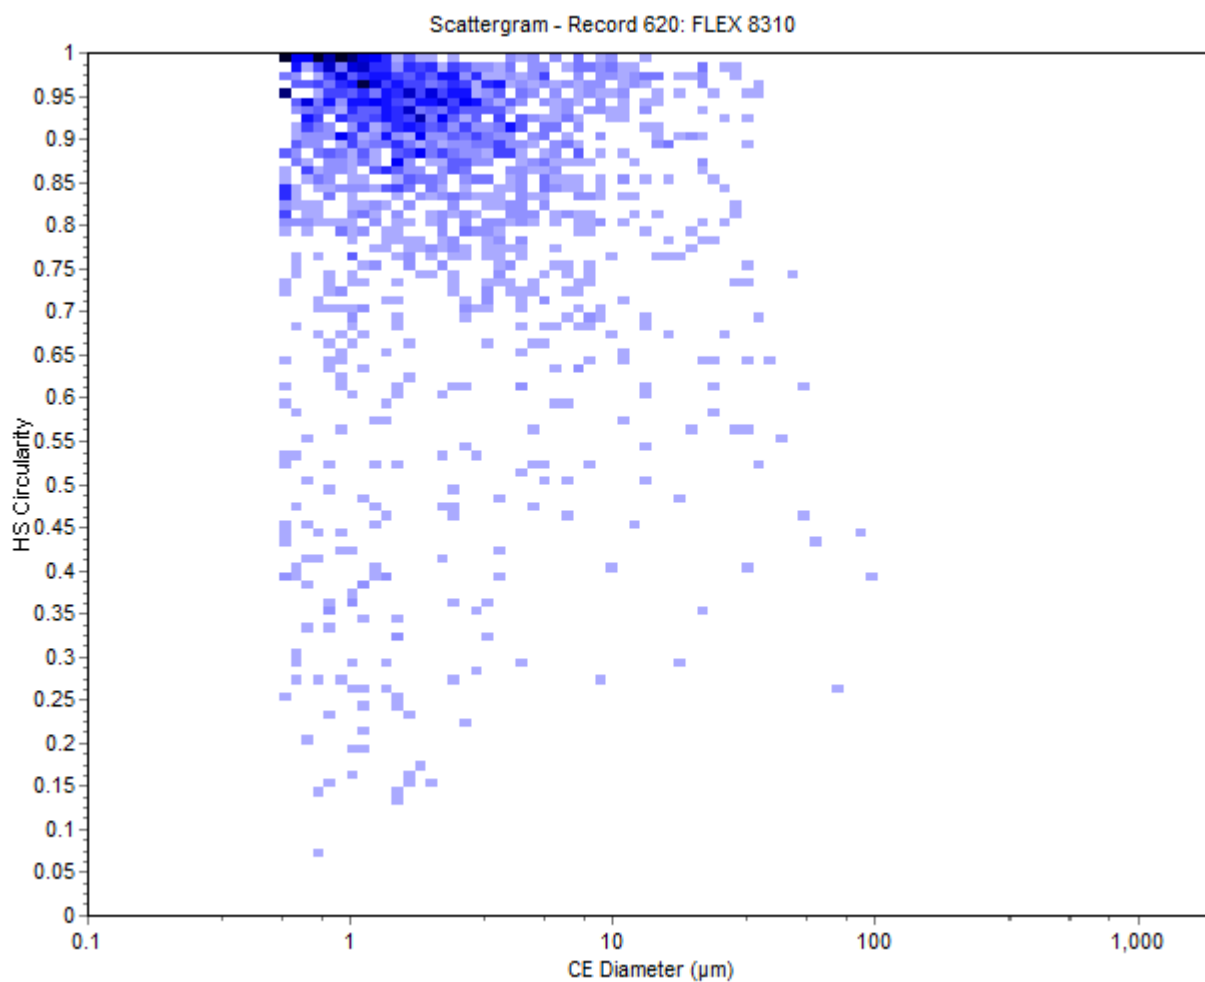

Comments:

Morphologi

Malvern Instruments Worldwide

www.malvern.com