

HS Circularity - Number Distribution



Measurement Details

Sample Name: DRY D1 C

SOP Name: MATERIE PRIME.vsop

User Name: Morphologi

Date: 28 April 2014 17:36:25

Edited: True

Edited On: 29 April 2014 08:29:25

Analysis

SOP Analysis: 3.0

SOP Fill Holes: True

SOP Segmentation: None

SOP Trash Size: 10

SOP Optic(s) used: 20x, 50x

Result

HS Circularity Minimum: 0.051

HS Circularity D[n, 0.1]: 0.546

HS Circularity Maximum: 1.000

HS Circularity D[n, 0.5]: 0.853


HS Circularity Mean: 0.799

HS Circularity D[n, 0.9]: 0.956

Particles Counted: 45250

HS Circularity STDV: 0.166

HS Circularity RSD (%): 20.771

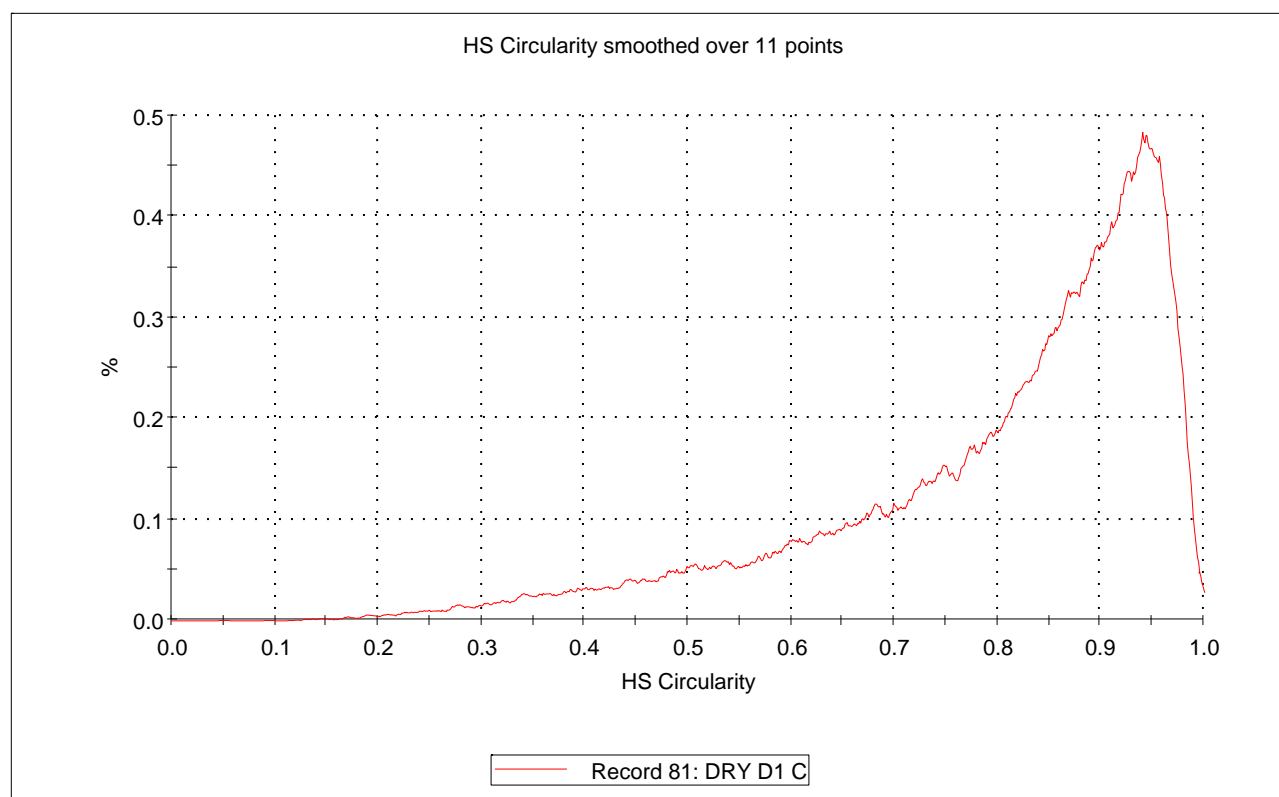

Comments: