HS Circularity - Number Distribution

Malvern

Measurement Details

Sample Name: MP 2100

SOP Name: MATERIE PRIME.vsop

User Name: Morphologi

Date: 14 April 2014 13:58:10

Edited: True

Edited On: 14 April 2014 14:33:09

Analysis

SOP Analysis: 3.0

SOP Segmentation: None

SOP Optic(s) used: 20x

SOP Fill Holes: True

SOP Trash Size: 10

Result

HS Circularity Minimum: 0.064

HS Circularity Maximum: 1.000

HS Circularity Mean: 0.659

Particles Counted: 3008

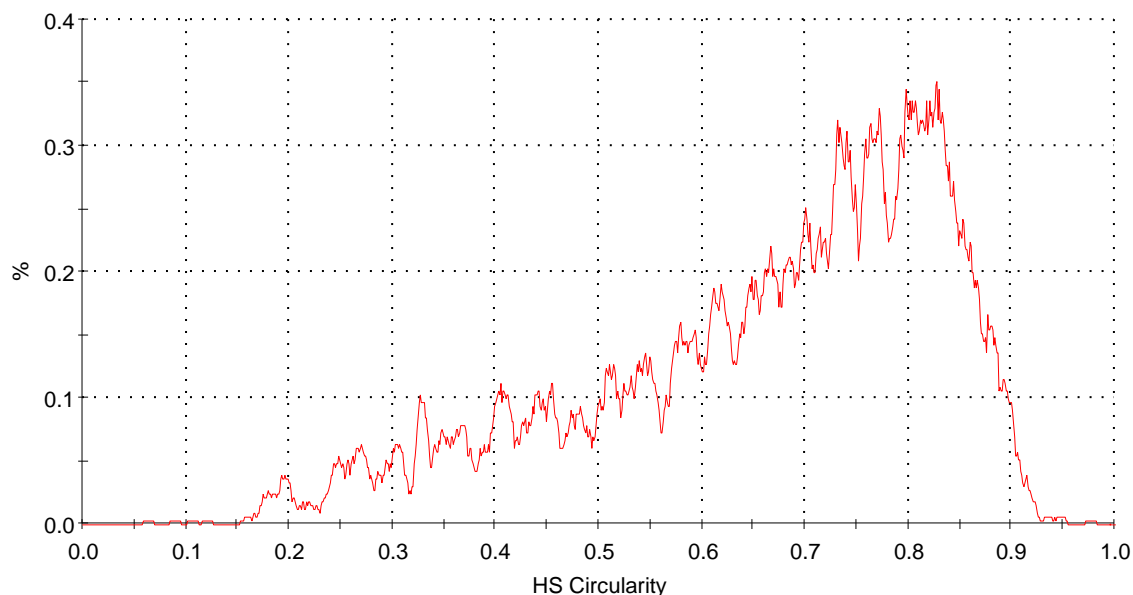**HS Circularity D[n, 0.1]:** 0.388

HS Circularity D[n, 0.5]: 0.703

HS Circularity D[n, 0.9]: 0.845

HS Circularity STDV: 0.175

HS Circularity RSD (%): 26.503

HS Circularity smoothed over 11 points

Record 596: MP 2100

Comments:

Morphologi

Malvern Instruments Worldwide

www.malvern.com