

SIGLENT

SDS 1052DL+
Digital Storage Oscilloscope

Easy hunting

50 MHz
500 MSa/s


glent

Armed

$\Delta V = ***$

CurB = ***

CurA = ***

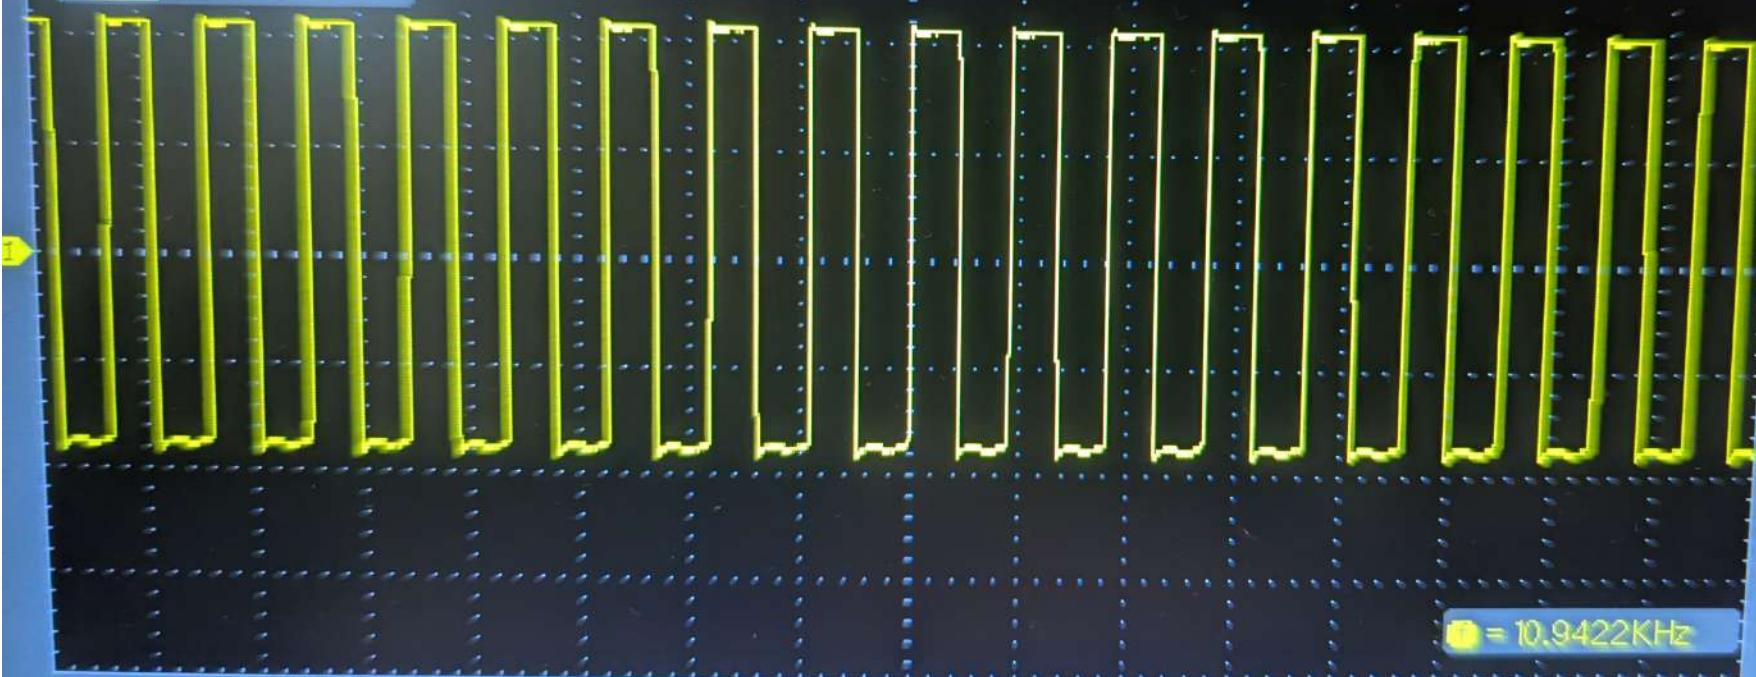

$f = 10.9422\text{KHz}$

CH1 = 2.00V

M 100 μs

M Pos: 0.00 μs

CH1 / 0.00mV

Print

SIGLENT

SDS 1052DL+
Digital Storage Oscilloscope

Easy hunting

50 MHz
500 MSa/s


Siglent

Trig'd

$\Delta V = \text{***}$

CurB = ***

CurA = ***

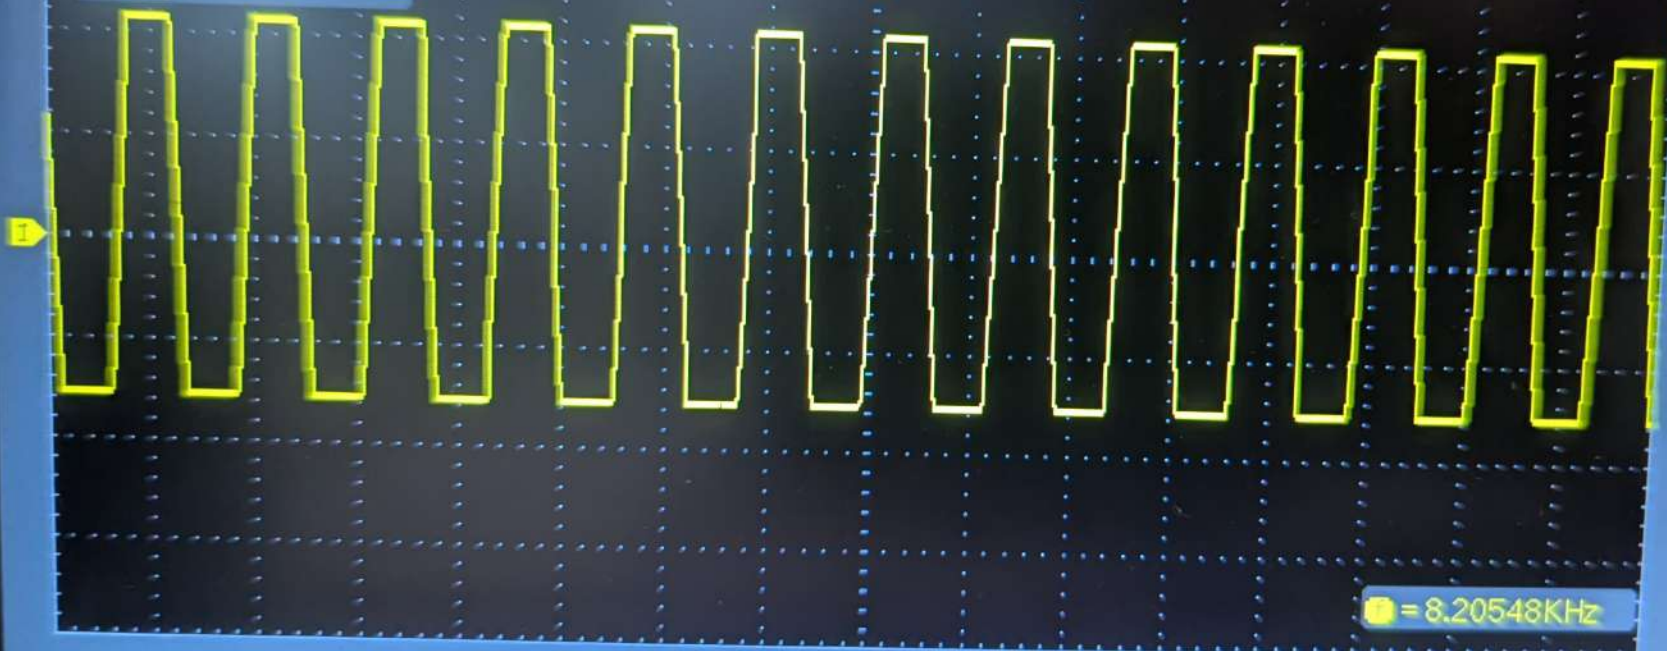

CH1=2.00V

M 100 μ s

MPos:0.00 μ s

CH1 /0.00mV

Print