

**BiofilmQ-HT**

Crystal violet assay · Tecan i-control

1 Plate map

2 Upload data

3 **Results**

Antibiofilm Results

20 strains/conditions grouped in 1 media condition(s) · 3 total blank wells

Publication-ready report

One PDF with methodology, thresholds used, instrument metadata, summary statistics, the chart, the full results table and the plate heatmap — ready to attach to a manuscript, thesis, or lab notebook.

 **Generate PDF report**

✓ Summary

20Strains/Conditions
analysed**1**

Media condition(s)

3

Total blank wells

99.5%Highest %
Inhibition**17**

Strong inhibition

1

Moderate inhibition

0

Weak inhibition

2

No/low inhibition

% Inhibition by strain/condition

Strong inhibition (≥75%)


Moderate inhibition (≥50%)

Weak inhibition (≥25%)

No/low inhibition

--- threshold lines

 **PNG**

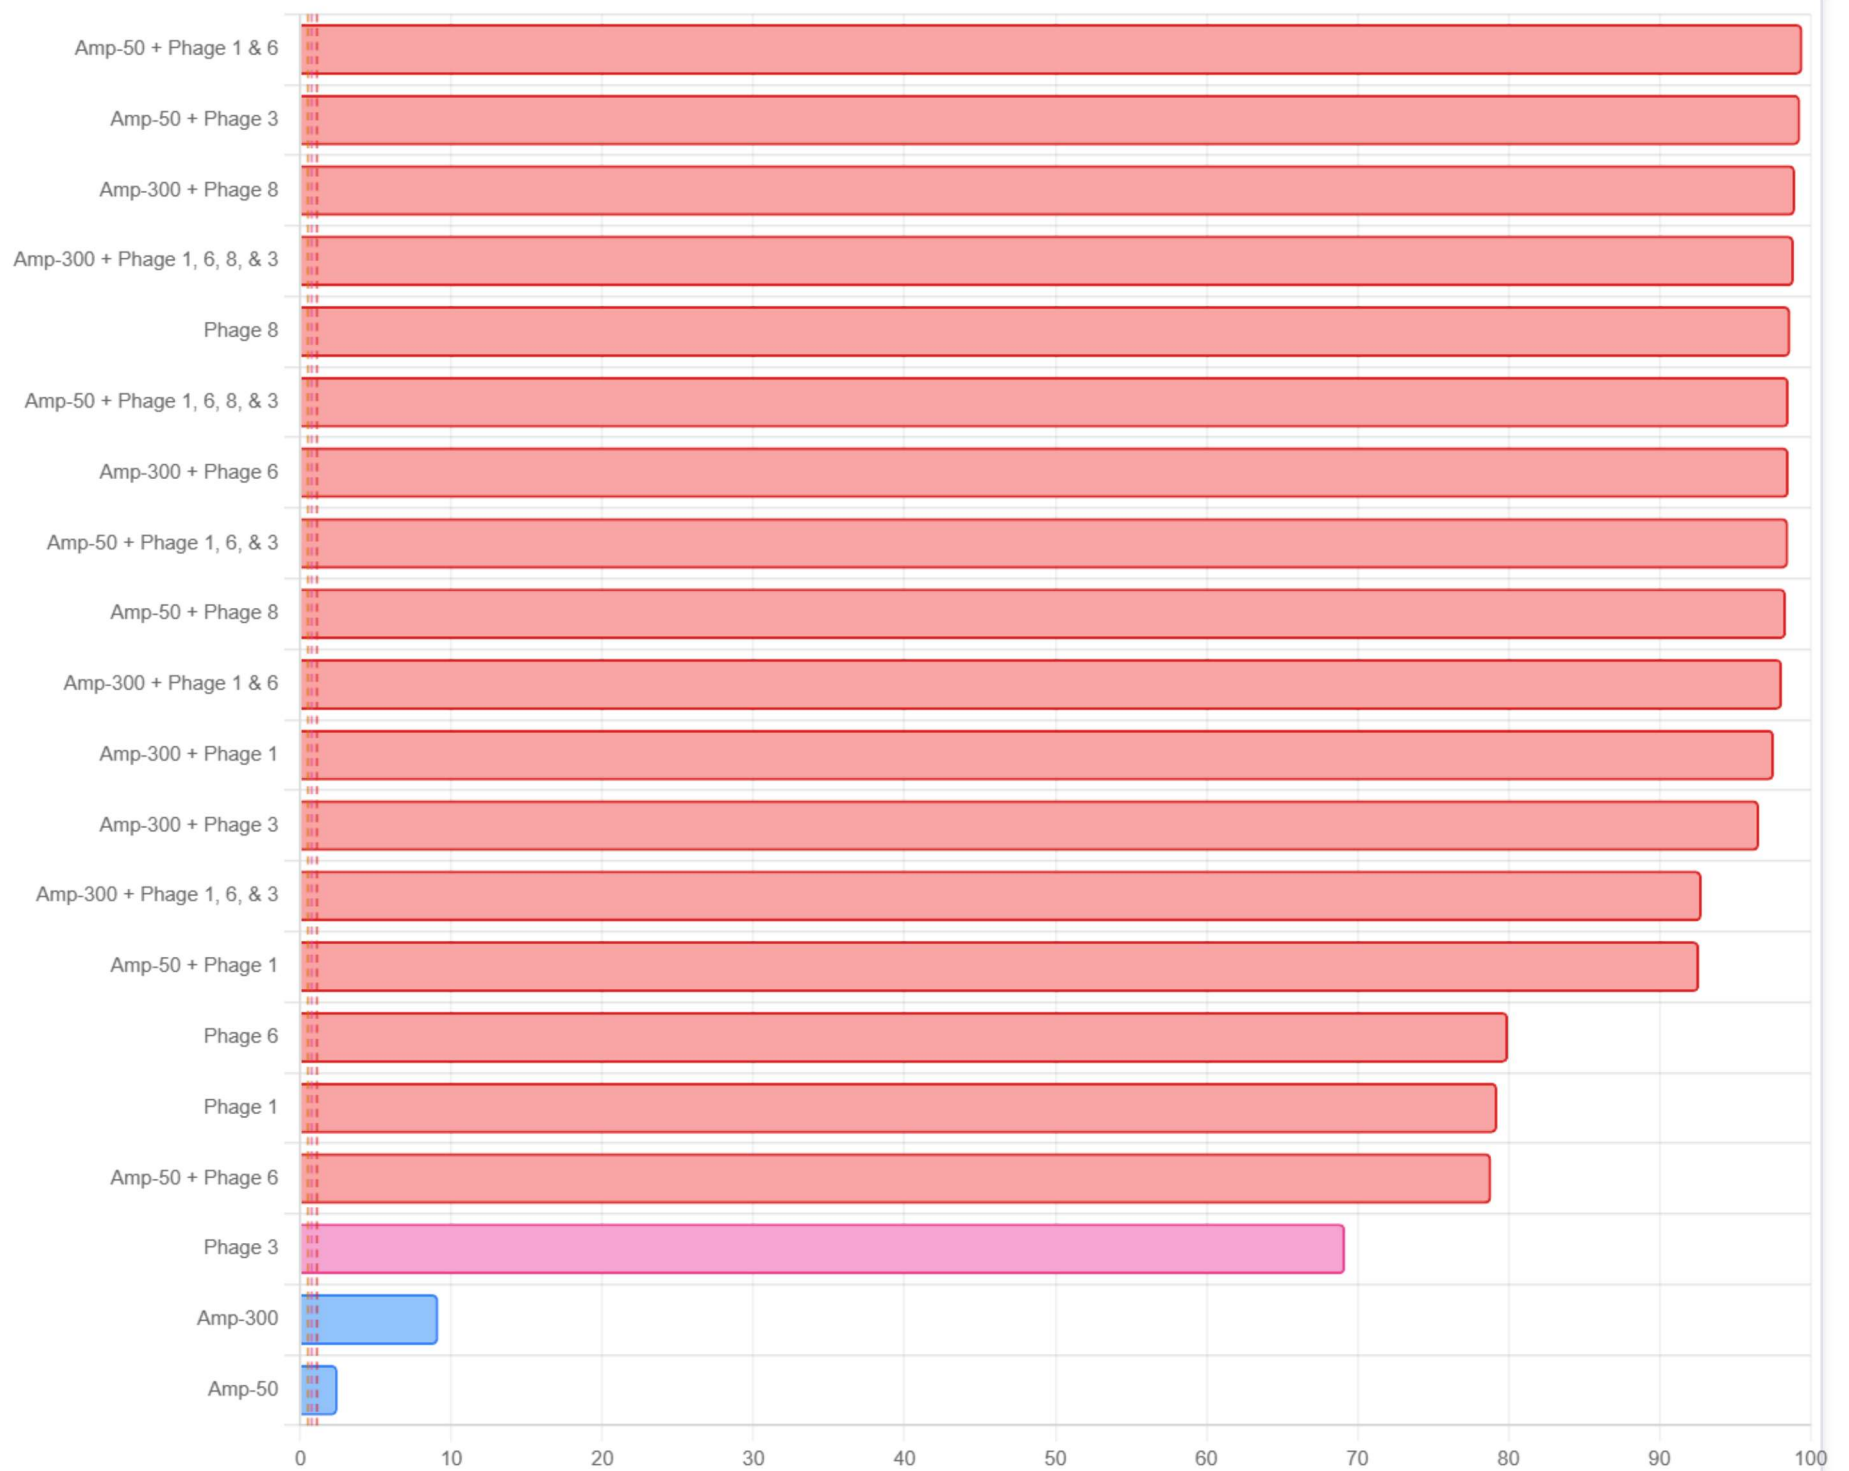

Detailed results table

↓ CSV ↓ PNG

STRAIN/CONDITION / ID	TYPE	MEDIA	N	MEAN OD570	BLANK OD570	% INHIBITION	CLASSIFICATION
Amp-300 + Phage 1, 6, & 3 E10, E11, E12	Strain/Condition	Default	3	0.205 (±0.097)	0.115	92.8%	Strong inhibition
Amp-50 + Phage 1 B10, B11, B12	Strain/Condition	Default	3	0.207 (±0.044)	0.115	92.6%	Strong inhibition
Phage 6 A7, A8, A9	Strain/Condition	Default	3	0.365 (±0.045)	0.115	80.0%	Strong inhibition
Phage 1 A4, A5, A6	Strain/Condition	Default	3	0.374 (±0.057)	0.115	79.3%	Strong inhibition
Amp-50 + Phage 6 C1, C2, C3	Strain/Condition	Default	3	0.378 (±0.127)	0.115	78.9%	Strong inhibition
Phage 3 B1, B2, B3	Strain/Condition	Default	3	0.499 (±0.062)	0.115	69.2%	Moderate inhibition
Amp-300 B7, B8, B9	Strain/Condition	Default	3	1.248 (±0.037)	0.115	9.1%	No/low inhibition
Amp-50 B4, B5, B6	Strain/Condition	Default	3	1.331 (±0.018)	0.115	2.5%	No/low inhibition

Plate heatmap — % Inhibition classification

↓ PNG

1 2 3 4 5 6 7 8 9 10 11 12

A	A1 K. pneumon...	A2 K. pneumon...	A3 K. pneumon...	A4 Phage 1 79.3%	A5 Phage 1 79.3%	A6 Phage 1 79.3%	A7 Phage 6 80.0%	A8 Phage 6 80.0%	A9 Phage 6 80.0%	A10 Phage 8 98.7%	A11 Phage 8 98.7%	A12 Phage 8 98.7%
B	B1 Phage 3 69.2%	B2 Phage 3 69.2%	B3 Phage 3 69.2%	B4 Amp-50 2.5%	B5 Amp-50 2.5%	B6 Amp-50 2.5%	B7 Amp-300 9.1%	B8 Amp-300 9.1%	B9 Amp-300 9.1%	B10 Amp-50 + P... 92.6%	B11 Amp-50 + P... 92.6%	B12 Amp-50 + P... 92.6%
C	C1 Amp-50 + P... 78.9%	C2 Amp-50 + P... 78.9%	C3 Amp-50 + P... 78.9%	C4 Amp-50 + P... 98.4%	C5 Amp-50 + P... 98.4%	C6 Amp-50 + P... 98.4%	C7 Amp-50 + P... 99.3%	C8 Amp-50 + P... 99.3%	C9 Amp-50 + P... 99.3%	C10 Amp-300 + ... 97.6%	C11 Amp-300 + ... 97.6%	C12 Amp-300 + ... 97.6%
D	D1 Amp-300 + ... 98.6%	D2 Amp-300 + ... 98.6%	D3 Amp-300 + ... 98.6%	D4 Amp-300 + ... 99.0%	D5 Amp-300 + ... 99.0%	D6 Amp-300 + ... 99.0%	D7 Amp-300 + ... 96.6%	D8 Amp-300 + ... 96.6%	D9 Amp-300 + ... 96.6%	D10 Amp-50 + P... 99.5%	D11 Amp-50 + P... 99.5%	D12 Amp-50 + P... 99.5%
E	E1 Amp-50 + P... 98.5%	E2 Amp-50 + P... 98.5%	E3 Amp-50 + P... 98.5%	E4 Amp-50 + P... 98.6%	E5 Amp-50 + P... 98.6%	E6 Amp-50 + P... 98.6%	E7 Amp-300 + ... 98.1%	E8 Amp-300 + ... 98.1%	E9 Amp-300 + ... 98.1%	E10 Amp-300 + ... 92.8%	E11 Amp-300 + ... 92.8%	E12 Amp-300 + ... 92.8%
F	F1 Amp-300 + ... 98.9%	F2 Amp-300 + ... 98.9%	F3 Amp-300 + ... 98.9%	F4 blank 0.116	F5 blank 0.111	F6 blank 0.118	F7	F8	F9	F10	F11	F12
G	G1	G2	G3	G4	G5	G6	G7	G8	G9	G10	G11	G12
H	H1	H2	H3	H4	H5	H6	H7	H8	H9	H10	H11	H12

☐ Blank / empty
 ☐ No/low inhib.
 ☐ Weak inhib.
 ☐ Moderate inhib.
 ☐ Strong inhib.
 ☐ Positive ctrl
 ☐ Negative ctrl

[← Back](#)
[↺ New experiment](#)