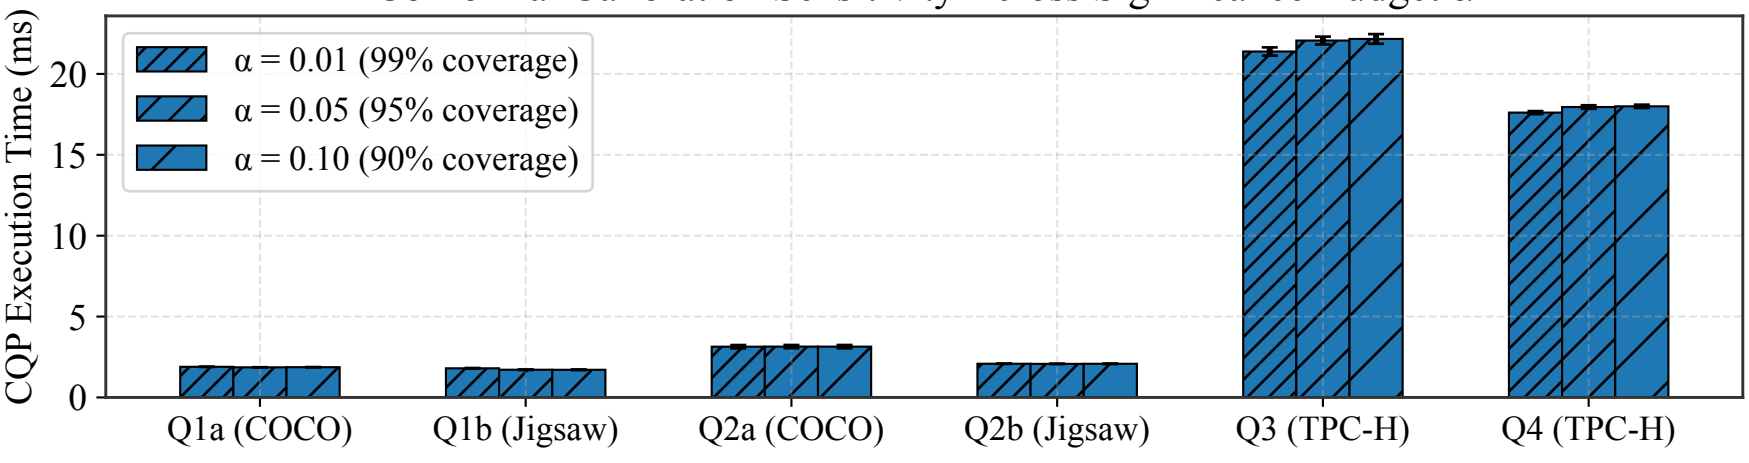
Conformal Calibration Sensitivity Across Significance Budget α
CQP Execution Time (ms)
0
5
10
15
20
α = 0.01 (99% coverage)
α = 0.05 (95% coverage)
α = 0.10 (90% coverage)
Q1a (COCO)
Q1b (Jigsaw)
Q2a (COCO)
Q2b (Jigsaw)
Q3 (TPC-H)
Q4 (TPC-H)