Data File F:\HPLC_Projects\Projects\Data\SHIBU 2024-11-06 15-15-45\010-P1-A10-9.D
Sample Name: 9

```
==================================================================
Acq. Operator   : SYSTEM                    Seq. Line :  10
Sample Operator : SYSTEM
Acq. Instrument : HPLC                       Location :   P1-A-10
Injection Date  : 06-11-2024 17:42:37          Inj :    1
                                         Inj Volume : 5.000 µl
Sequence File   : F:\HPLC_Projects\Projects\Data\SHIBU 2024-11-06 15-15-45\SHIBU.S
Method          : F:\HPLC_Projects\Projects\Data\SHIBU 2024-11-06 15-15-45\SHIBU 6-11-24.M (
                  Sequence Method)
Last changed    : 06-11-2024 15:13:29 by SYSTEM
```
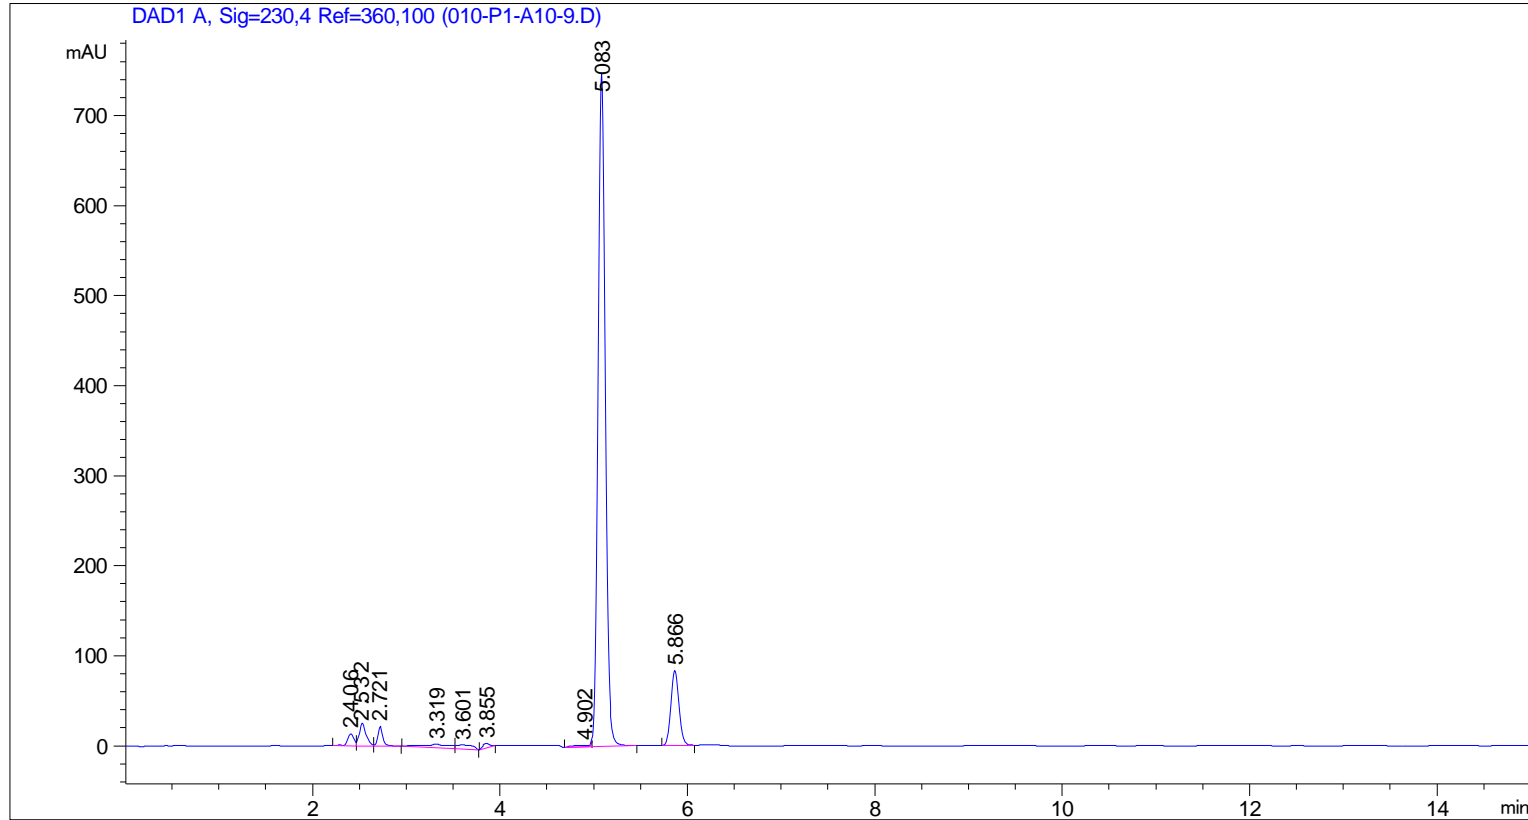

DAD1 A, Sig=230,4 Ref=360,100 (010-P1-A10-9.D)

```
==================================================================
                      Area Percent Report
==================================================================
```

```
Sorted By          :       Signal
Multiplier         :       1.0000
Dilution           :       1.0000
Use Multiplier & Dilution Factor with ISTDs
```

Signal 1: DAD1 A, Sig=230,4 Ref=360,100

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	2.406	VV R	0.0766	63.23073	13.03651	1.2997
2	2.532	VV	0.0687	118.72138	25.33381	2.4404
3	2.721	VB	0.0592	84.07114	21.70911	1.7281
4	3.319	BV	0.2188	72.46712	4.16985	1.4896
5	3.601	VB	0.1498	54.00230	4.70800	1.1100
6	3.855	BB	0.0808	25.89617	5.13633	0.5323
7	4.902	BV E	0.1633	23.76090	1.90777	0.4884
8	5.083	VB R	0.0815	4639.89868	747.52551	80.9861

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
9	5.866	BB	0.0897	482.85638	83.16213	9.9253

Totals :   5568.90482 906.68901

===
                        *** End of Report ***