Data File F:\HPLC_Projects\Projects\Data\SHIBU 2024-11-06 15-15-45\014-P1-B3-13.D
Sample Name: 13

```
================================================================
Acq. Operator   : SYSTEM                    Seq. Line :  14
Sample Operator : SYSTEM
Acq. Instrument : HPLC                       Location :   P1-B-03
Injection Date  : 06-11-2024 18:47:18          Inj :    1
                                         Inj Volume : 5.000 µl
Sequence File   : F:\HPLC_Projects\Projects\Data\SHIBU 2024-11-06 15-15-45\SHIBU.S
Method          : F:\HPLC_Projects\Projects\Data\SHIBU 2024-11-06 15-15-45\SHIBU 6-11-24.M (
                  Sequence Method)
Last changed    : 06-11-2024 15:13:29 by SYSTEM
```
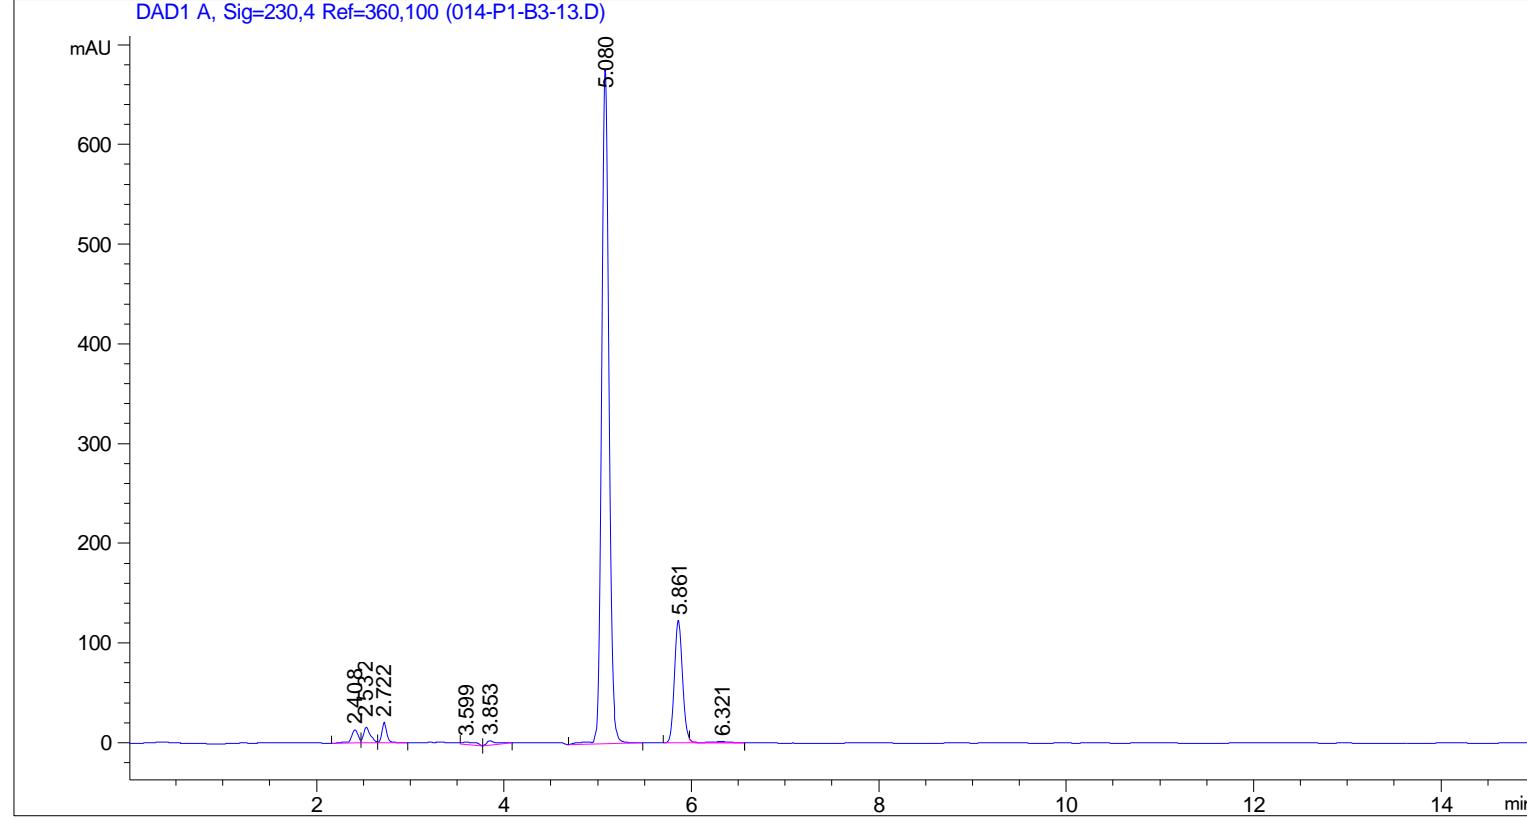


```
================================================================
                    Area Percent Report
================================================================
```

```
Sorted By          :       Signal
Multiplier         :       1.0000
Dilution           :       1.0000
Use Multiplier & Dilution Factor with ISTDs
```

Signal 1: DAD1 A, Sig=230,4 Ref=360,100

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	2.408	VV R	0.0791	66.58421	13.15145	1.4408
2	2.532	VV	0.0721	78.80859	15.82377	1.7054
3	2.722	VB	0.0592	80.92266	20.89067	1.7511
4	3.599	VB	0.1348	27.89024	2.69281	0.6035
5	3.853	BB	0.1073	30.25806	4.13876	0.6548
6	5.080	BB	0.0820	4600.97339	677.66248	77.9230
7	5.861	BV R	0.0921	717.90497	122.93662	15.5351
8	6.321	VB E	0.1843	17.85217	1.26728	0.3863

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
Totals :				5621.19428	858.56383	

==
*** End of Report ***