Data File F:\HPLC_Projects\Projects\Data\SHIBU 2024-11-06 15-15-45\015-P1-B4-14.D
Sample Name: 14

```
=====================================================================
Acq. Operator   : SYSTEM                        Seq. Line :   15
Sample Operator : SYSTEM
Acq. Instrument : HPLC                           Location :   P1-B-04
Injection Date  : 06-11-2024 19:03:29                Inj :   1
                                             Inj Volume : 5.000 µl
Sequence File   : F:\HPLC_Projects\Projects\Data\SHIBU 2024-11-06 15-15-45\SHIBU.S
Method          : F:\HPLC_Projects\Projects\Data\SHIBU 2024-11-06 15-15-45\SHIBU 6-11-24.M (
                  Sequence Method)
Last changed    : 06-11-2024 15:13:29 by SYSTEM
```
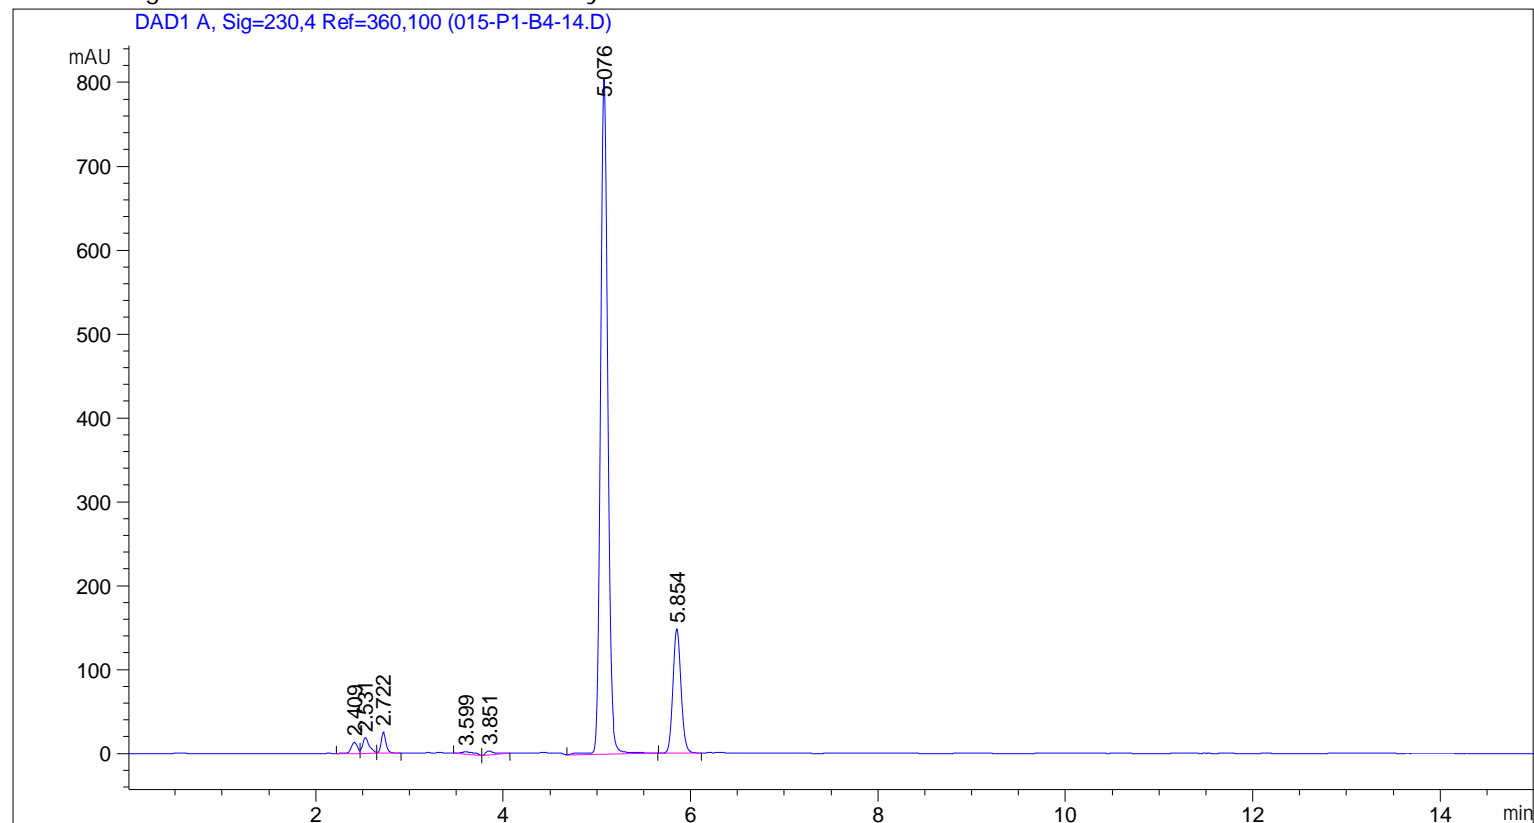


```
=====================================================================
                        Area Percent Report
=====================================================================
```

```
Sorted By           :        Signal
Multiplier          :        1.0000
Dilution            :        1.0000
Use Multiplier & Dilution Factor with ISTDs
```

Signal 1: DAD1 A, Sig=230,4 Ref=360,100

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	2.409	VV R	0.0741	63.74567	13.26242	1.1661
2	2.531	VV	0.0703	91.70961	18.99722	1.6777
3	2.722	VB	0.0582	97.25664	25.64586	1.7792
4	3.599	BB	0.1366	27.35208	2.64509	0.5004
5	3.851	BB	0.0983	31.06136	4.62789	0.5682
6	5.076	BB	0.0842	4287.65967	804.76843	78.4363
7	5.854	BB	0.0902	867.63593	148.35283	15.8721

```
Totals :                 5466.42095 1018.29974
```

==

*** End of Report ***