


Sample Name: 11

```
=====
Acq. Operator   : SYSTEM                      Seq. Line :   12
Sample Operator : SYSTEM
Acq. Instrument : HPLC                      Location  : P1-B-01
Injection Date  : 06-11-2024 18:15:00        Inj       :    1
                                           Inj Volume: 5.000 µl
Method          : F:\HPLC_Projects\Projects\Data\SHIBU 2024-11-06 15-15-45\SHIBU 6-11-24.M (
                  Sequence Method)
Last changed    : 06-11-2024 15:13:29 by SYSTEM
=====
```

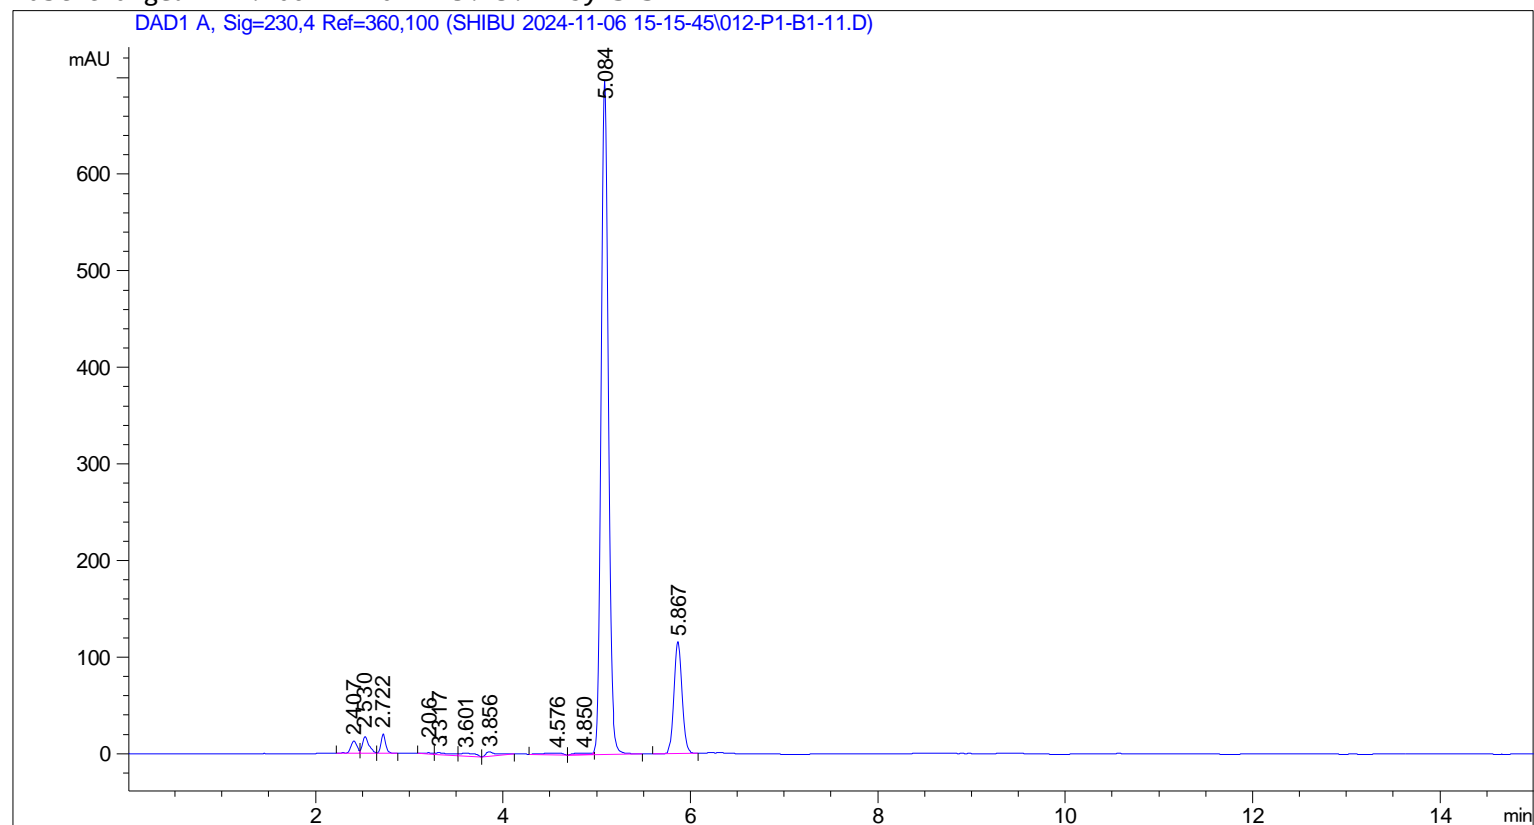

```
=====
                        Area Percent Report
=====
```

```
Sorted By      : Signal
Multiplier     : 1.0000
Dilution       : 1.0000
Use Multiplier & Dilution Factor with ISTDs
```

Signal 1: DAD1 A, Sig=230,4 Ref=360,100

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	2.407	VV R	0.0750	59.74181	12.66384	1.2659
2	2.530	VV	0.0696	83.04310	17.41568	1.7596
3	2.722	VB	0.0570	75.39556	20.47352	1.5975
4	3.206	BV	0.0970	7.46411	1.07508	0.1582
5	3.317	VV	0.1561	21.56291	1.76996	0.4569
6	3.601	VB	0.1392	32.76907	3.10367	0.6943
7	3.856	BB	0.1119	35.34558	4.48789	0.7489
8	4.576	BB	0.2113	22.03384	1.50032	0.4669
9	4.850	BV E	0.1664	21.66650	1.70345	0.4591

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
10	5.084	VB R	0.0836	4684.42285	697.64502	78.0684
11	5.867	BB	0.0899	676.03418	116.08817	14.3243

Totals : 5719.47952 877.92659

*** End of Report ***