```
=====================================================================
Acq. Operator   : SYSTEM                        Seq. Line :   1
Sample Operator : SYSTEM
Acq. Instrument : HPLC                           Location :   P1-A-01
Injection Date  : 06-11-2024 15:16:58               Inj :   1
                                             Inj Volume : 5.000 µl
Sequence File   : F:\HPLC_Projects\Projects\Data\SHIBU 2024-11-06 15-15-45\SHIBU.S
Method          : F:\HPLC_Projects\Projects\Data\SHIBU 2024-11-06 15-15-45\SHIBU 6-11-24.M (
                  Sequence Method)
Last changed    : 06-11-2024 15:13:29 by SYSTEM
```
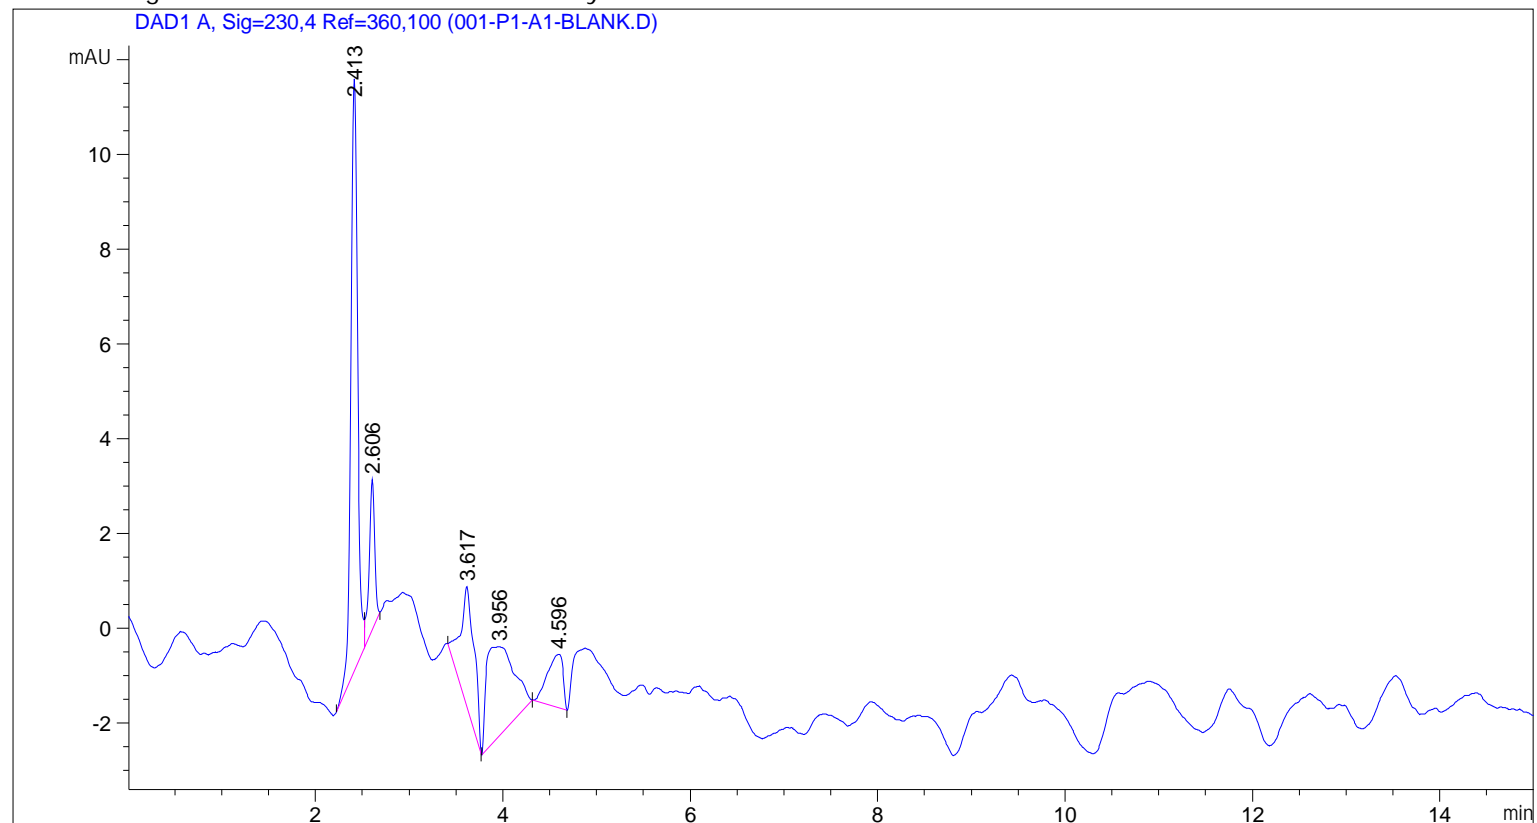

DAD1 A, Sig=230,4 Ref=360,100 (001-P1-A1-BLANK.D)

```
=====================================================================
                    Area Percent Report
=====================================================================
```

```
Sorted By            :        Signal
Multiplier           :        1.0000
Dilution             :        1.0000
Use Multiplier & Dilution Factor with ISTDs
```

Signal 1: DAD1 A, Sig=230,4 Ref=360,100

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	2.413	BV	0.0766	62.76912	12.50059	40.9983
2	2.606	VB	0.0613	12.81307	3.16106	8.3690
3	3.617	BB	0.1350	25.94261	2.54242	16.9447
4	3.956	BB	0.2465	38.70786	1.89372	25.2825
5	4.596	BB	0.1732	12.86898	1.12727	8.4055

```
Totals :                        153.10164   21.22507
```

Data File F:\HPLC_Projects\Projects\Data\SHIBU 2024-11-06 15-15-45\001-P1-A1-BLANK.D
Sample Name: BLANK

```
=====================================================================
                         *** End of Report ***
```

```
                         *** End of Report ***
```