```
========================================================================
Acq. Operator   : SYSTEM                       Seq. Line :   6
Sample Operator : SYSTEM
Acq. Instrument : HPLC                          Location :   P1-A-05
Injection Date  : 05-11-2024 15:16:14              Inj :   1
                                              Inj Volume : 5.000 µl
Sequence File   : F:\HPLC_Projects\Projects\Data\SHIBU SEQUENCE  2024-11-05 13-54-07\SHIBU
                  SEQUENCE .S
Method          : F:\HPLC_Projects\Projects\Data\SHIBU SEQUENCE  2024-11-05 13-54-07\SHIBU 5-
                  11-24.M (Sequence Method)
Last changed    : 05-11-2024 13:46:40 by SYSTEM
```
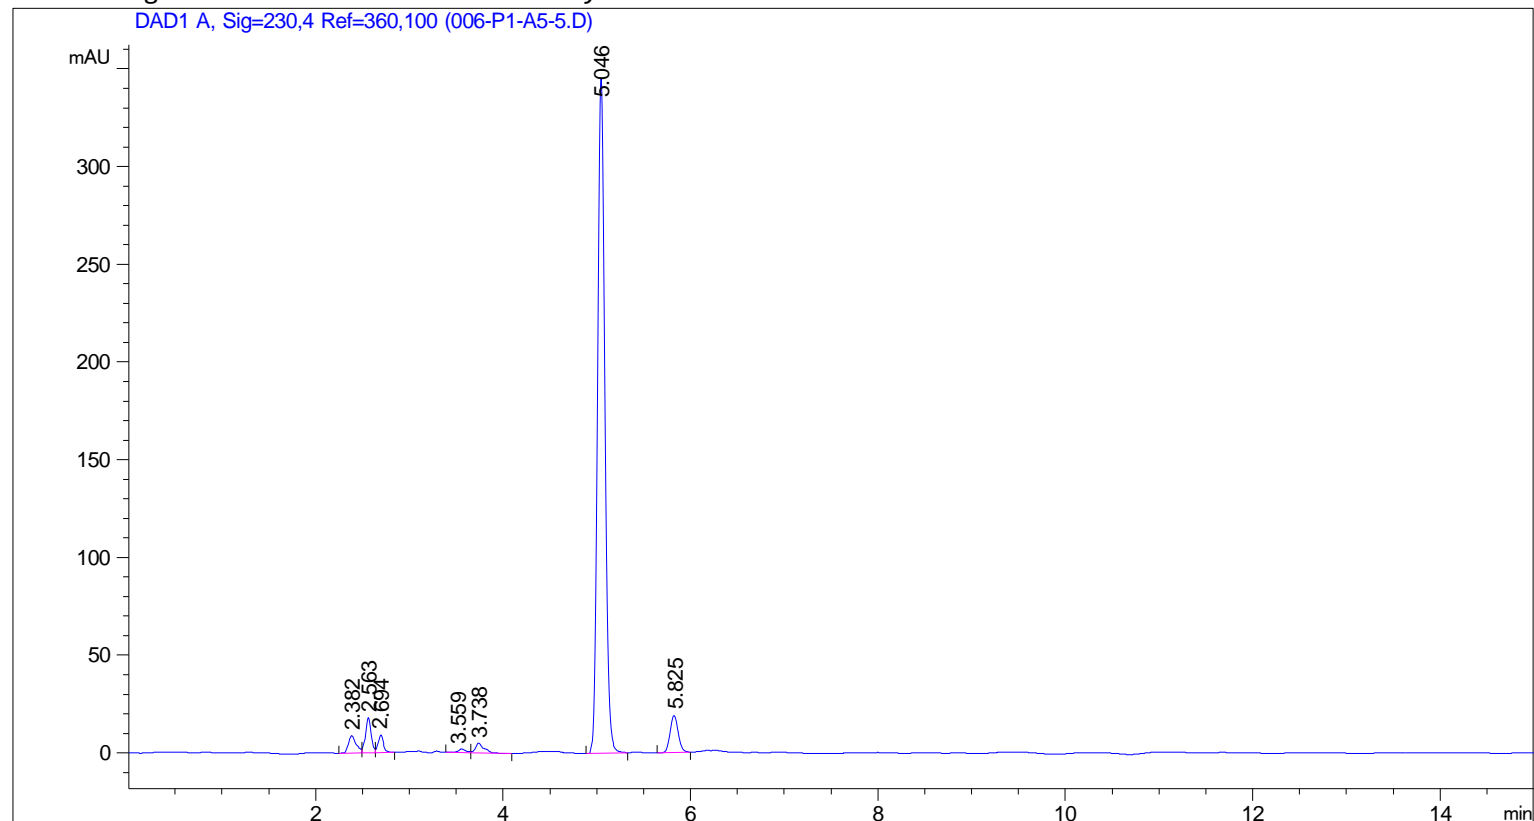


```
========================================================================
                        Area Percent Report
========================================================================


Sorted By          :      Signal
Multiplier         :      1.0000
Dilution           :      1.0000
Use Multiplier & Dilution Factor with ISTDs



Signal 1: DAD1 A, Sig=230,4 Ref=360,100
```

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	2.382	BV	0.0812	49.57729	8.87690	2.3331
2	2.563	VV	0.0599	70.89616	18.03724	3.3363
3	2.694	VB	0.0588	34.55378	8.99891	1.6261
4	3.559	BV	0.0866	11.96624	1.97840	0.5631
5	3.738	VB	0.0890	32.54956	5.06585	1.5318
6	5.046	BB	0.0811	2316.33081	346.83475	85.4755
7	5.825	BB	0.0892	109.09791	18.94500	5.1341

Data File F:\HPLC_Projects\Projects\Data\SHIBU SEQUENCE 2024-11-05 13-54-07\006-P1-A5-5.D
Sample Name: 5

```
Peak RetTime Type  Width     Area       Height     Area
  #   [min]        [min]   [mAU*s]      [mAU]        %
----|-------|----|-------|----------|----------| -------- |
Totals :                  2624.97176  408.73704
```

===
                          *** End of Report ***