```
========================================================================
Acq. Operator   : SYSTEM                    Seq. Line :   3
Sample Operator : SYSTEM
Acq. Instrument : HPLC                       Location :   P1-A-03
Injection Date  : 06-11-2024 15:49:41            Inj :   1
                                          Inj Volume : 5.000 µl
Sequence File   : F:\HPLC_Projects\Projects\Data\SHIBU 2024-11-06 15-15-45\SHIBU.S
Method          : F:\HPLC_Projects\Projects\Data\SHIBU 2024-11-06 15-15-45\SHIBU 6-11-24.M (
                  Sequence Method)
Last changed    : 06-11-2024 15:13:29 by SYSTEM
```
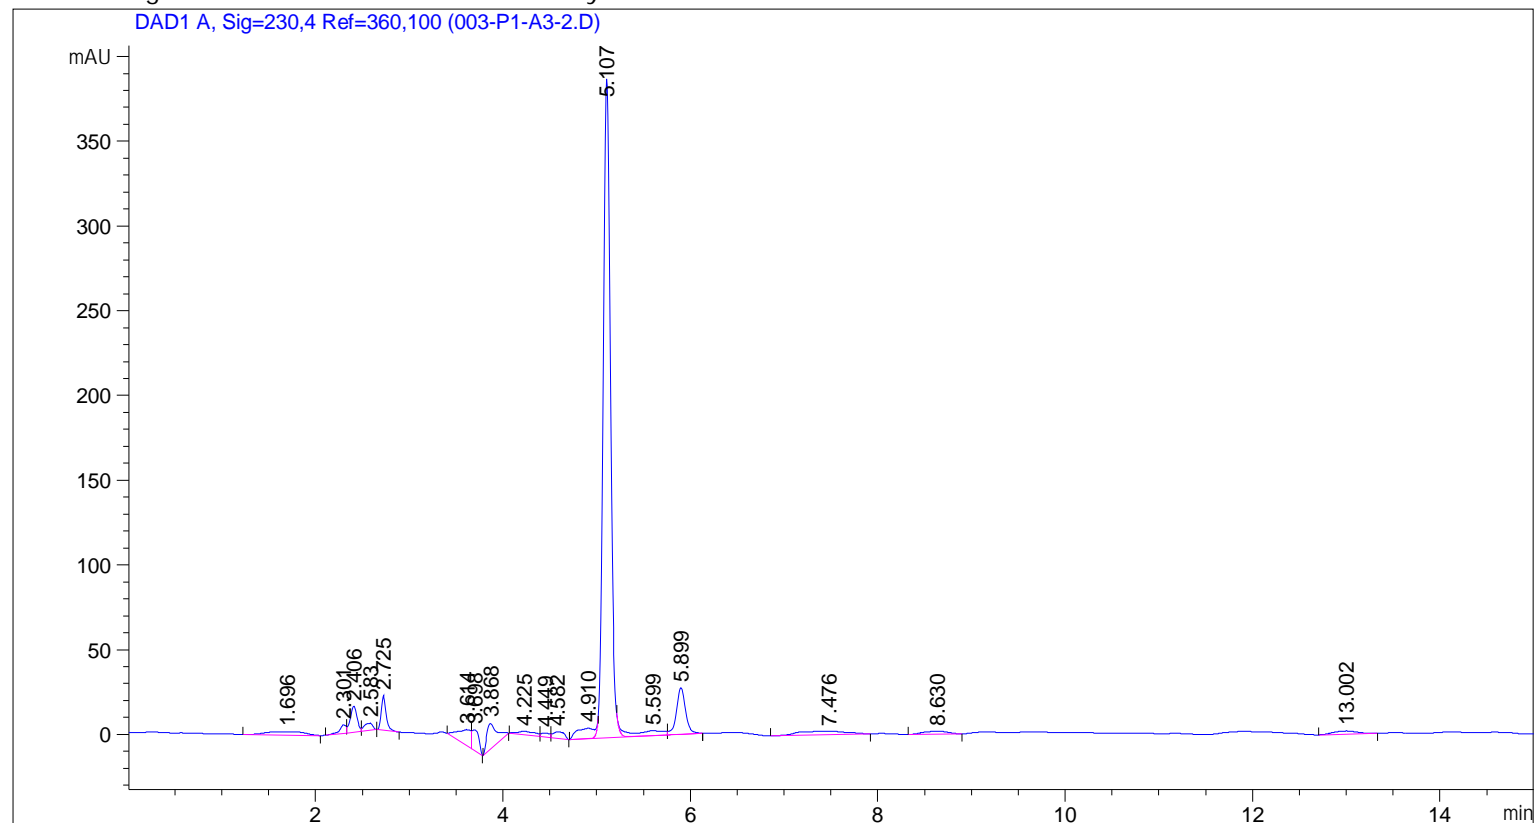


```
========================================================================
                        Area Percent Report
========================================================================
```

Sorted By   :   Signal
Multiplier   :   1.0000
Dilution   :   1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: DAD1 A, Sig=230,4 Ref=360,100

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	1.696	BB	0.3376	55.51863	1.97739	1.7540
2	2.301	BV	0.0665	23.37099	4.99867	0.7384
3	2.406	VV	0.0762	76.68607	15.37054	2.4228
4	2.583	VB	0.0875	26.58469	4.22001	0.8399
5	2.725	BB	0.0594	79.75568	20.49316	2.5197
6	3.614	BV	0.1214	85.63894	9.30224	2.7056
7	3.698	VB	0.0816	61.32646	12.01170	1.9375
8	3.868	BB	0.1103	111.10152	15.02420	3.5101

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
9	4.225	BV	0.1712	26.88610	2.07401	0.8494
10	4.449	VV	0.0904	15.06635	2.42686	0.4760
11	4.582	VB	0.1396	34.55378	3.96608	1.0917
12	4.910	BV E	0.1778	82.61153	6.26859	2.6100
13	5.107	VV R	0.0826	2089.21851	389.14438	66.0053
14	5.599	VV E	0.3108	73.90047	2.98509	2.3348
15	5.899	VB E	0.0995	182.46877	27.48252	5.7648
16	7.476	BB	0.4386	75.60491	2.10707	2.3886
17	8.630	BB	0.2239	31.07112	1.72736	0.9816
18	13.002	BB	0.2579	33.86528	1.90041	1.0699

Totals :   3165.22980   523.48028

===
*** End of Report ***