```
=====================================================================
Acq. Operator   : SYSTEM                    Seq. Line :    7
Sample Operator : SYSTEM
Acq. Instrument : HPLC                       Location :   P1-A-07
Injection Date  : 06-11-2024 16:54:14           Inj :    1
                                          Inj Volume : 5.000 µl
Sequence File   : F:\HPLC_Projects\Projects\Data\SHIBU 2024-11-06 15-15-45\SHIBU.S
Method          : F:\HPLC_Projects\Projects\Data\SHIBU 2024-11-06 15-15-45\SHIBU 6-11-24.M (
                  Sequence Method)
Last changed    : 06-11-2024 15:13:29 by SYSTEM
```
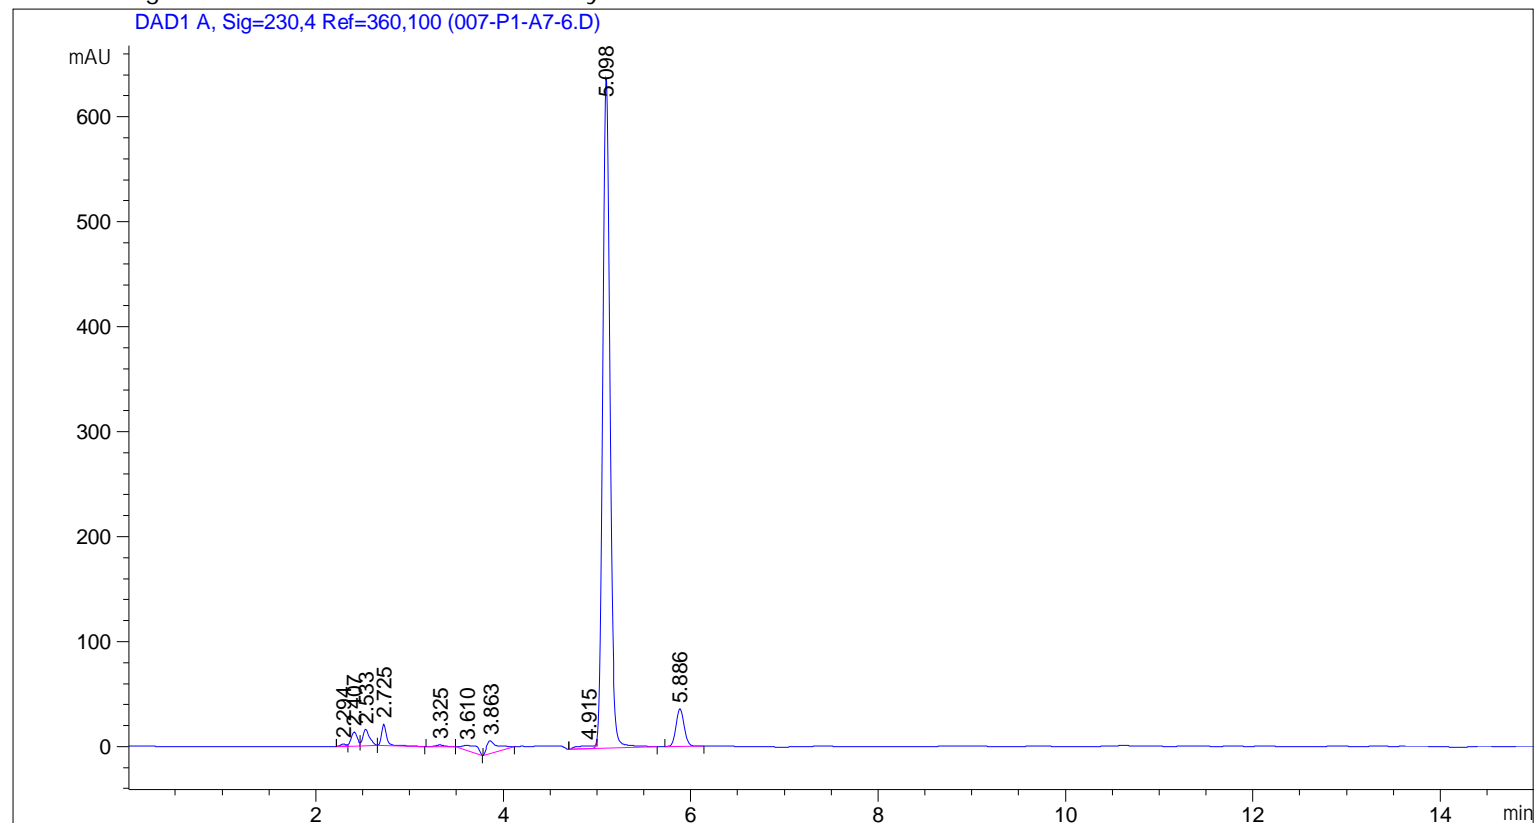

DAD1 A, Sig=230,4 Ref=360,100 (007-P1-A7-6.D)

```
=====================================================================
                       Area Percent Report
=====================================================================
```

```
Sorted By            :        Signal
Multiplier           :        1.0000
Dilution             :        1.0000
Use Multiplier & Dilution Factor with ISTDs
```

Signal 1: DAD1 A, Sig=230,4 Ref=360,100

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	2.294	BV E	0.0536	6.65091	1.96019	0.1636
2	2.407	VV R	0.0726	61.15491	13.06609	1.5044
3	2.533	VB	0.0692	74.17412	15.67525	1.8246
4	2.725	BV R	0.0610	83.30956	20.66789	2.0494
5	3.325	BB	0.0809	8.92334	1.60364	0.2195
6	3.610	BB	0.1729	64.73694	4.75410	1.5925
7	3.863	BB	0.1140	95.24526	11.82315	2.3430
8	4.915	BV E	0.1713	37.78677	2.91453	0.9295

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
9	5.098	VB R	0.0824	3420.81372	639.50690	84.1497
10	5.886	BB	0.0930	212.35892	35.88292	5.2239

Totals :   4065.15445   747.85465

===
*** End of Report ***