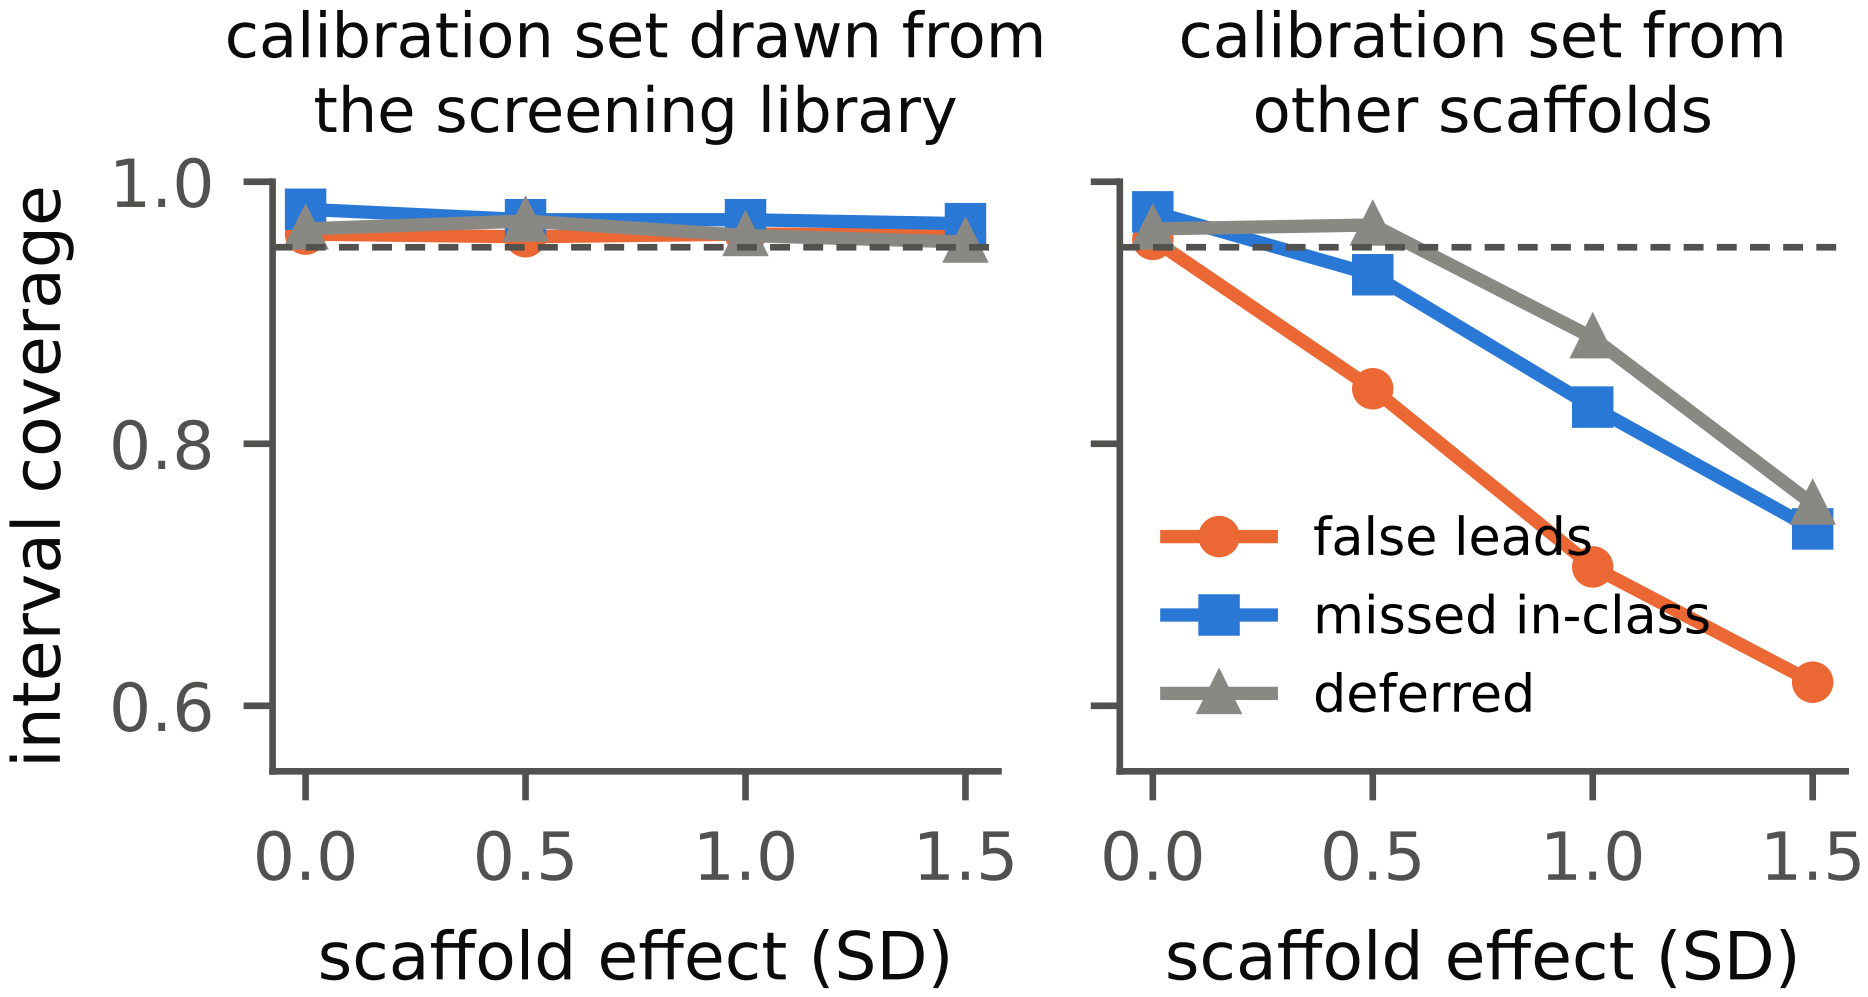
calibration set drawn from the screening library
calibration set from other scaffolds
interval coverage
1.0
0.8
0.6
0.0
0.5
1.0
1.5
scaffold effect (SD)
false leads
missed in-class
deferred