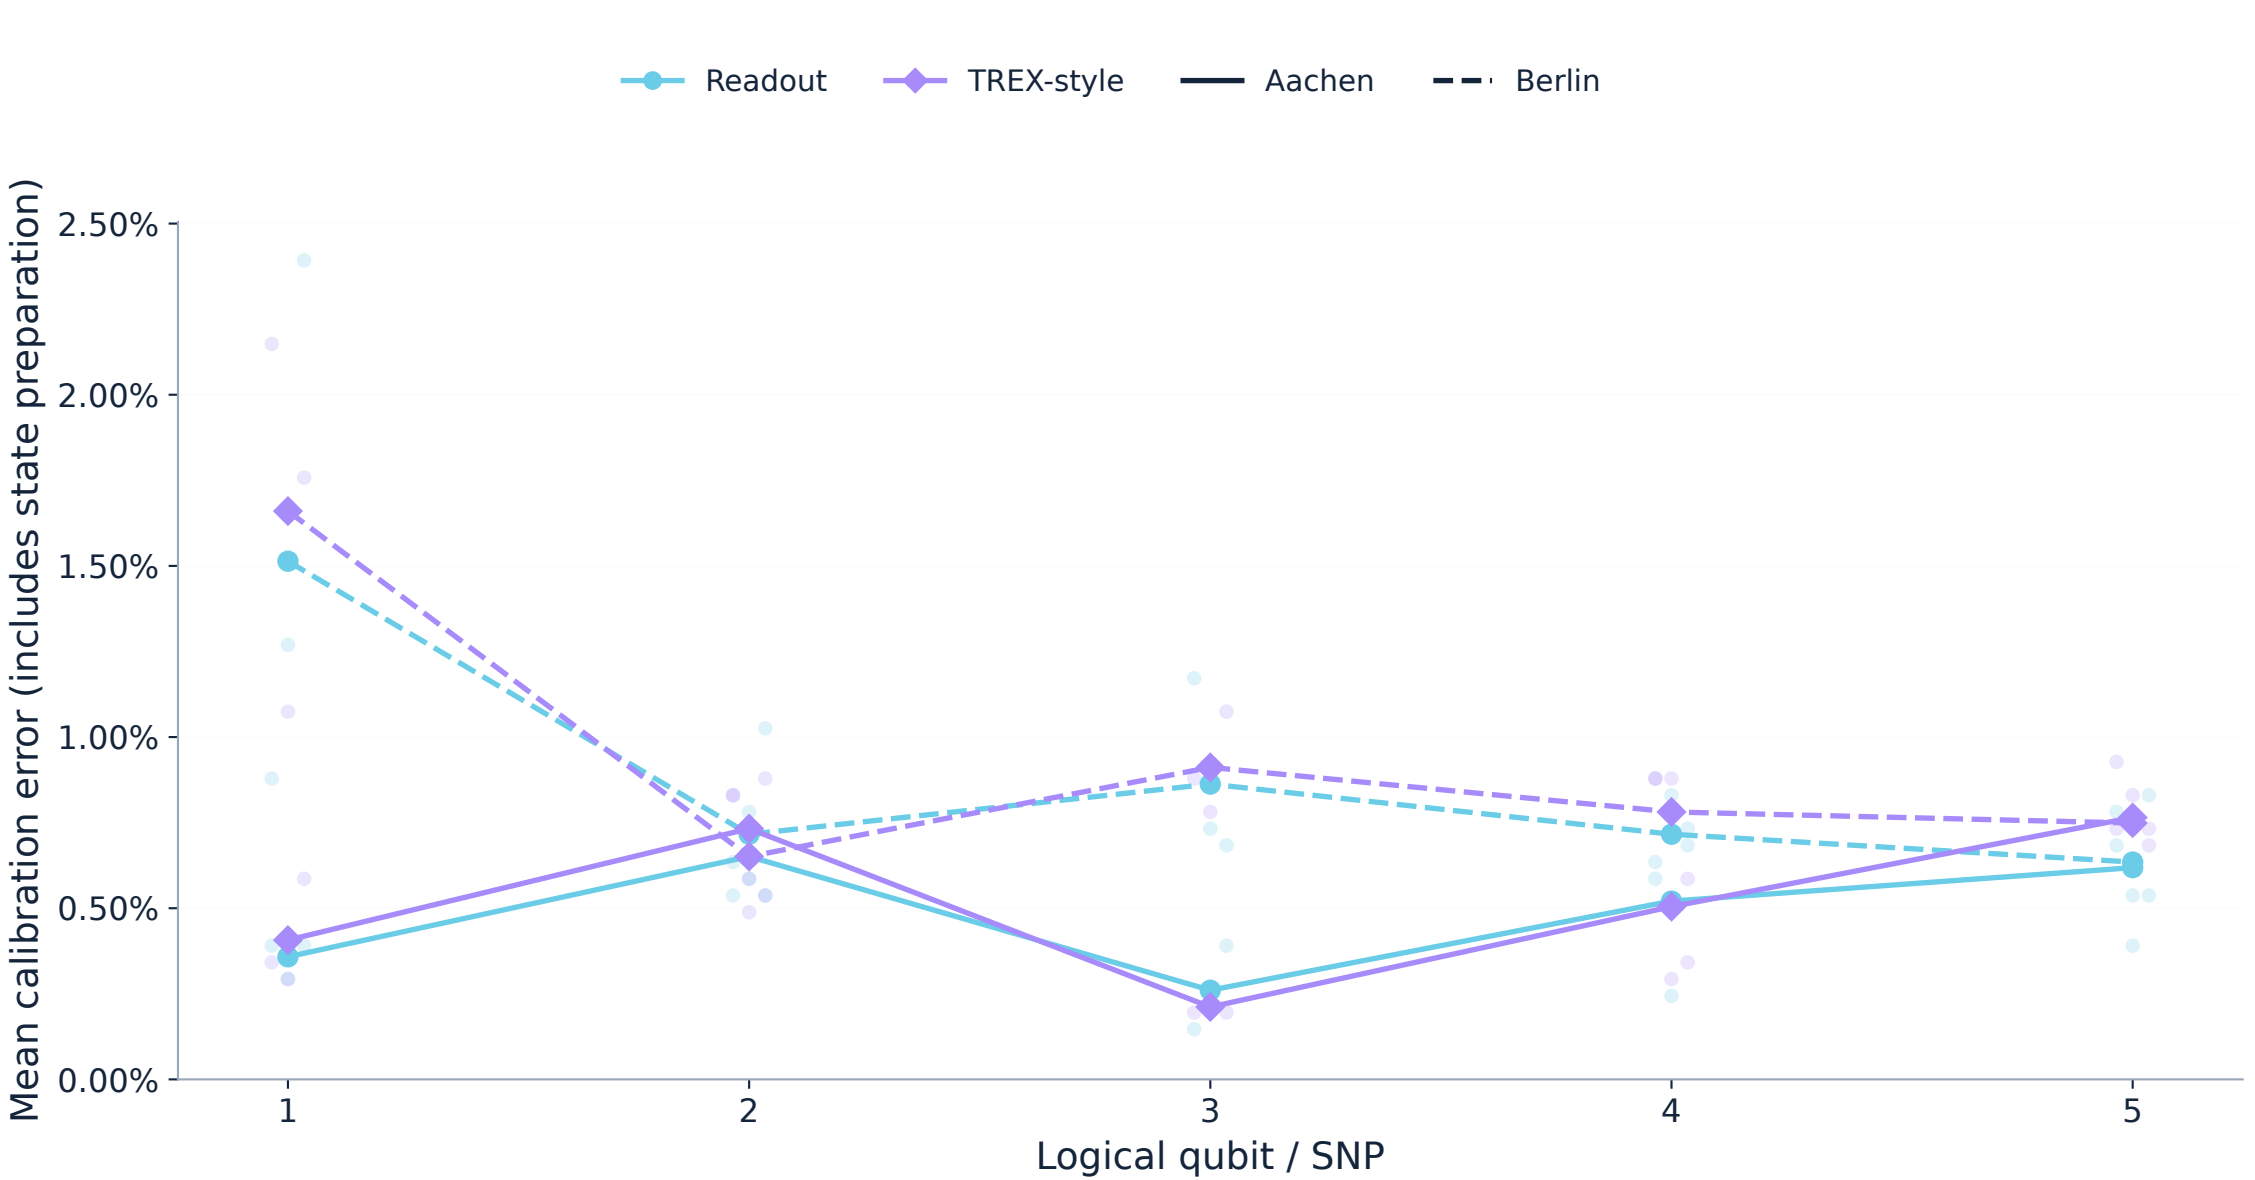
Hardware: readout calibration by qubit
Readout
TREX-style
Aachen
Berlin
Mean calibration error (includes state preparation)
2.50%
2.00%
1.50%
1.00%
0.50%
0.00%
1
2
3
4
5
Logical qubit / SNP