
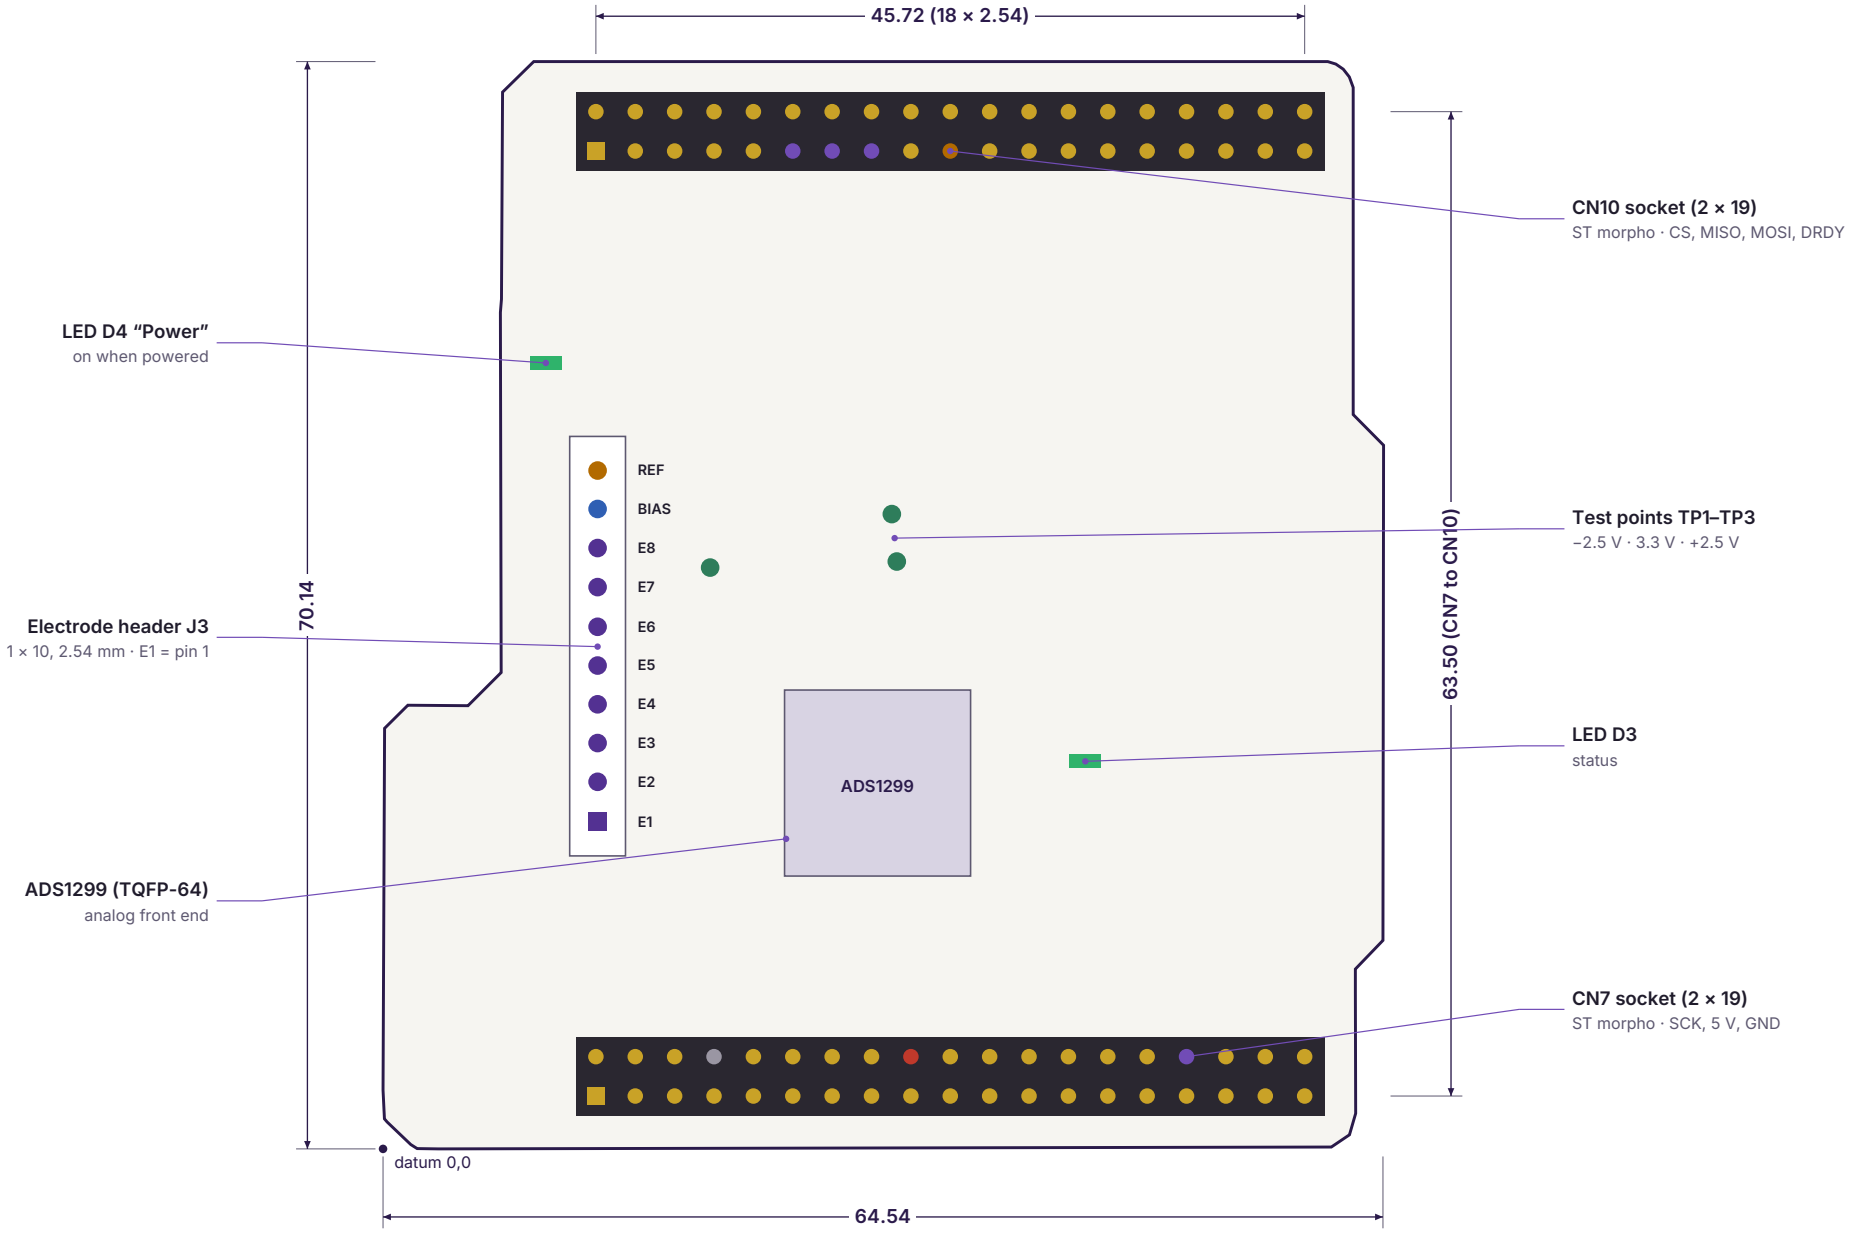



For research and education only. Not a medical device. Specifications subject to change.

02 INTERFACE LOCATIONS

Interface	Position from datum (mm)	Details
CN10 socket	X 13.73–59.45; Y 64.37 (odd) / 66.91 (even)	2 × 19, 2.54 mm onto ST morpho CN10; pin 1 square, left end, inner row
CN7 socket	X 13.73–59.45; Y 3.41 (odd) / 5.95 (even)	2 × 19, 2.54 mm onto ST morpho CN7; pin 1 square, left end, outer row
Electrode header J3	X 13.84; Y 21.10 (E1) … 43.76 (Ref)	1 × 10, 2.54 mm: E1…E8, Biasout, Ref; pin 1 = E1 (square pad)
Test points	TP1 (33.1, 37.9) · TP2 (21.1, 37.5) · TP3 (32.8, 41.0)	TP1 −2.5 V · TP2 3.3 V · TP3 +2.5 V (supply check)
LEDs	D4 (10.5, 50.7) · D3 (45.3, 25.0)	D4 “Power” · D3 status
Outline	64.54 × 70.14 mm	Contoured: side notches clear parts of the NUCLEO-WB55
Mounting	—	No holes; held by the two morpho sockets

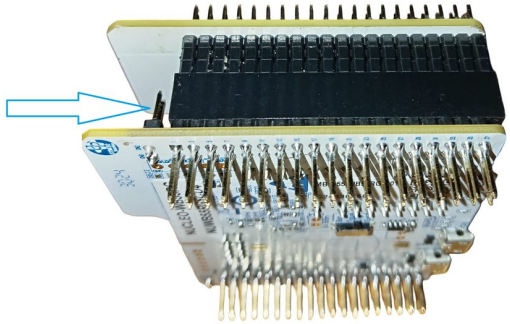

Alignment: match the end pin marked by the arrow.

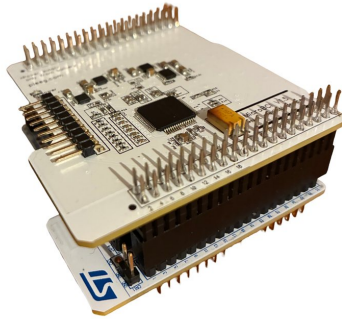

Mounted on the NUCLEO-WB55.

CAUTION Alignment.

A shield shifted by one pin will not read the ADS1299. Check the end pin against the photo every time, with the Nucleo unpowered.

Title	MicroBCI outline & interfaces
Doc. No.	MB-MD-002
Revision	Rev. A · 10 Nov 2026
Board	MicroBCI V1.0
Units	mm; datum lower-left of bounding box
Scale	2 : 1 (A4 print)

For research and education only. Not a medical device. Specifications subject to change.