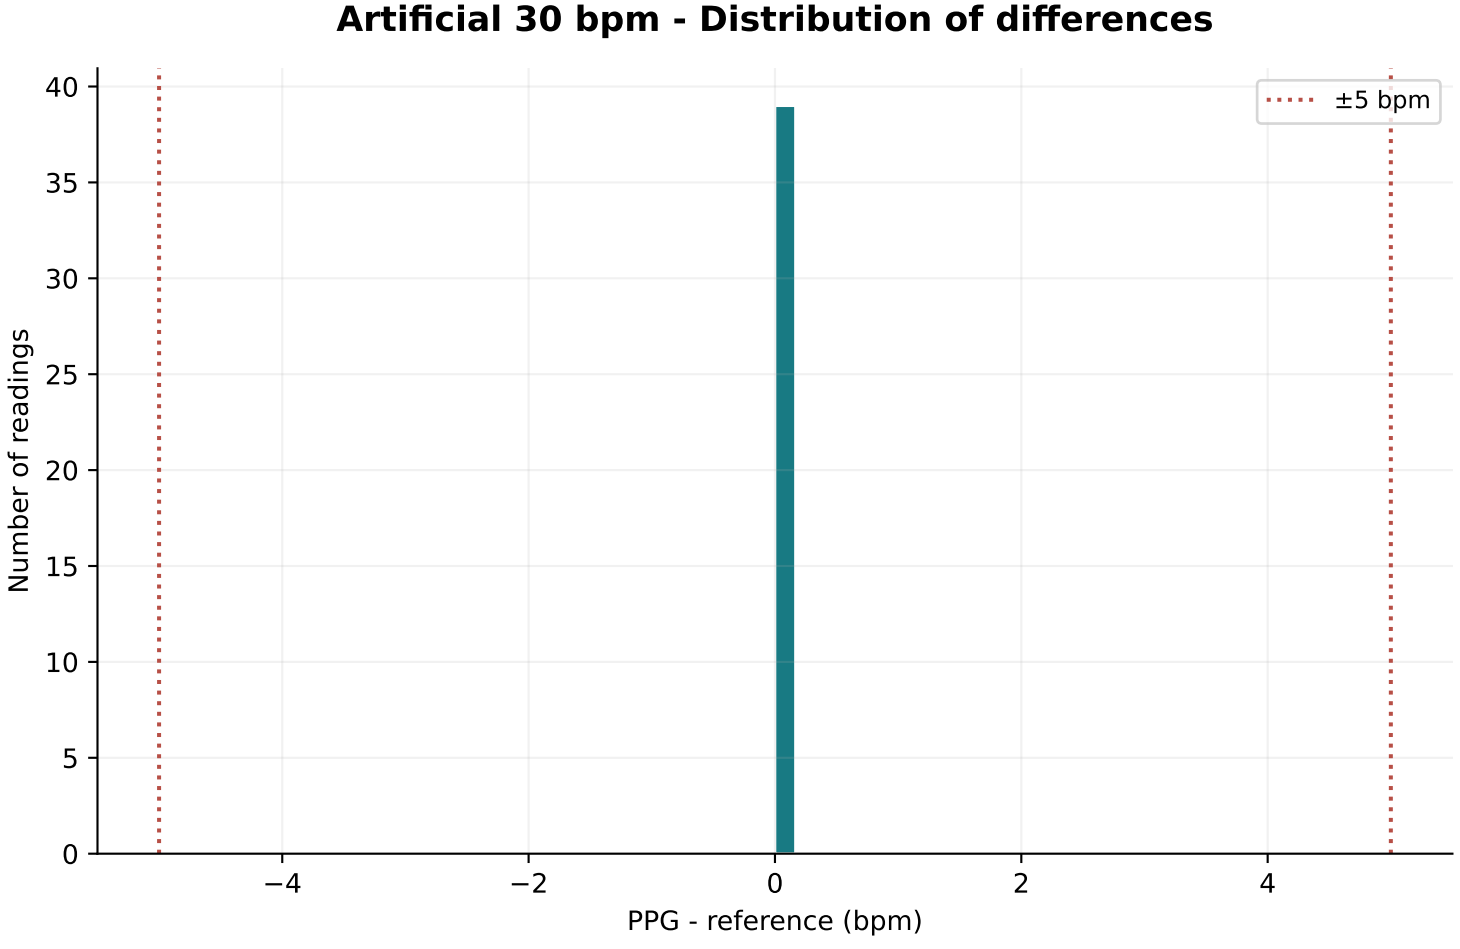
Artificial 30 bpm - Distribution of differences
±5 bpm
Number of readings
0
5
10
15
20
25
30
35
40
−4
−2
0
2
4
PPG - reference (bpm)