
Disperse CHIP

P. Vern Perrove: slan 1 7 grom h Pashites Paru. Assmortin Jerdi Rases 2400 Sam Gialle = chiaunto apria dalle schim Programma Fion Scorse Wali bah BOOTSRAP SVELTEKIT

Events -> OP/PH (Bot.) PILL DISPENSER VO.1 Read ouly Aloren Configurazione Parte 2 Status Configurazione POST DOSAGGIO PRE (min) 50 Device Error 01:20 Dose 1 23:10/ 00:00 POST (min) Dosage time alarm 09:40 08:20 Dose 2 07;30 n dos Dose taken 12:20 11:00 Dose 3 10:10 Dose not taken PRE POST 0 sound Dose 4 16:15 17:05 18:25 Dose left in tray light Dose 5 17:10 18:00 19:20 Battery type 0 **Battery low** Dose 6 17:40 18:30 19:50 Tray type Dosage Device tilted 18:50 20:10 Dose 7 18:00 **Device Tilted** Time Format 0 19:00 20:20 Dose 8 18:10 Daylight sm 1 Sound flag 22:20 Dose 9 20:10 21:00 Pulse 2 output 0 Thread run level 01:20 00:00 Dose 10 23:10 Tray warning 24 Power drain 00:00 00:00 Dose 11 00:00 Start date and time 0 **USB** state Dose 12 00:00 00:00 00:00 Stop date and time 99 SMS state 00:00 Dose 13 00:00 00:00 Serial Number 0 SMS alarm Dose 14 00:00 00:00 00:00 Tray advance counter 00:00 00:00 Dose 15 00:00 Battery level 5322 00:00 00:00 Dose 16 00:00 GSM status 00:00 Dose 17 00:00 00:00 Attitude 00:00 00:00 Dose 18 00:00 Next dose index 00:00 00:00 Dose 19 00:00 Take dose signal 00:00 00:00 Dose 20 00:00 Flip counter Dose 21 00:00 00:00 00:00 Device Error code 00:00 00:00 Dose 22 00:00 Get Status 00:00 00:00 Dose 23 00:00 00:00 00:00 Dose 24 00:00 Set Config Get Config Log file Impostazioni di connessione Log Log 192.168.10.25 65432 Socket Versione FW IV-005 Program Values Informazioni orario Ora Pill dispenser set Data Get Data



2 83 60 • info@vsas.ch Fax 032 32 Tel. 032 322 85 78 • 2503 Biel/Bienne Werkhofstrasse 9

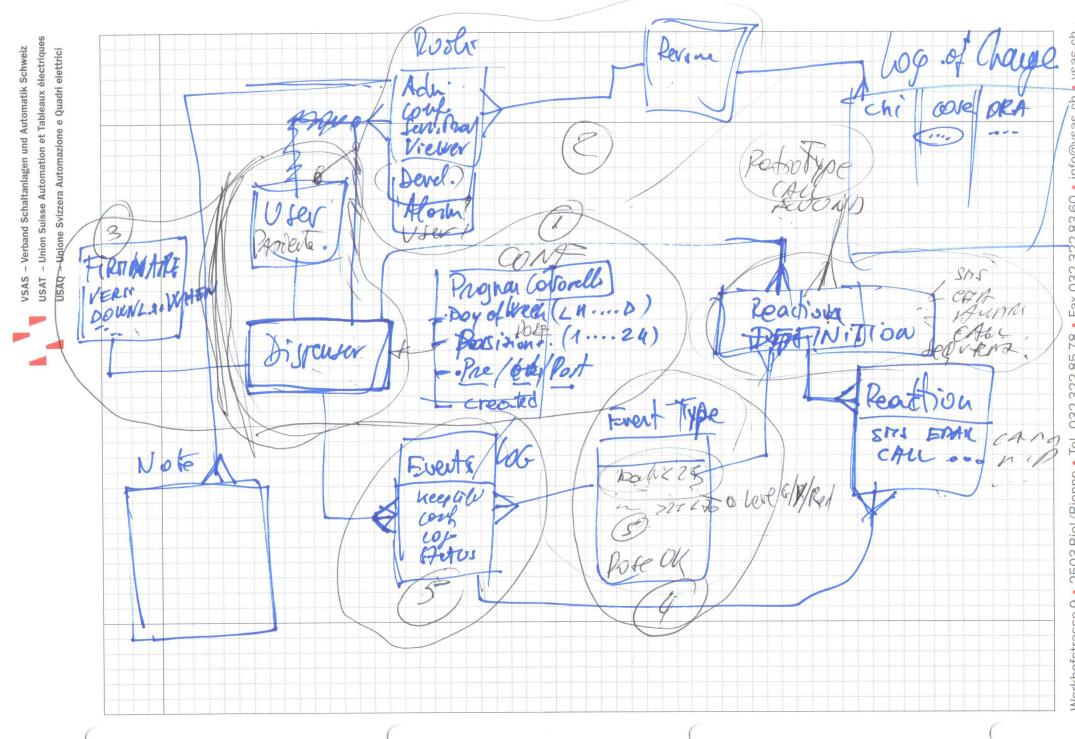