
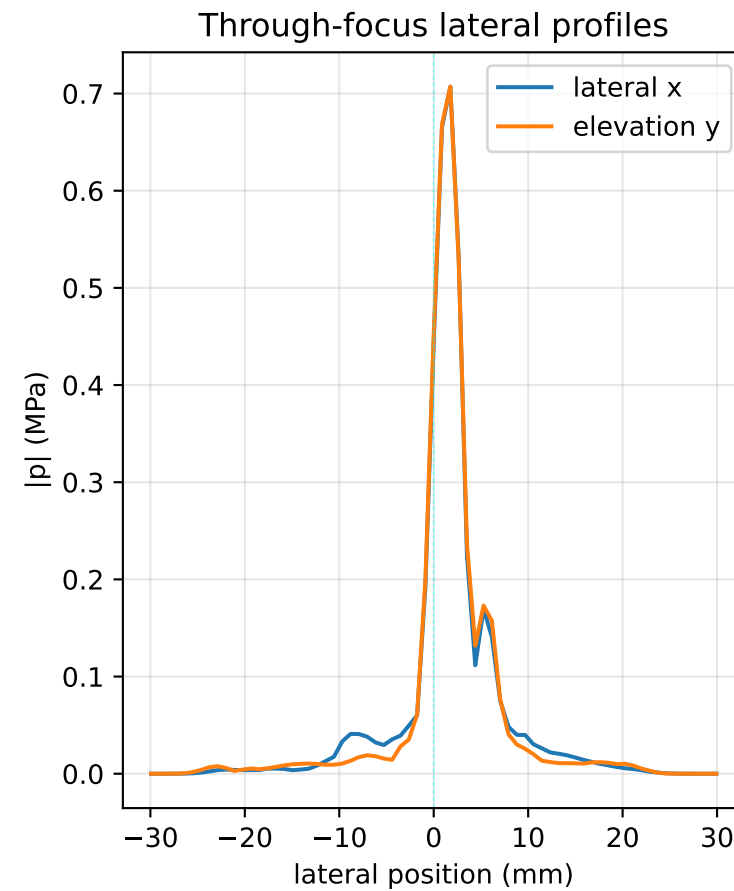
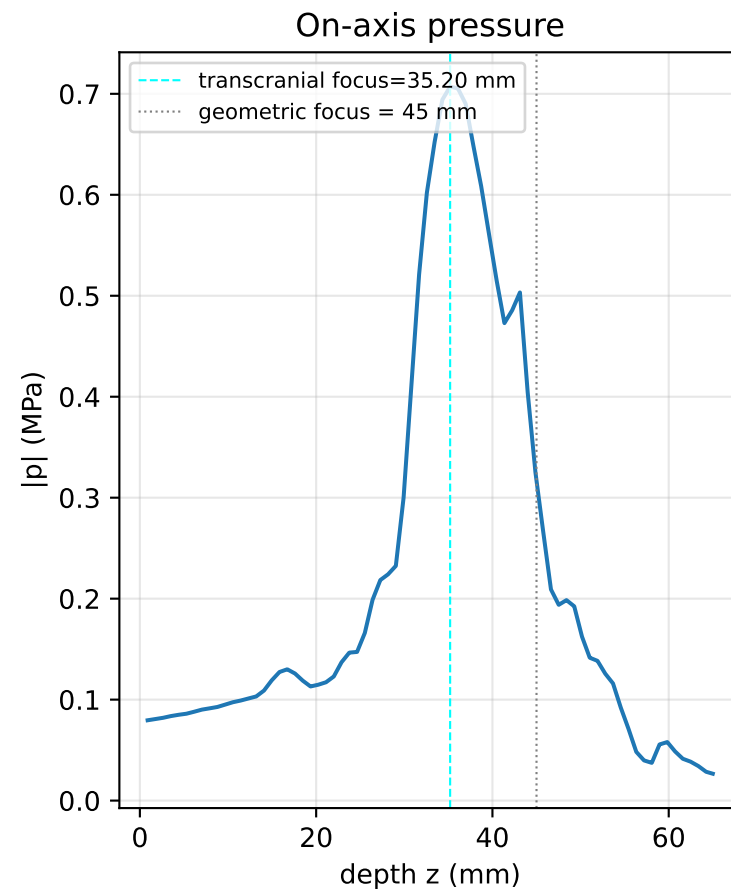


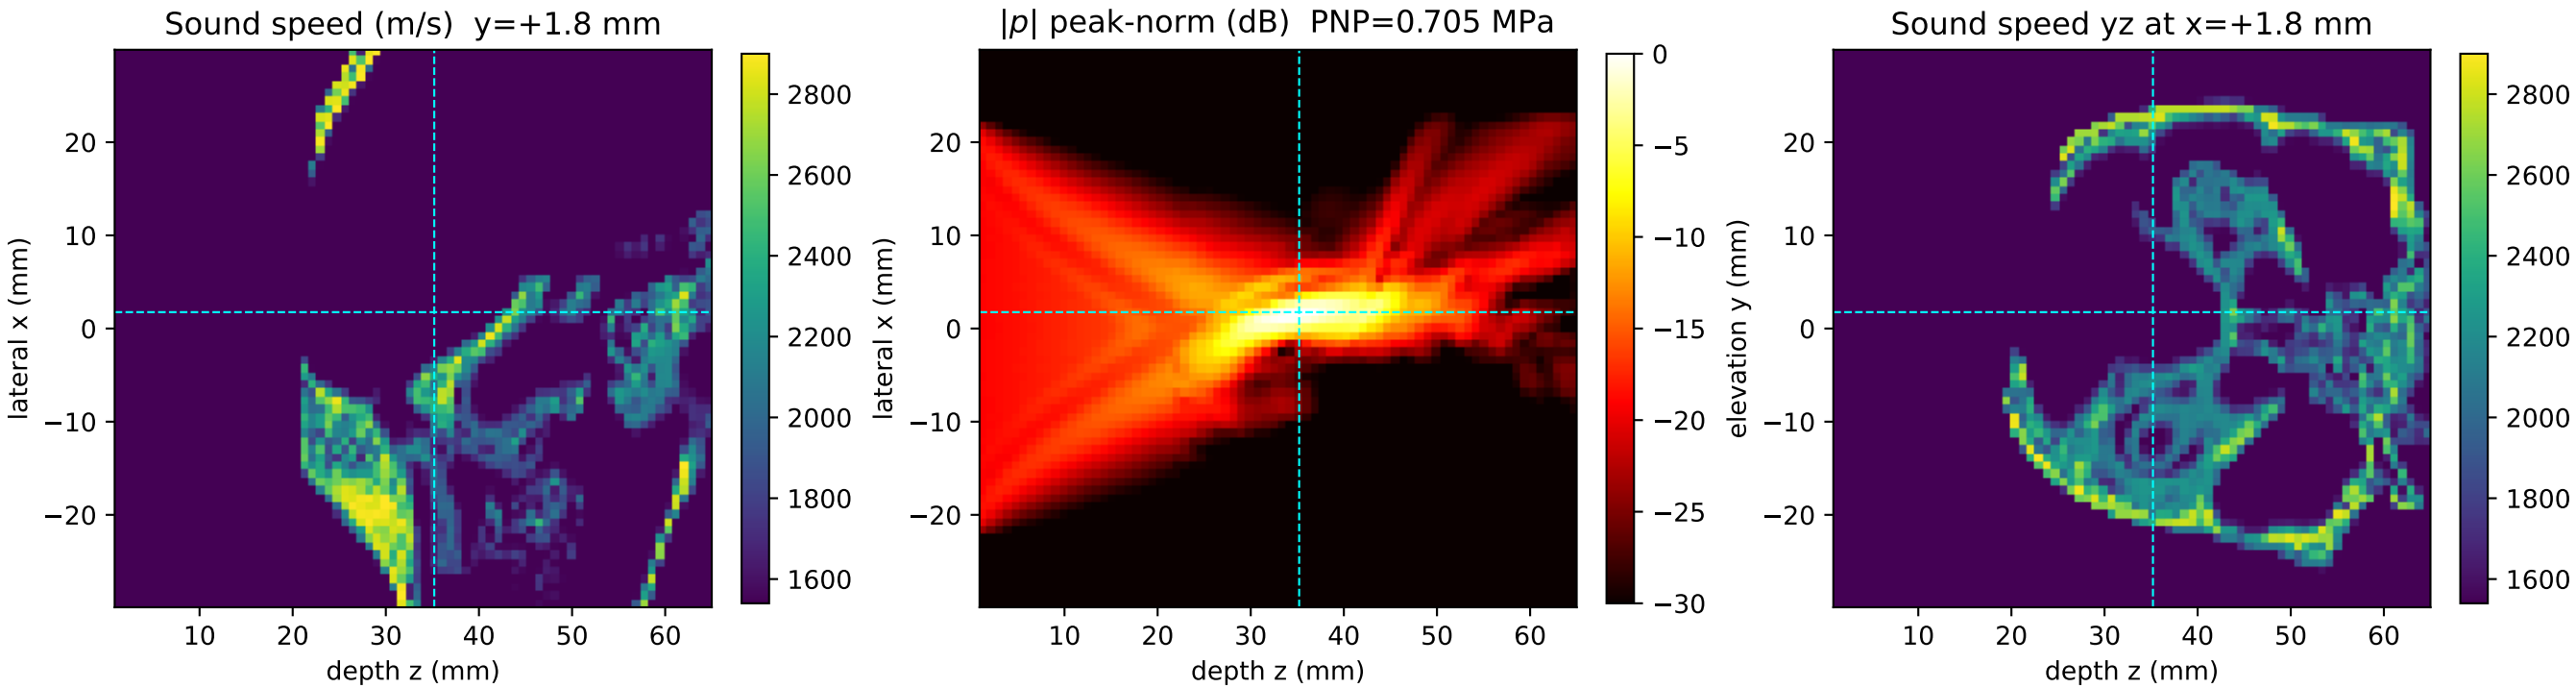

$f_0 = 500$ kHz
 Aperture = 45 mm
 ROC = 45 mm
 $f\# = 1.0$
 MI target = 1.0
 Free-field PNP target = 0.707 MPa
 Drive p_0 at source = 78.3 kPa

Transcranial focal $z = 36.08$ mm
 Geometric focus $z = 45.00$ mm
 Refraction shift = -8.92 mm
 Transcranial peak PNP = 0.705 MPa
 Focal loss = -0.02 dB

Grid: 69x69x241
 $\Delta x = 880 \mu\text{m}$ $\Delta t = 114.3$ ns