
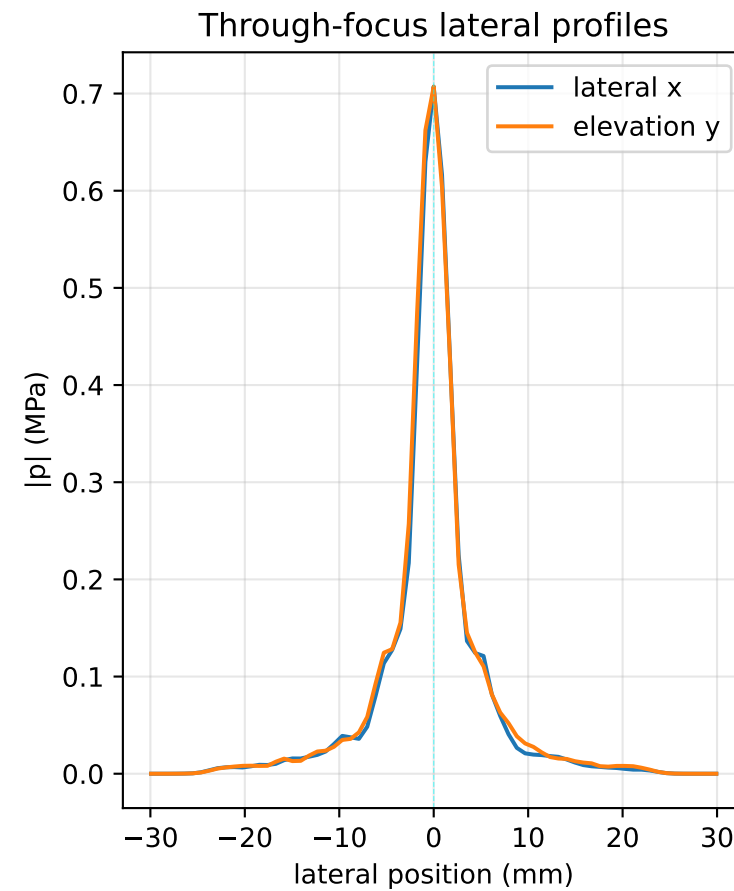
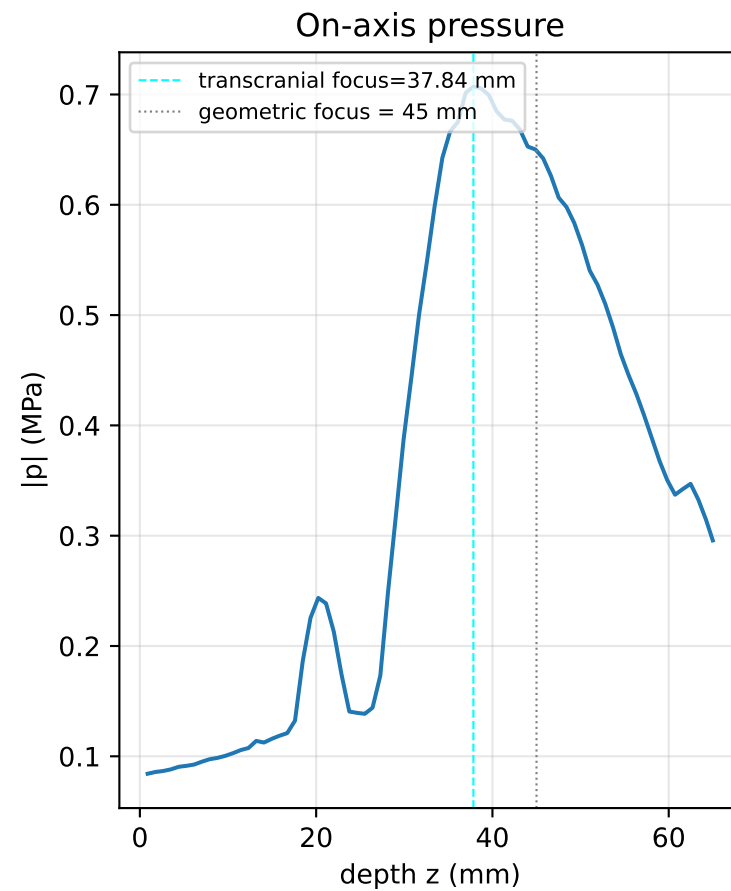


AMNH M-87264 macaque dACC, 500 kHz f/1 transcranial focal field

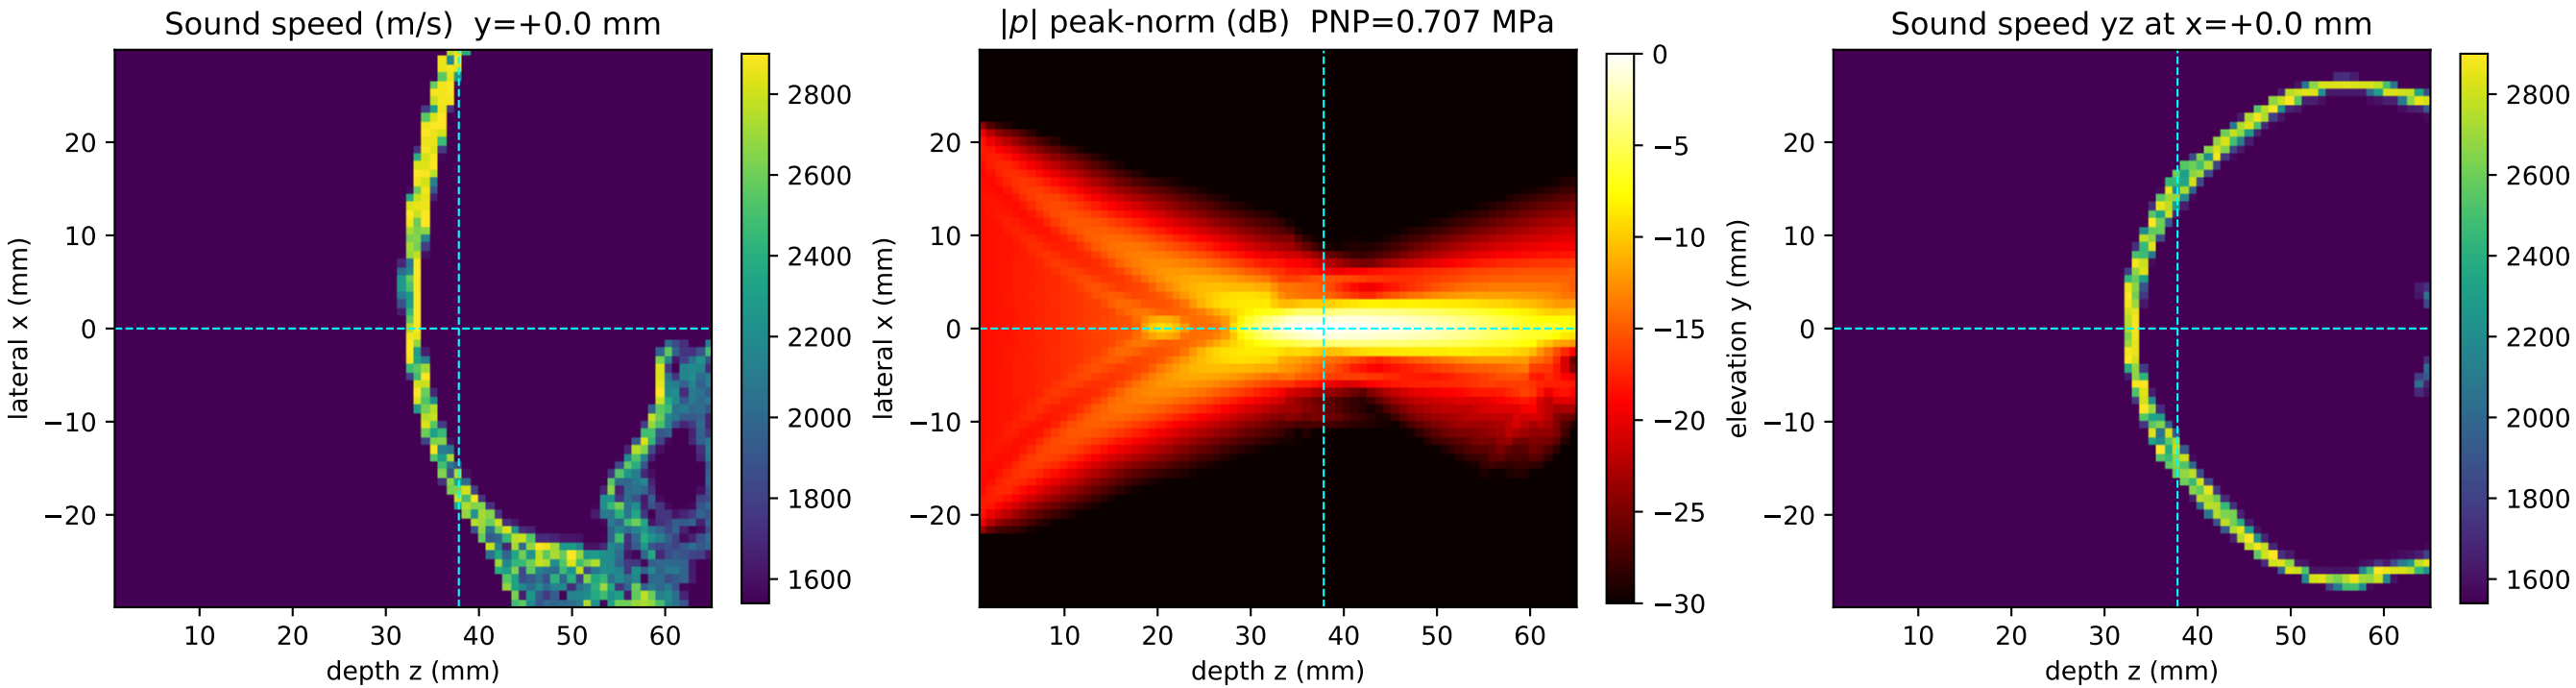

$f_0 = 500$ kHz
 Aperture = 45 mm
 ROC = 45 mm
 $f\# = 1.0$
 MI target = 1.0
 Free-field PNP target = 0.707 MPa
 Drive p_0 at source = 83.0 kPa

 Transcranial focal z = 37.84 mm
 Geometric focus z = 45.00 mm
 Refraction shift = -7.16 mm
 Transcranial peak PNP = 0.707 MPa
 Focal loss = +0.00 dB

Grid: 69x69x241
 $\Delta x = 880 \mu\text{m}$ $\Delta t = 114.3$ ns