




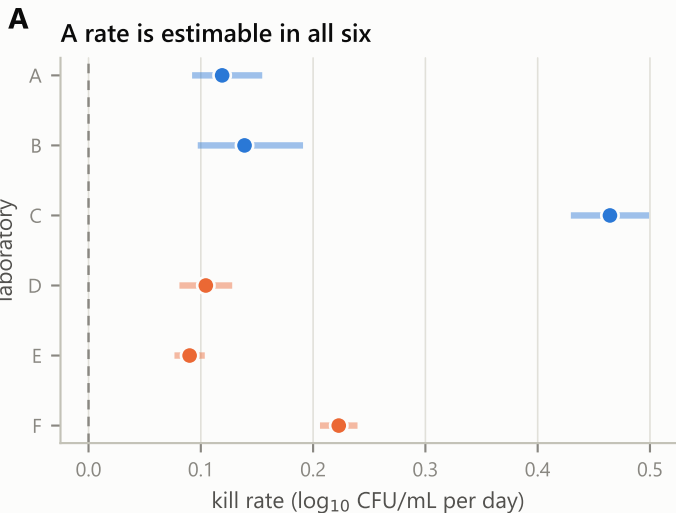


MXF 10x MIC. Bars are 95% profile-likelihood intervals from the censored (Tobit) fit. Blue: laboratory ever cleared a flask. Orange: never cleared, in any arm.

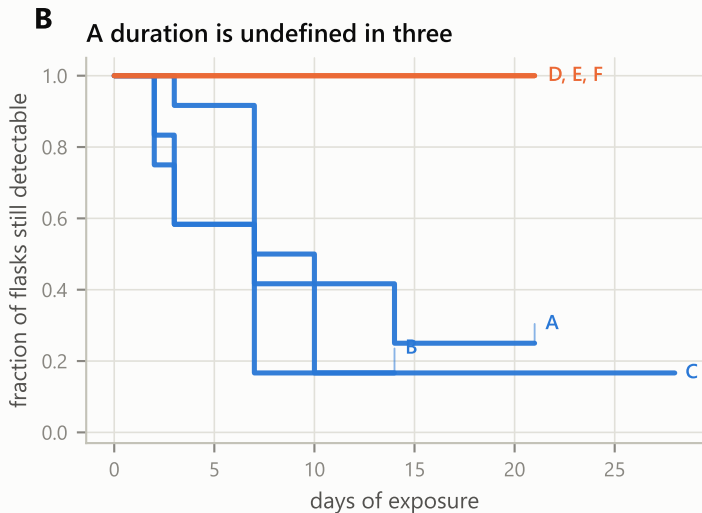

Kaplan-Meier over all treated flasks. Three curves never descend: those laboratories recorded no flask below the limit in any arm, so no clearance time exists for them.

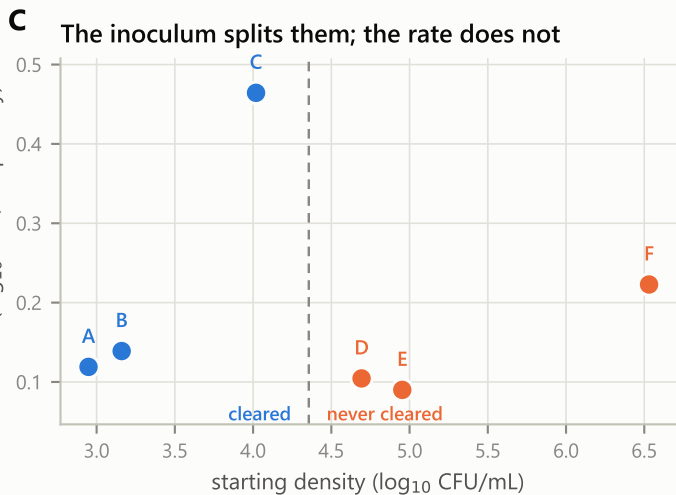

The three lowest starting densities are exactly the three laboratories that cleared. F kills faster than four of the other five and never clears.

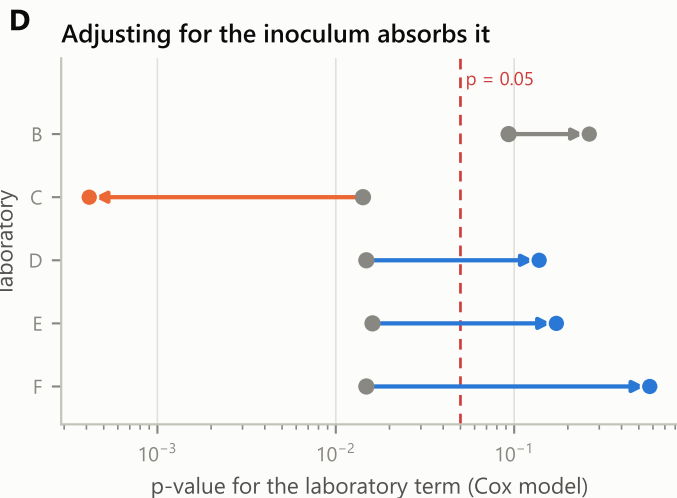

Grey: laboratory alone. Arrow head: after adding starting density. Blue crosses from significant to not. Orange (C) stays significant and also has the fastest rate.