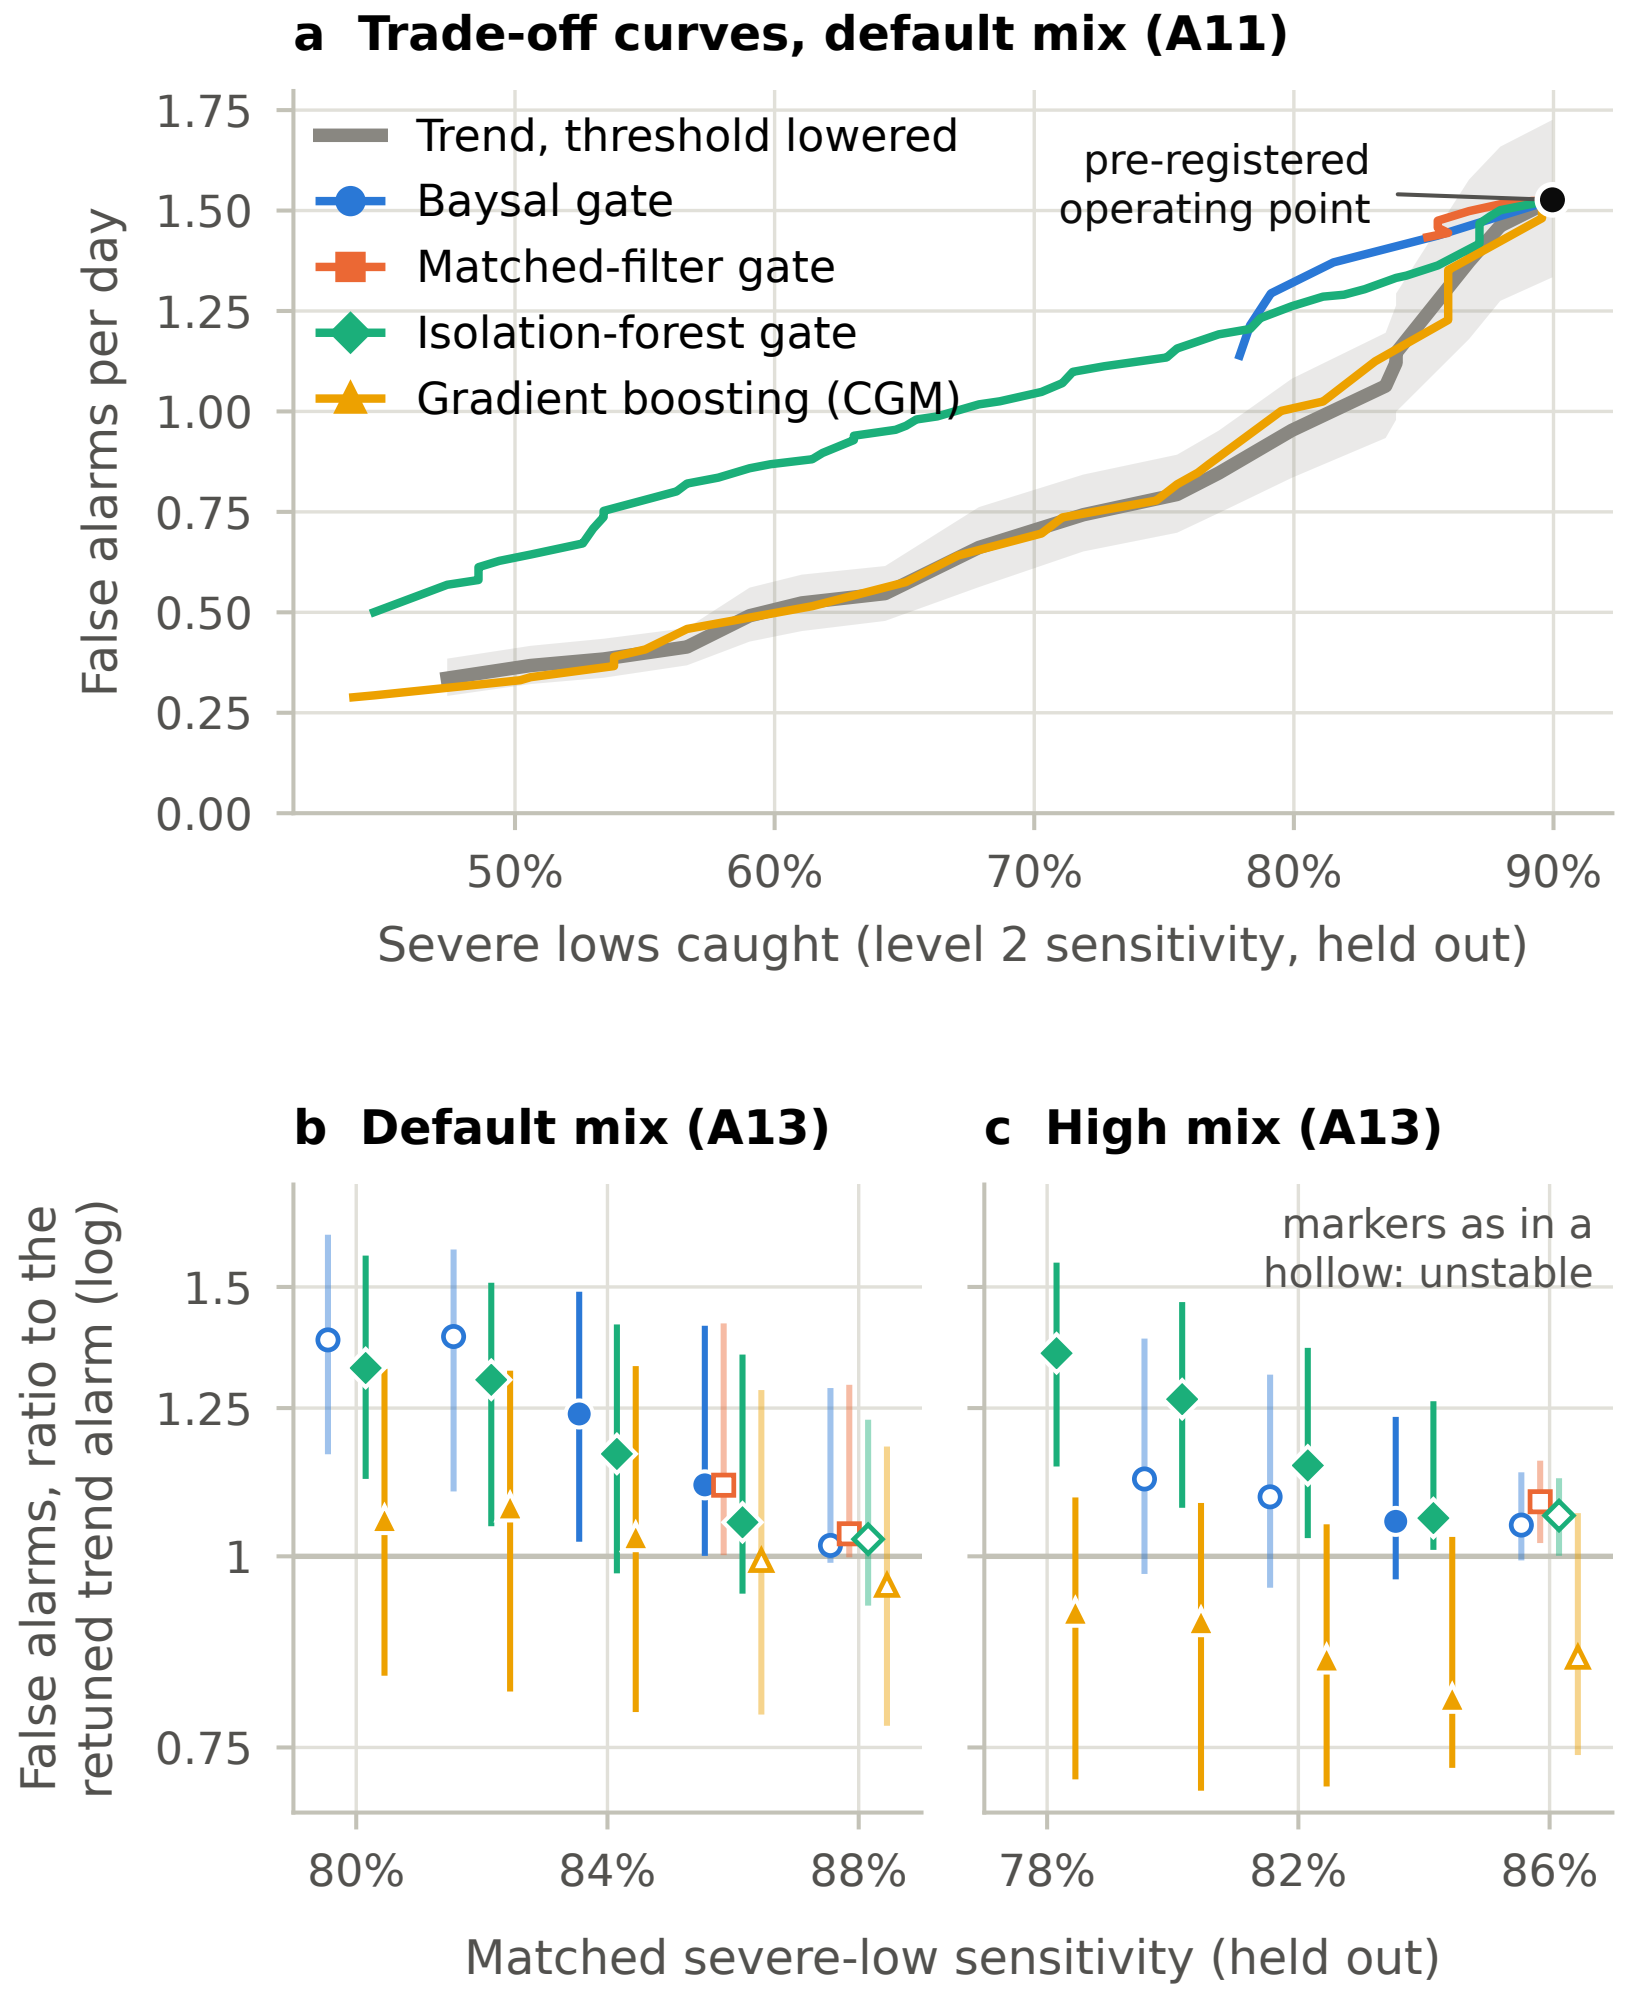
a Trade-off curves, default mix (A11)
Trend, threshold lowered
Baysal gate
Matched-filter gate
Isolation-forest gate
Gradient boosting (CGM)
pre-registered
operating point
False alarms per day
1.75
1.50
1.25
1.00
0.75
0.50
0.25
0.00
50%
60%
70%
80%
90%
Severe lows caught (level 2 sensitivity, held out)
b Default mix (A13)
c High mix (A13)
markers as in a
hollow: unstable
False alarms, ratio to the
retuned trend alarm (log)
1.5
1.25
1
0.75
80%
84%
88%
78%
82%
86%
Matched severe-low sensitivity (held out)