High Fidelity: Calibrated Gemini Judge Matches 93.3% of Human Ground Truth

Blind evaluation on 90 human Gold Standard cases in SpecMine (Cohen's κ = 0.907, Gwet's AC_1 = 0.926, Friction Recall = 100%)

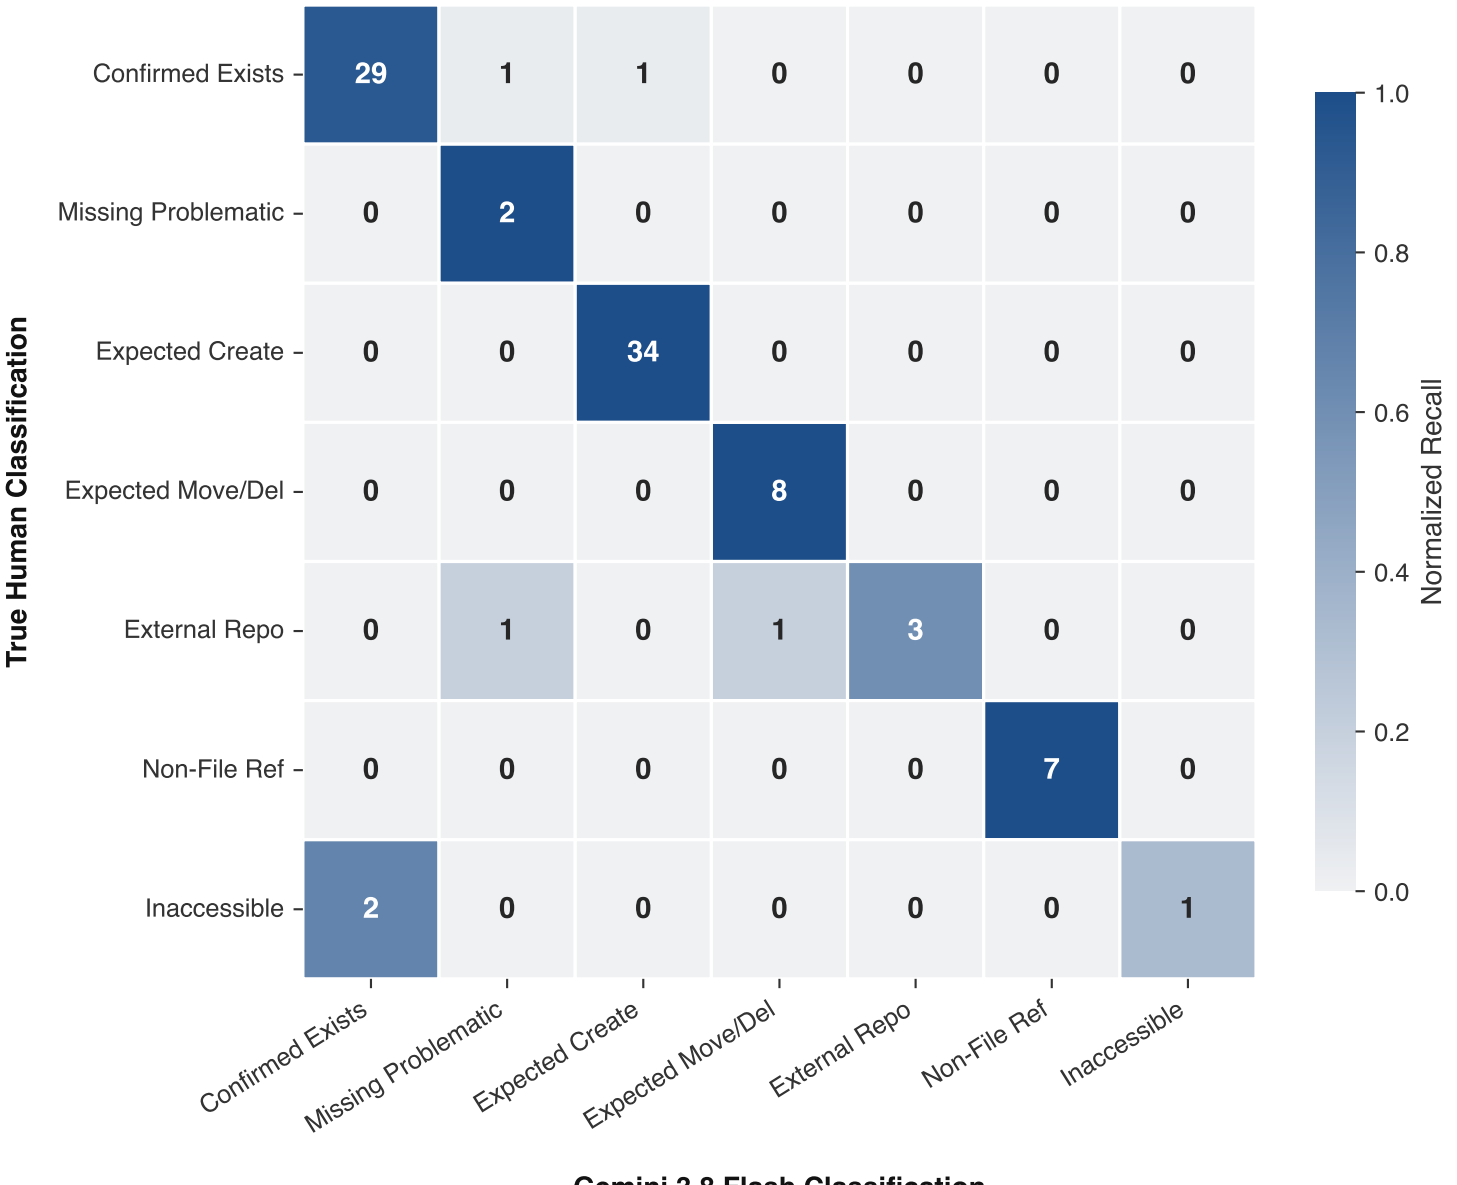

Source: Hand-validated Gold Standard (N = 90 distinct repositories). Evaluated blindly without prior exposure.