

Streamline urine collection and transport

New 3-tube BD Vacutainer® Urine closed collection kits



Studies show that specimen contamination, deterioration and overgrowth are widespread.^{1,2}

The BD Vacutainer® Urine Collection System can help:



Reduce
contamination*



Improve treatment
decisions and outcomes*



Improve diagnostic
accuracy*



Reduce the risk of
leaks and exposure*

*As compared to open collection methods

Closed collection kits
can yield:



Efficiency*



Consistency*³



Sample integrity⁴




Automation ready⁵

*As compared to sourcing from various bulk
device and tube options available



BD Vacutainer® Urine closed collection kits

Standardization to closed collection kits may:*

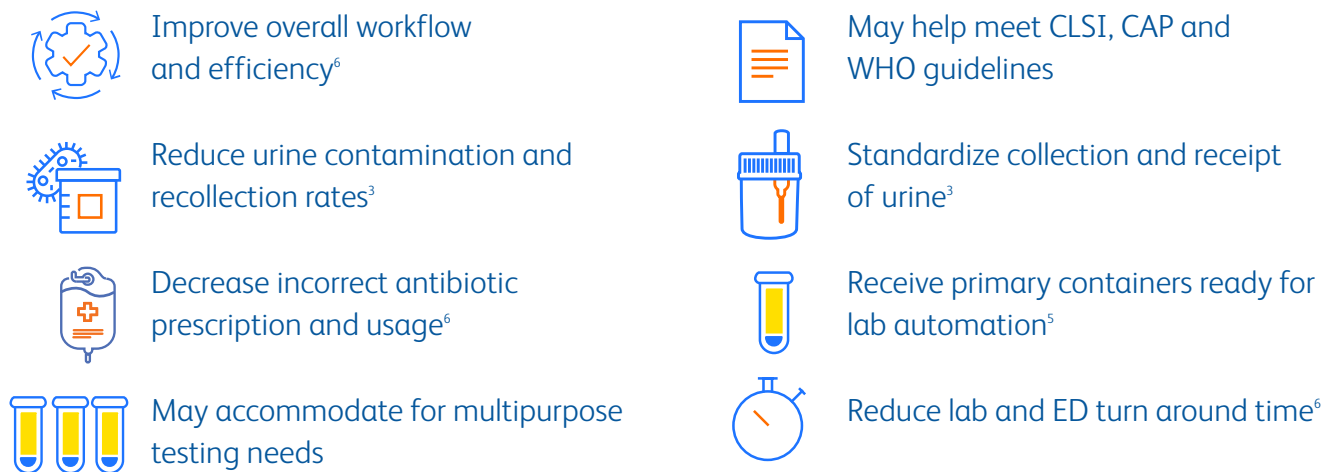

*when using the 3-tube Urine Closed System in conjunction with 2-step urine culture ordering

Quality sample in = Quality result out

Ordering information:

BD Vacutainer® Urine Complete Cup Kit (3-tube) Hemogard® Stopper	BD Vacutainer® Urine Complete Cup Kit (3-tube) Conventional Stopper
BD REF# 364932 (50/case)	BD REF# 364934 (50/case)
Castile soap wipe	Castile soap wipe
BD Vacutainer® Urine Collection Cup with integrated transfer device	BD Vacutainer® Urine Collection Cup with integrated transfer device
BD Vacutainer® C&S Preservative, 4.0 mL round bottom tube	BD Vacutainer® C&S Preservative, 4.0 mL round bottom tube
BD Vacutainer® Urinalysis Preservative, 8.0 mL round bottom tube	BD Vacutainer® Urinalysis No Additive, 8.0 mL conical tube
BD Vacutainer® No Additive (Z) Discard Tube, 6.0 mL round bottom tube	BD Vacutainer® Urinalysis No Additive, 10.0 mL round bottom tube

References: 1. Bekeris LG, Jones BA, Walsh MK, Wagar EA. Urine culture contamination: a College of American Pathologists Q-Probes study of 127 laboratories. *Arch Pathol Lab Med*. 2008;132(6):913–917. 2. Eisinger SW, Schwartz M, D am L, Riedel S. Evaluation of the BD Vacutainer Plus Urine C&S Preservative Tubes compared with nonpreservative urine samples stored at 4°C and room temperature. *Am J Clin Pathol*. 2013;140(3):306–313. 3. F. Charra et al. Quality improvement program of adult urinary tract infection management: Review and impact, *Médecine et Maladies Infectieuses*, 2017;47(8):519-525. ISSN 0399-077X, <https://doi.org/10.1016/j.medmal.2017.07.008>. 4. Instructions for Use. BD Vacutainer Urine Products. VDP40397(02). Becton, Dickinson and Company. 2021. 5. BD Kiestra™ Urine Culture Application User's Manual. L012256(01). Becton, Dickinson and Company. 2021. 6. Stagg A, Lutz H, Kirpalaney S, Matelski JJ, Kaufman A, Leis J, McCready J, Powis J. Impact of two-step urine culture ordering in the emergency department: a time series analysis. *BMJ Qual Saf*. 2018 Feb;27(2):140-147. doi: 10.1136/bmjqs-2016-006250. Epub 2017 May 3. PMID: 28468911; PMCID: PMC5867434.

BD, 1 Becton Drive, Franklin Lakes, NJ 07417-1880, U.S.
201.847.6800

bd.com



BD, the BD Logo, Hemogard and Vacutainer are trademarks of Becton, Dickinson and Company or its affiliates.
© 2025 BD. All rights reserved. (BBD-138311 4371-US-0925 September 2025)