

PHILIPS

University

Monitoring and Analytics
Therapeutic Care

Product Information that **Resonates**

Product Description and Sales Text Guidelines, June 2018

Launch

Contents

Introduction to product information

- Meaning 4
- Components 5
- Importance 6
- Onus of creation and validation 7
- Systems in which product information is updated and stored 8
- Flow of product information within Philips' systems 9
- Flow of product information within Philips' systems (contd.) 10
- Translation and localization 11

Creating good product information

- Limiting factors 13
- Validation criteria 14
- Guidelines for writing good sales texts 15
- Points to avoid 16
- Points to avoid (contd.) 17
- Good sales text examples 18

Formatting guidelines

- Formatting 20
- Language 21
- Product names 22
- Capital letters 23
- Spacing 24
- Hyphens 25
- Units of measurement 26
- Numbering 27
- Acronyms and abbreviations 28
- General considerations 29



Introduction


This section describes the meaning, components, and the importance of product information.

It also identifies the systems in which the product information is updated and stored, and outlines it's flow within these systems, right up till the translation process.

Meaning of **product information**


Product information is the text used in customer facing documents like quotes (offers), invoices and shipment documents.

It explains to our customers what we, at Philips, are offering, delivering and invoicing.

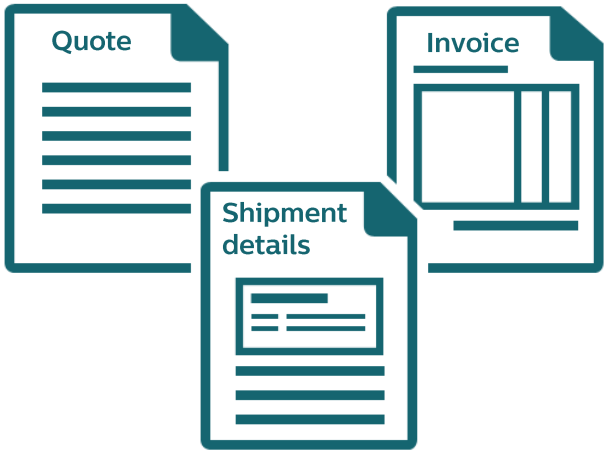

Components of **product information**

Product information includes a description and the sales text, used to precisely describe a product and the product options.

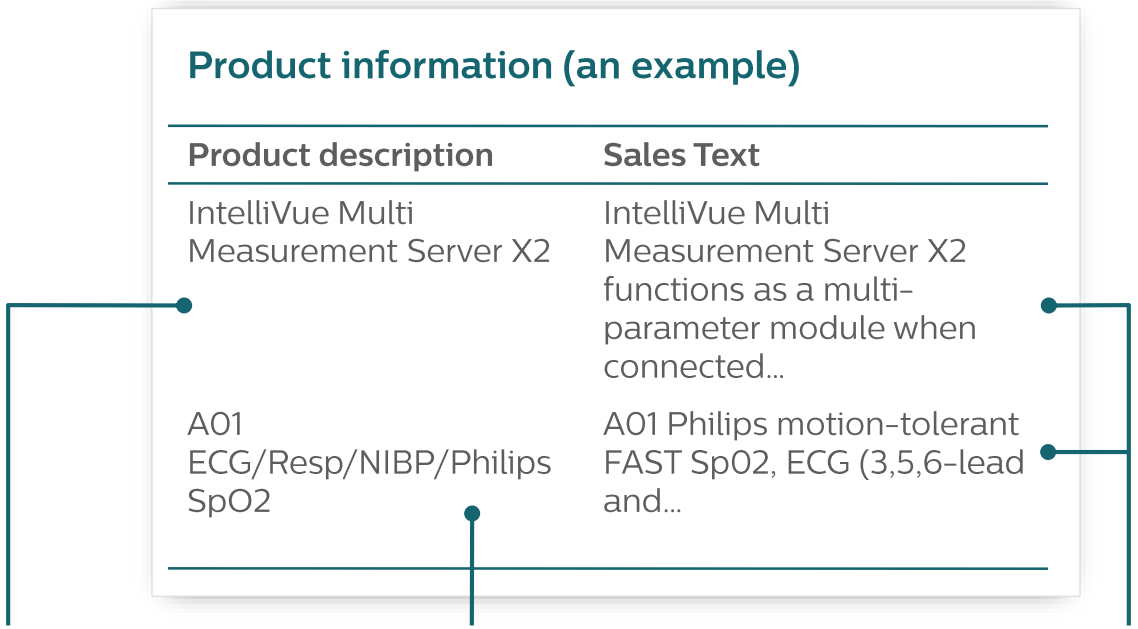

Product description:

Also known as short sales text, the product description is used to briefly describe the base product.

Product option description:

This is a brief description for each product option available for the base product.

The first three letters (for example, A01) form the option code and the rest describes the option.

Sales text:

Also known as long sales text, the sales text is used to describe the base product and product options in detail.

Importance of **good product information**



Can be easily understood

Good product information can be easily understood by the customer, and effectively conveys the purpose of the information.



Avoids confusion and wastage of time

It does not confuse the customer, thereby saving the commercial teams' time in explaining what is being offered, delivered and invoiced.



Upholds Philips' professional image

Well written product information upholds Philips' professional image, and augments the efforts made by the sales teams.



Leads to timely acceptances and payments

Good product information effectively conveys what was intended, resulting in timely installation acceptances and payments of invoices.

1500 workdays are being wasted annually by the MA/TC sales teams in manually rewriting the texts in customer facing documents, because good product information was missing in the earlier version(s).

(Source: MA/TC sales team CPQ survey, 2017 and Six Sigma study in Sweden, 2016).

Onus of creation and validation of **product information**



Creation

The product information (English versions) is created by the **product managers** in collaboration with global M2O sales enablement.



Validation

It is then validated by the **Market Sales teams**. It is the responsibility of the product managers to get the product information validated.



Entry in eDMR/ SAP MP1

Depending upon whether the product is eDMR or non-eDMR controlled, product information is loaded in the following systems:

- For eDMR controlled products, the descriptions and sales texts are loaded into eDMR.
- In the case of non-eDMR controlled products (i.e. HRC and CS), the descriptions and sales texts are maintained by the business units (BUs), and loaded into the MA/TC pricing database for commercial catalog integration.

It is the responsibility of the **business unit** to have the product information entered, and to keep it updated.

Systems in which product information is **updated and stored**




eDMR

Product information is updated in eDMR by product managers.



SAP MP1

- Product information is transferred to SAP MP1 (long sales texts for options are not stored).
- Product information for non-eDMR products is either fed from other systems or entered directly into SAP MP1 by knowledge engineers.



MA/TC pricing database

Sales texts for eDMR and non-eDMR controlled products are loaded into the MA/TC pricing database.

From this database, the sales texts are extracted for translation and transferred to the Philips' commercial quotation tool.




Philips' commercial quoting tool

Both product descriptions (in English) and sales texts (in local languages) are received from the MA/TC pricing database.

Flow of product information within **Philips' systems**


For eDMR controlled products

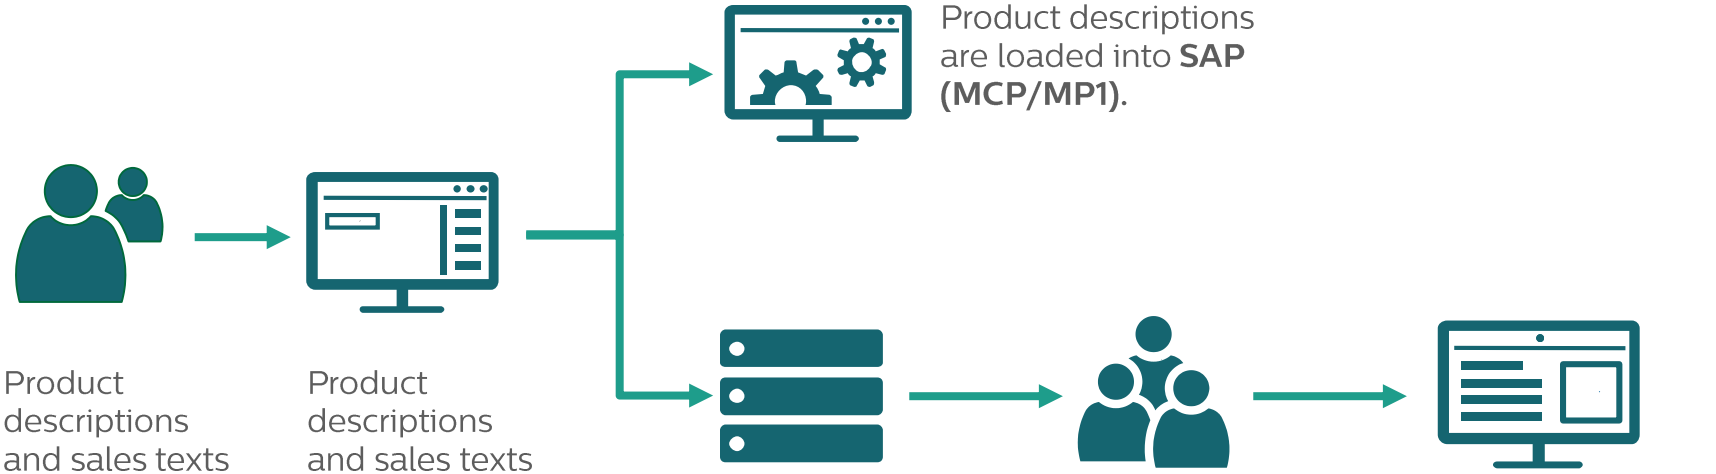

*Other ad hoc processes may also exist.

Flow of product information within **Philips' systems** (contd.)

For non-eDMR controlled products

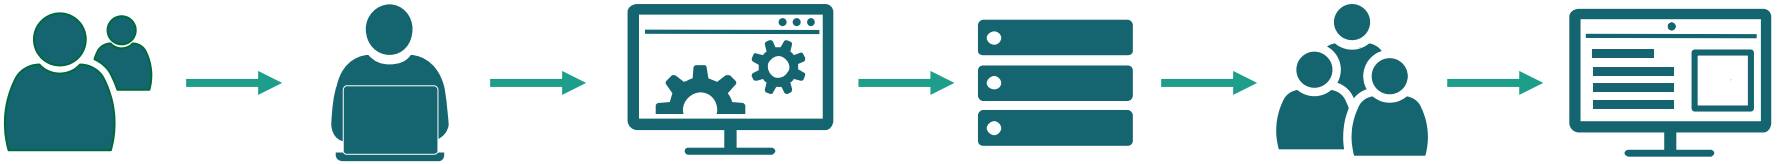

Product descriptions and sales texts (English versions) are created by the **Product Managers.**

SAP structures are created by the **Knowledge Engineers.**

SAP structures are updated to the **SAP MP1** by the knowledge engineers.

Product descriptions (from SAP MP1) and sales texts (manually) are loaded into the **MA/TC pricing database.**


Product descriptions and sales texts are extracted and sent to an **external translation agency (SDL)** for translation.

Product descriptions (in English) and sales texts (in local languages) are imported from the MA/TC pricing database to the **Philips' commercial quotation tool.**

*Other ad hoc processes may also exist.

Translation and localization of **product information**

4. The translated texts are loaded back into the **MA/TC pricing database.**

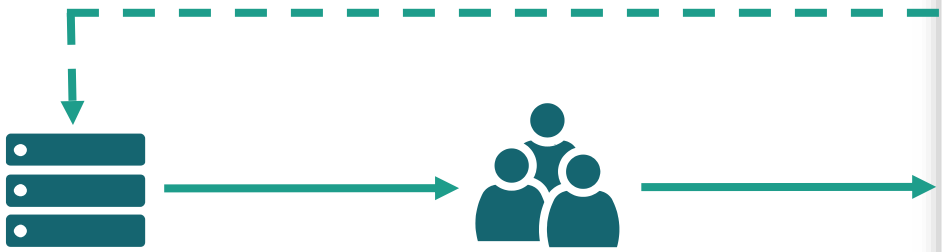

1. English versions of the product descriptions and sales texts (both new and recently modified) are loaded in the **MA/TC pricing database.**

2. Product descriptions and sales texts are extracted and sent to an **external translation agency (SDL)** for translation.


Standard translations:

- Dutch
- Finnish
- French
- German
- Italian
- Spanish
- Swedish

Possible localizations:

- Russian
- ...

3. The SDL translates them into a **standard set of languages** and **localized languages.**

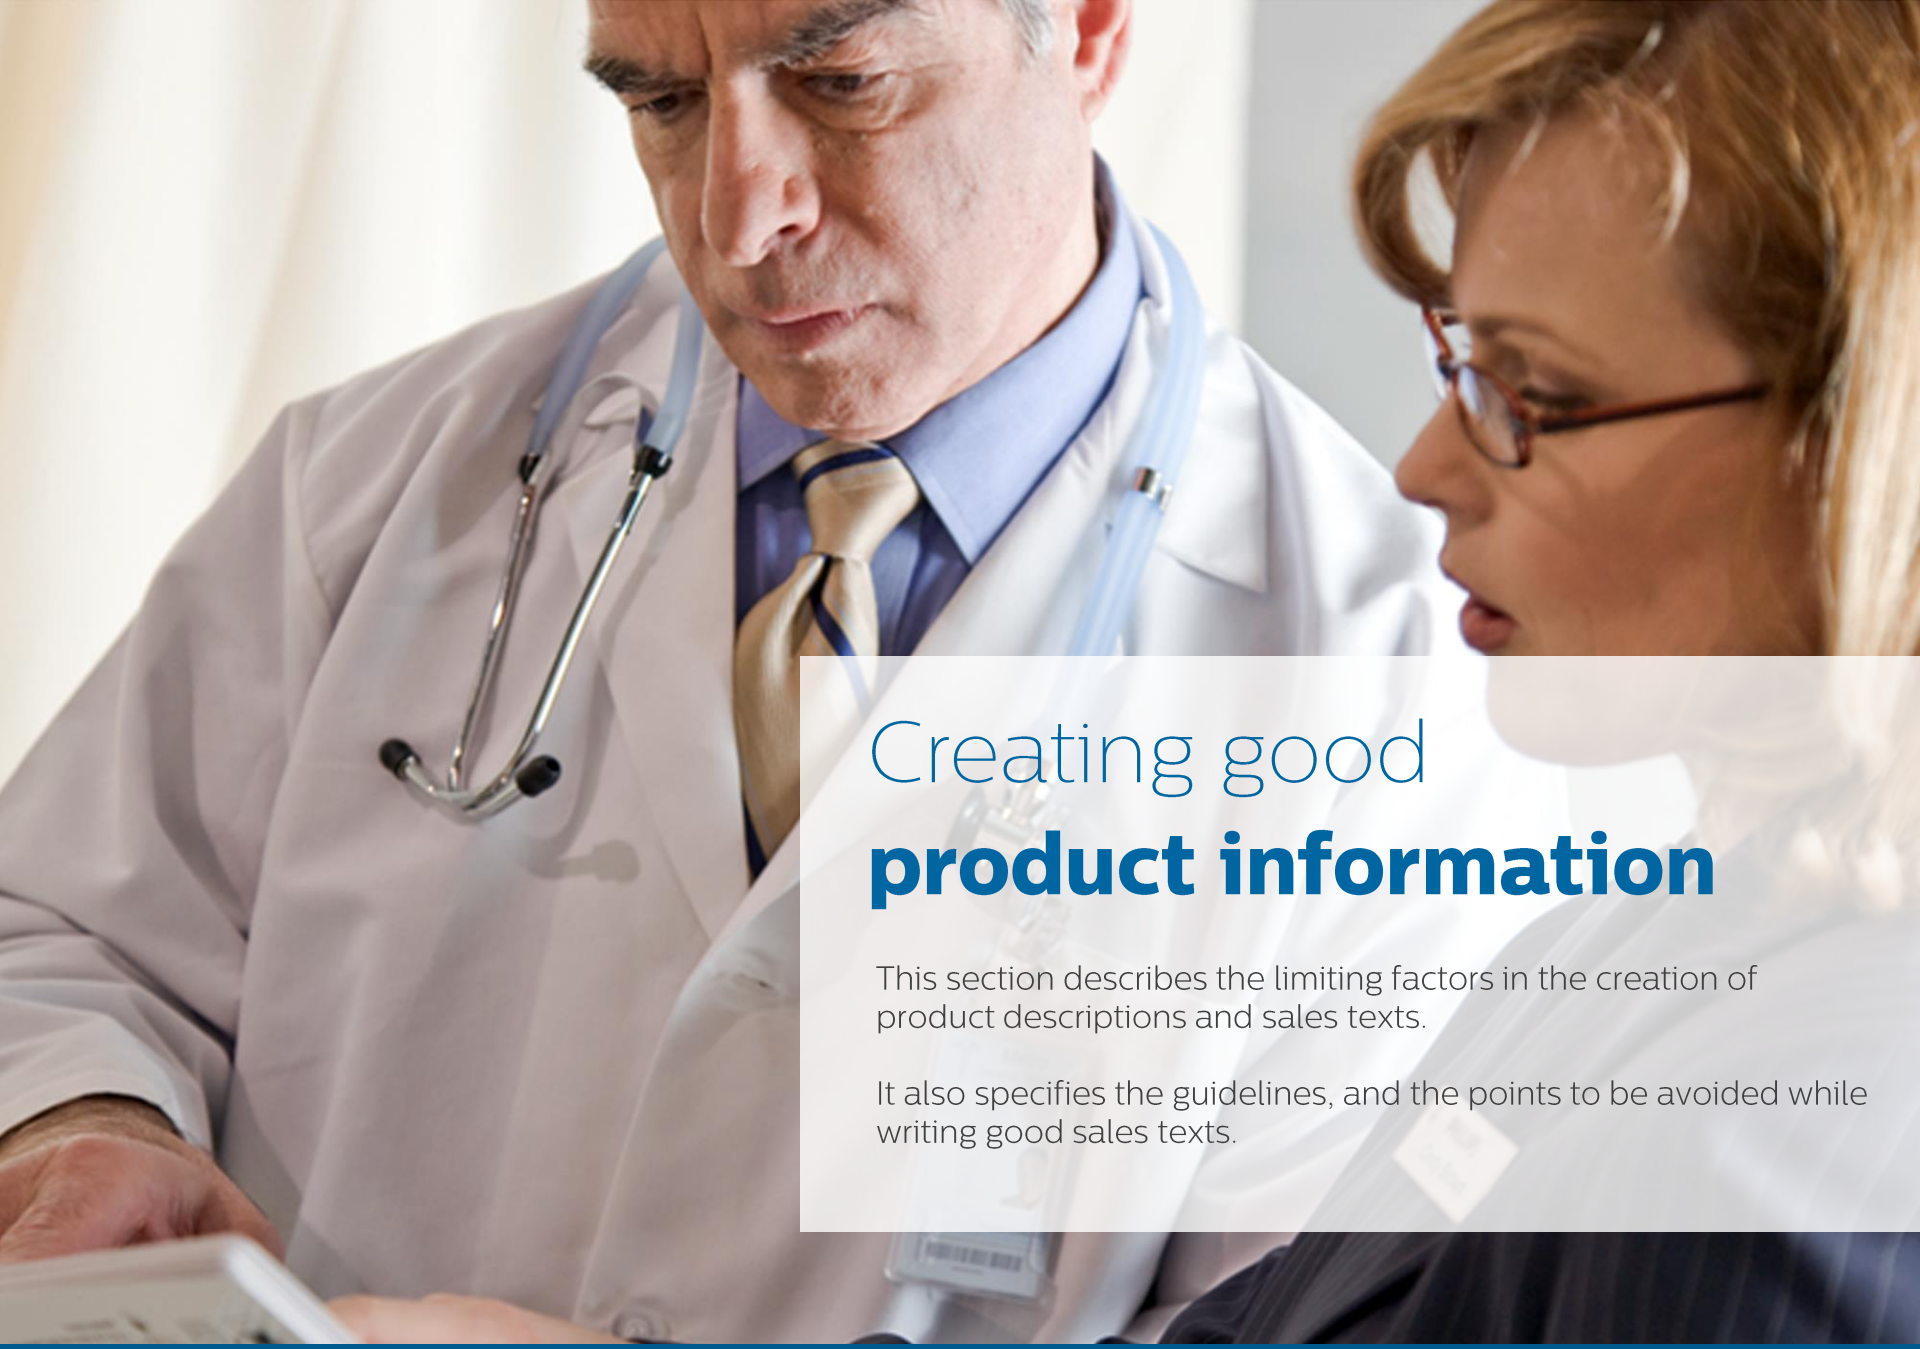

Creating good **product information**

This section describes the limiting factors in the creation of product descriptions and sales texts.

It also specifies the guidelines, and the points to be avoided while writing good sales texts.

Limiting factors

Due to layout constraints in the SAP MP 1 document, the following limiting factors exist in the creation of product descriptions and sales texts.

Product description

IntelliVue Multi Measurement...

Text limited to 40 characters.
Remaining: 9

The product description should not exceed 40 characters (including spaces). This limitation also applies to the translated product description.

Product option short sales text

A01 ECG/Resp/NIBP/PhilipsSpO2

Text limited to 30 characters.
Remaining: 1

The product options short sales text should not exceed 30 characters (including spaces), of which the first three characters are reserved for the three-letter option code (A01, as shown in the illustration), followed by a space. The remaining 26 characters are available for describing the product option.
This limitation also applies to the translated option text.

Sales text and internal ordering instructions


The IntelliVue Multi Measurement...

Sales text and internal ordering instructions do not have a limitation on the number of characters.

*The above illustrations have been created only for the purpose of understanding, and do not represent the SAP MP1/ eDMR interface.

Validation criteria

Product information can be considered good, when a trained healthcare professional like a doctor, purchasing officer, bio-med (bio-medical engineer), or a nurse (who is not familiar with the Philips' portfolio), understands what (s)he is getting while accepting Philips' offer, without the sales team having to explain the offer content.

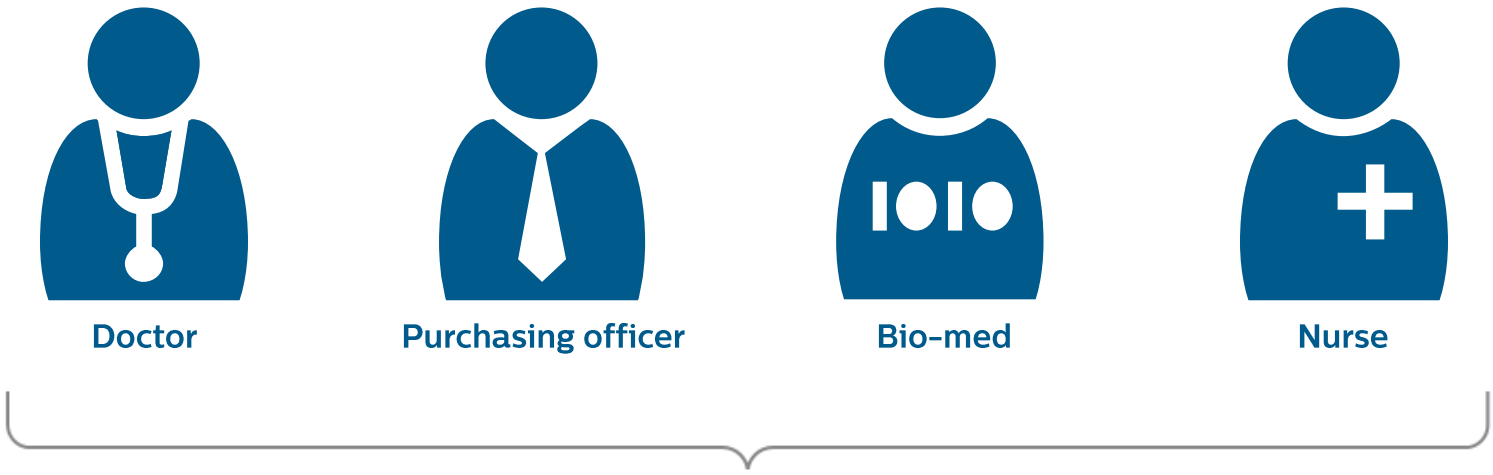

"We understand the offer!"

Guidelines for writing **good sales texts**



Be concise
Sales texts should concisely describe what is being offered, delivered and invoiced. The description should be factual, without abbreviations, and should comprise of complete sentences.



Emphasize on value
Product's features that are of value to the customer should be given emphasis within the sales texts.



Check for linkages
Sales texts should conceptually link to existing sales collaterals like brochures, datasheets, etc. The intent should be to complement the existing sales material, and not to paraphrase or replace it.



Run a word-check
Sales texts should be checked for spellings, and should be validated for correct grammar and syntax by a native English speaker.



Ensure correct product name spellings
The product names should be correctly spelled (as per the official spellings) in the sales texts.



Follow formatting guidelines
Formatting guidelines should be followed while creating the sales texts.

Points to **avoid**



Claims and comparisons

Do not make claims, statements or comparisons that differentiate Philips' products from those of the competitors. If required, this may be done in other regulatory approved sales collaterals.



Optional features and functionalities not in the product

Avoid listing or describing the optional features and functionalities that are not included in the base product or the product option.



Technical part descriptions or manufacturing lists of components

Avoid the use of technical part descriptions or manufacturing lists of components, unless they are commonly understood and provide important clarifications. Sales texts, however, may contain the list of supplies included in the kit.



Bullet points, incomplete sentences, and uncommon abbreviations

Do not use bullet points, incomplete sentences, uncommon abbreviations, or Philips' specific terms (unless they have been clearly explained in the given context, or have been mentioned in the existing sales collaterals). Acronyms may be included in short sales texts, provided they are clearly explained in the sales texts.

Points to **avoid** (contd.)



Payment or service related disclosures
Avoid mentioning payment terms, warranty, installation and training conditions or durations.



Configurations and references
Avoid using Philips' internal product configuration/order instructions or product number references.
These details can be specified in the internal ordering instructions field of the product reference.



Special symbols
Do not use special symbols, as they may disturb the formatting of the document. For example, using the inch symbol (“) in place of “inch” should be avoided.

Good sales **text examples**

Features of the product

The IntelliVue Multi Measurement Server X2 functions as a multi parameter module when connected to IntelliVue MX/MP series patient monitor, or as a compact patient monitor when operating standalone. It has a 3.5 inch TFT touch display and customizable screen layouts with numerics, trends and up to 3 waveforms. It provides adjustable alarms for all measurements and arrhythmias, and Philips ST Map (ST changes over time in multi-axis spider diagrams). This device has patient report printing capabilities, ECG sync pulse output, and battery power backup for upto 3 hours with basic monitoring. It is robust, compact in size with an ergonomic design that supports easy loading/unloading from the hospital transport.

This is a good example because:


- It concisely describes the IntelliVue Multi Measurement Server X2.
- It emphasizes on the product features that are of value to the customer.
- It uses correct grammar and spellings.
- The sentences used are complete.

Options

A03 Masimo SET SpO2, ECG (3, 5, 6-lead and derived EASI/Hexad 12-lead with 5/6 electrodes), Respiration and Non-invasive Blood Pressure measurement.

This is a good example because:

- It concisely describes the product.
- It uses correct product spellings.

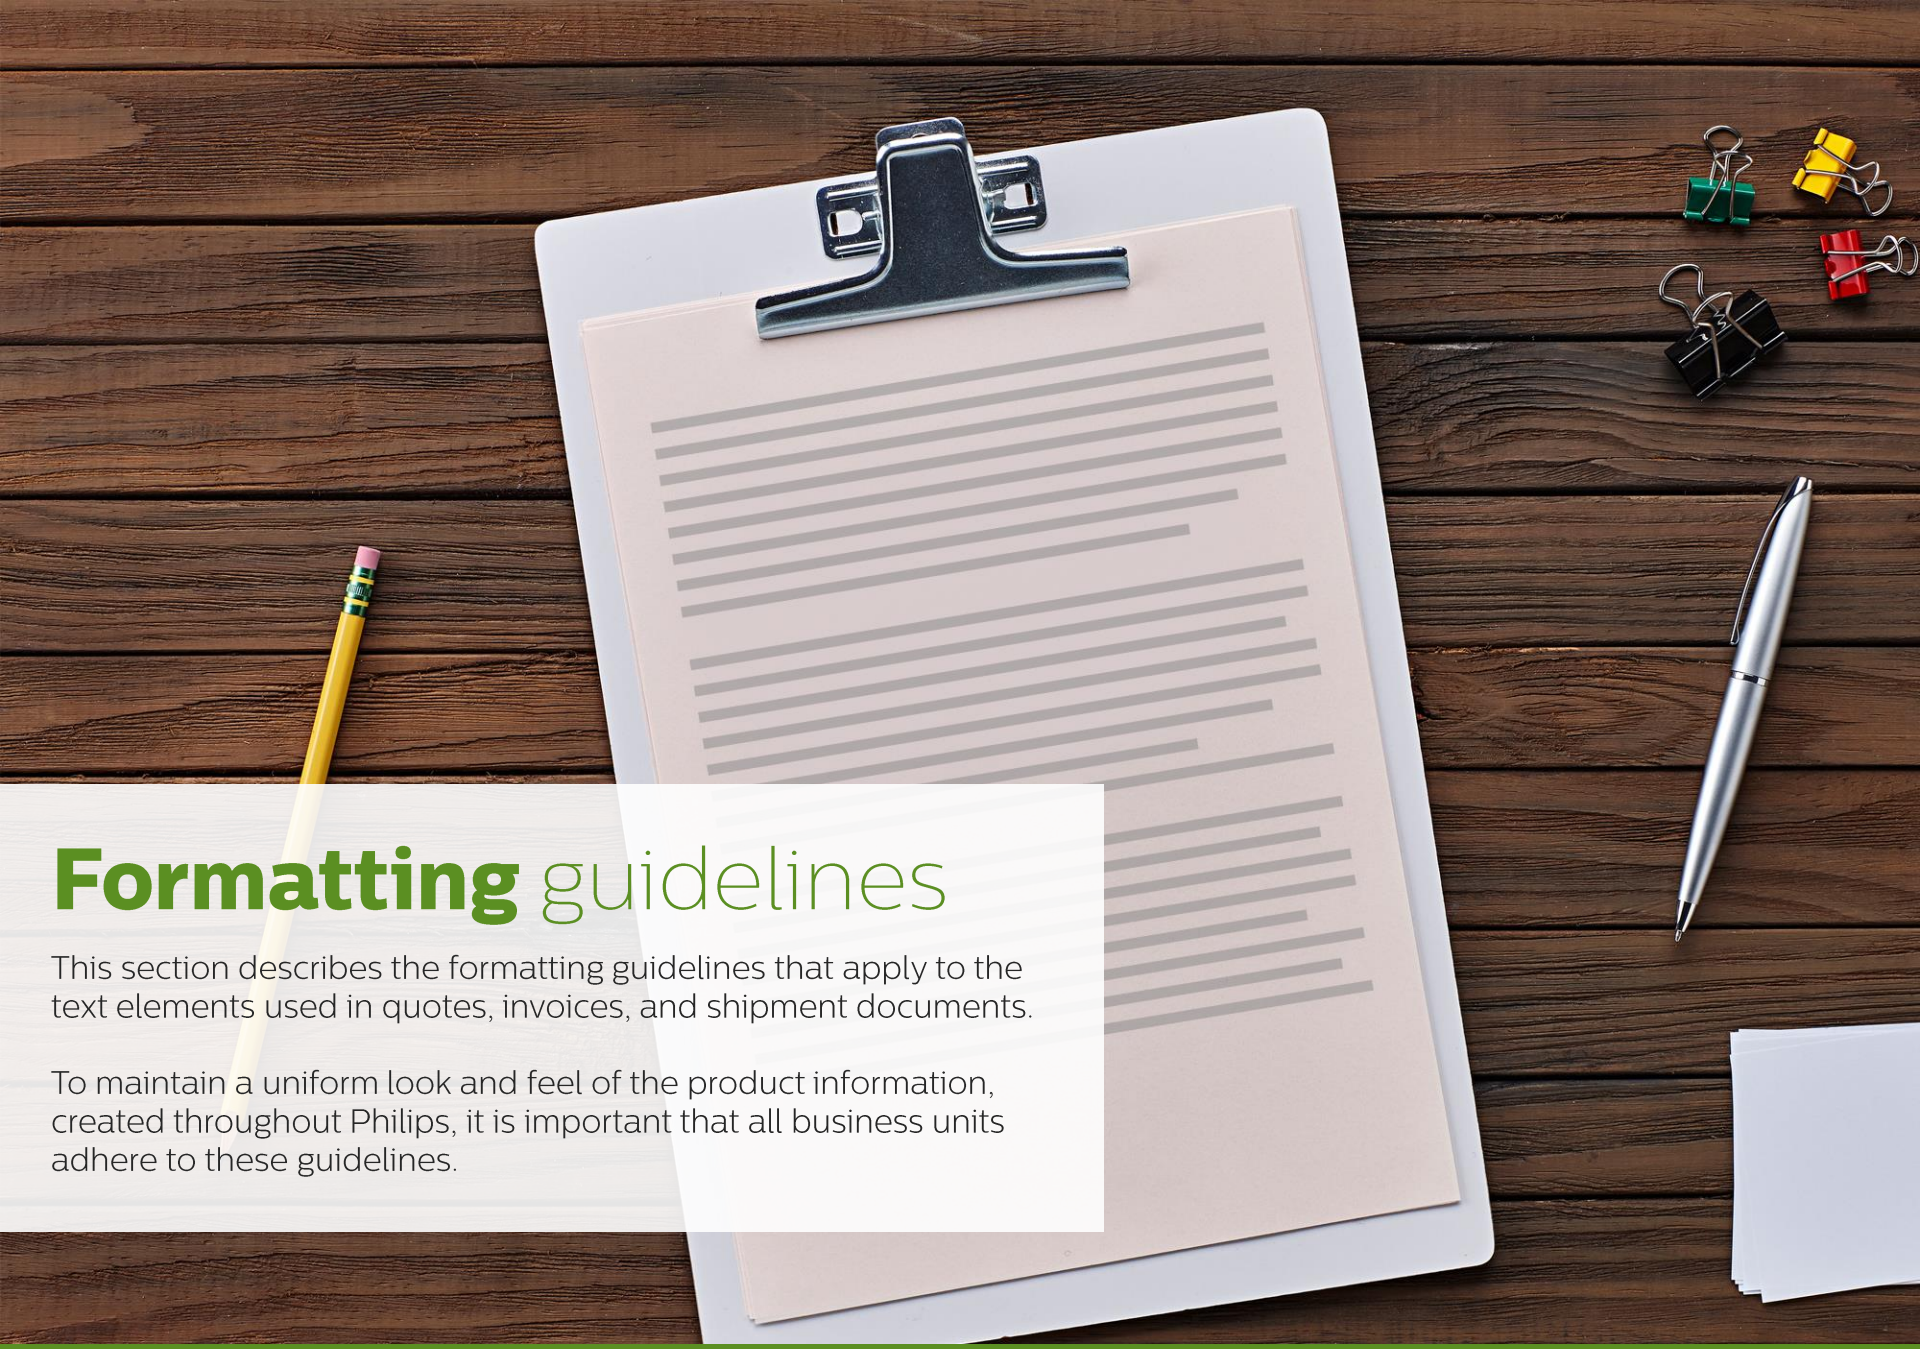

Formatting guidelines

This section describes the formatting guidelines that apply to the text elements used in quotes, invoices, and shipment documents.

To maintain a uniform look and feel of the product information, created throughout Philips, it is important that all business units adhere to these guidelines.

Formatting

Philips uses the following formatting standards in it's quotes, invoices and shipment documents:

Font Type	Calibri
Font Size	11
Font Color	Philips' colors
Italics	Use italics to emphasize words within a text.
Bold text	Bold text is also used for laying emphasis within a text. In addition, it may be used for creating paragraph headings. For example, a paragraph heading may use the "Calibri" font, with font size "11," bold text.
Underline	Use text-underlining for subparagraph headings.

Good example:

"The IntelliVue Multi Measurement Server X2 functions as a multi parameter module when connected to IntelliVue MX/MP series patient monitor or as a compact patient monitor when it operates standalone."

Good because: The font used is "Calibri," and the font size is "11" (which are as per Philips' standards).

Bad example:

"The IntelliVue Multi Measurement Server X2 functions as a multi parameter module when connected to IntelliVue MX/MP series patient monitor or as a compact patient monitor when it operates standalone."

Bad because: The font used is "Times New Roman," and the font size is "12" (which are not as per Philips' standards).

Language

Sales texts at Philips are written in American English, hence the spellings of the words must be as per American English.

The following words, commonly used in sales texts, are often spelled as per British English (which is not a Philips' standard):

American English (Philips' standard)	British English (Not Philips' standard)
Analog	Analogue
Catalog	Catalogue
Meter	Metre
Centimeter	Centimetre
Localization	Localisation
Color	Colour

Good example:

"H07 Supplies Kit for ICU with 5-lead ECG lead set (IEC **color** coding) and trunk cable, SpO2 Adult Sensor, NIBP Adult Cuff and Hose.."

Good because: "Color" has been spelled as per American English.

Bad example:

"H07 Supplies Kit for ICU with 5-lead ECG lead set (IEC **colour** coding) and trunk cable, SpO2 Adult Sensor, NIBP Adult Cuff and Hose."

Bad because: "Colour" has been spelled as per British English.

Product **names**

Product names at Philips are legal, registered trade names, and must be written in the official way. While writing the product names, use correct capitalization, spellings, and spaces.

The following product names are commonly used in sales texts, but are often used incorrectly:

Correct usage	Incorrect usage
IntelliVue	Intelliview
SureSigns	Sure Signs
Avalon	AVALON
PageWriter	Pagewriter

The complete list of product names can be found on Philips' intranet site at http://pww.apps.anr.ms.philips.com/namingrequestsite/nrs/trademark.htm

Good example:

"**IntelliVue** Multi Measurement Server X2"

Good because: "IntelliVue," which is product name, has been written in the official way.

Bad example:

"**IntelliView** Multi Measurement Server X2"

Bad because: "IntelliView," which is a product name, has not been written in the official way.

Capital **letters**

While writing sales texts at Philips, use capital letters only in the following cases:

At the start of a sentence.
As required for trademarked feature names. For example: SKYLight, Xcelera.
For acronyms. For example: LCD, TFT.
For proper use of units of measurement. For Example: Hz, W, V.

Good example:

"It has a 3.5 inch **TFT** touch display and customizable screen layouts with numerics, trends and up to 3 waveforms. It provides adjustable alarms for all measurements and arrhythmias, and Philips **ST** Map."

Good because: "TFT" and "ST," being acronyms, have been written in capital letters.

Bad example:

"It has a 3.5 inch **tft** touch display and customizable screen layouts with numerics, trends and up to 3 waveforms. It provides adjustable alarms for all measurements and arrhythmias, and Philips **st** Map."

Bad because: "tft" and "st," though acronyms, have not been written in capital letters.

Spacing

While writing sales texts at Philips, use only one space after a word, comma, period, or any other punctuation mark except for the “slash.”

The slash (as a replacement of “or”), is used to separate two possible options within a sentence.

Do not use a space after a slash, unless one or both of the options consist of more than one word. The following examples show the correct usage of space with the slash:

His/her (each of these are one-word options, hence no space is required after the slash).
Products/ product accessories (as “product accessories” is a two-word option, a space is required after the slash).
Product accessories/ products (as “product accessories” is a two-word option, a space is required after the slash).
Product accessories/ optional products (as both “product accessories” and “optional products” are two-word options, a space is required after the slash).

✓ Good example:

“The IntelliVue Multi Measurement Server X2 functions as a multi parameter module when connected to IntelliVue **MX/MP** series patient monitor or as a compact patient monitor when it operates standalone. ”

Good because: Both “MX” and “MP” are one-word options, hence no space is required after the slash.

✗ Bad example:

“The IntelliVue Multi Measurement Server X2 functions as a multi parameter module when connected to IntelliVue **MX/ MP** series patient monitor or as a compact patient monitor when it operates standalone. ”

Bad because: Although both “MX” and “MP” are one-word options, a space has been provided after the slash.

Hyphens

While writing sales texts at Philips, use hyphens only between words that collectively represent an idea or item.

The following situations show where hyphens can be applied effectively:

For numerical fractions written as text.
For example: two-thirds, three-fourths.

For most words that begin with “anti,” “non,” and “euro.”
For example: anti-radiation coating, non-compliance document, Euro-American venture.

To avoid ambiguities while describing the subject.
For example: a little-used car/ a little used-car.

For separating identical letters within a word.
For example: co-operate.

For nouns formed from prepositional verbs.
For example: pay-off, set-up.

Good example:

“A03 Masimo SET SpO2, ECG (3, 5, **6-lead** and derived EASI/Hexad 12-lead with 5/6 electrodes), Respiration and Non-invasive Blood Pressure measurement.”

Good because: As “6” and “lead” are collectively describing the ECG, they are written with a hyphen between them.

Bad example:

“A03 Masimo SET SpO2, ECG (3, 5, **6 lead** and derived EASI/Hexad 12-lead with 5/6 electrodes), Respiration and Non-invasive Blood Pressure measurement.”

Bad because: Although “6” and “lead” are collectively describing the ECG, they are written without a hyphen between them.

Units of **measurement**

While writing sales texts at Philips, symbols and units of measurement should be written in the following manner:

Use both units of measurement i.e., the metric system (cm/kg/etc.) and the US units of measurement (inch/lbs/etc.).

Do not add a period after a unit symbol unless it is the last word of the sentence.

Do not start the unit symbol with a capital letter (uppercase) unless it has been derived from a proper noun.

Use a space to separate the magnitude (number) from the unit symbol. For example: 2.2 kg, 40 inch.

Additional information about the units of measurement is available at
http://www.bipm.org/en/si/si_brochure/

Good example:

"It has a **3.5 inch (8.9 cm)** TFT touch display and customizable screen layouts with numerics, trends and up to 3 waveforms."

Good because: The units of measurement are given in both the metric as well as the US systems. Moreover, the unit symbol "inch" does not start with a capital letter, and there is a space between "3.5" and "inch."

Bad example:

"It has a **3.5Inch** TFT touch display and customizable screen layouts with numerics, trends and up to 3 waveforms."

Bad because: Only the US units of measurement have been used. Also the first letter in the unit symbol "inch" is a capital letter, and there is no space between "3.5" and "inch."

Numbering

While writing numbers in the sales texts, use the dot (.) to separate the integer from the decimal part of the number.

For numbers that have more than four digits, add a comma after every third digit, when counted from the right.

The usage of the dot and the comma in numbers is illustrated below:

15.52 (The integer “15” has been separated from the decimal part “52” by a dot).
15 (As “15” is an integer, no dot is required here).
1500 (As “1500” does not have more than four digits, no comma is required).
15,000 (As “15,000” consists of more than four digits, a comma is required after the third digit from the right).
150,000,000 (As “150,000,000” consist of more than four digits, a comma is required after every third digit from the right).

Good example:

“Trend database stores a maximum of **16** measurement numerics for up to **1.5** hours.”

Good because: “16” is an integer, and has been correctly represented without a dot, and in “1.5” the dot has effectively separated the integer from the decimal part.

Bad example:

“Trend database stores a maximum of **16.0** measurement numerics for up to 1.5 hours. ”

Bad because: “16,” which is an integer, has been incorrectly represented with a decimal part.

Acronyms and **abbreviations**

As acronyms and abbreviations are frequently misunderstood by the customer, consider the following points while including them in the sales texts:

Ensure that the correct acronyms and abbreviations are included in the sales texts.

For including Philips' specific acronyms within sales texts, ensure that descriptions/definitions for those acronyms have been included.

Good example:

"J35 Wireless **LAN** connectivity enables IntelliVue Multi Measurement Server X2 to wirelessly communicate with IntelliVue monitoring network through industry standard **WLAN** 802.11a/b/g network."

Good because: This sales text uses commonly known acronyms and does not use any Philips' specific acronyms.

Bad example:

"J35 Wireless LAN connectivity enables IntelliVue **MMS** X2 to wirelessly communicate with IntelliVue monitoring network through industry standard WLAN 802.11a/b/g network."

Bad because: This sales text uses a Philips' specific acronym "MMS" which has not been defined/described in the sales text.

General **considerations**

In addition to the guidelines already mentioned, also consider the following points:

Avoid using personal pronouns	For example: Use “the customer,” or “the patient,” instead of “he” or “she.”
Avoid using colloquial terms, complicated words, clichés and jargon	For example: • Use “microphone” instead of “mike.” • Use “use” instead of “utilize.” • Use “free software” instead of “freeware.” • Use “LCD/LED monitor” instead of “flat screen/monitor.” • Use “CRT monitor” instead of “monitor/screen.”
Use the accepted date notation	The YYYY-MM-DD format is accepted at Philips, and the MM-DD-YYYY format is not accepted at Philips.

Good example:

“**Using** the Masimo technology, the **patient’s** oxygen status on **2018-03-18** was… ”

Good because: This sales text avoids the use of personal pronouns and colloquial terms/ complicated words. Moreover, the date is in a format that is accepted at Philips.

Bad example:

“**Utilizing** the Masimo technology, **her** oxygen status on **03-18-2018** was… ”

Bad because: This sales text uses a personal pronoun “her,” a complicated word “utilize,” and a date format which is not accepted at Philips.


PHILIPS