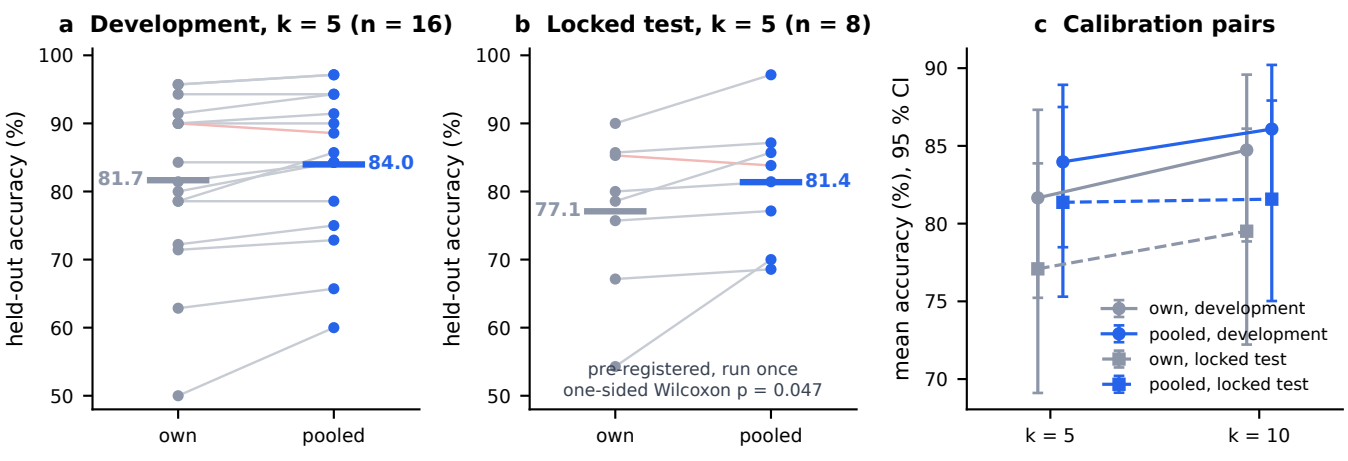
a Development, k = 5 (n = 16)
b Locked test, k = 5 (n = 8)
c Calibration pairs
held-out accuracy (%)
mean accuracy (%), 95 % CI
81.7
84.0
77.1
81.4
pre-registered, run once
one-sided Wilcoxon p = 0.047
own
pooled
k = 5
k = 10
own, development
pooled, development
own, locked test
pooled, locked test