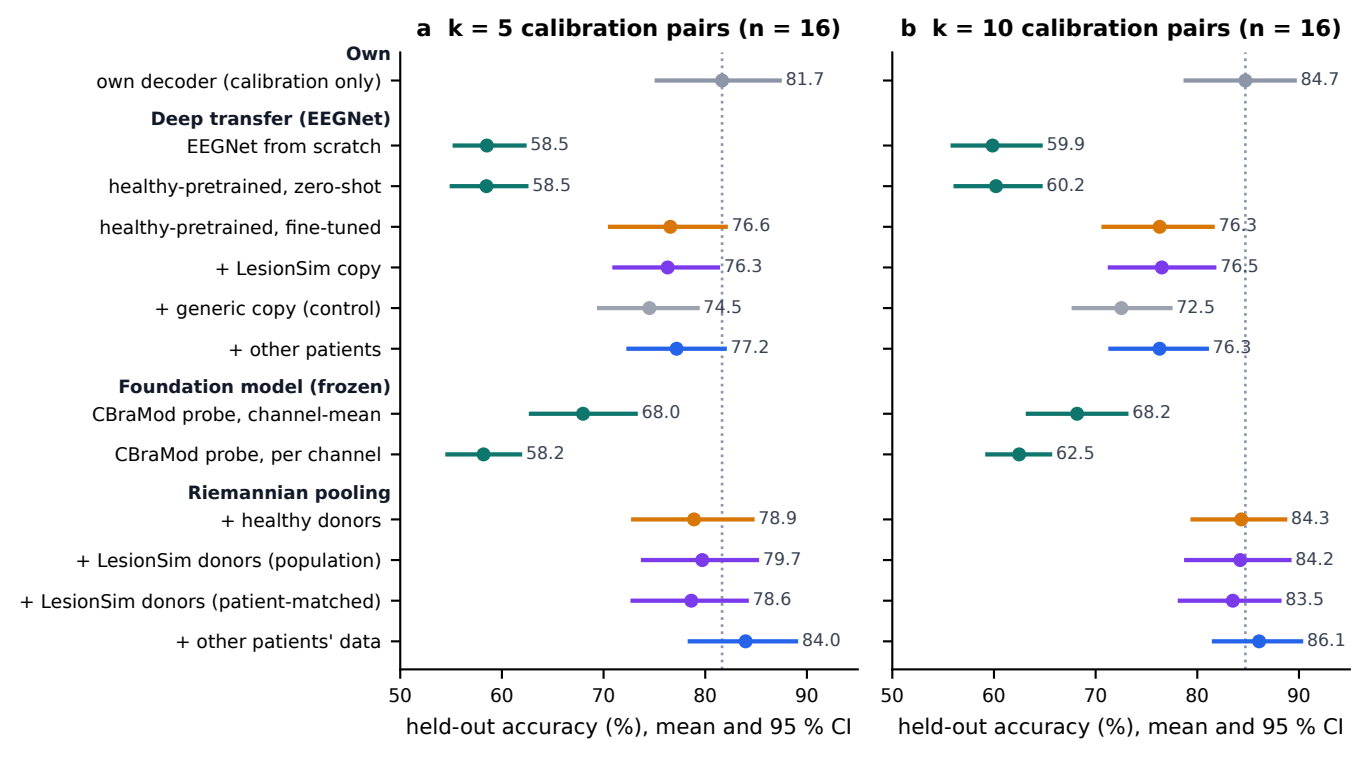
a k = 5 calibration pairs (n = 16)
b k = 10 calibration pairs (n = 16)
Own
own decoder (calibration only)
81.7
84.7
Deep transfer (EEGNet)
EEGNet from scratch
58.5
59.9
healthy-pretrained, zero-shot
58.5
60.2
healthy-pretrained, fine-tuned
76.6
76.3
+ LesionSim copy
76.3
76.5
+ generic copy (control)
74.5
72.5
+ other patients
77.2
76.3
Foundation model (frozen)
CBraMod probe, channel-mean
68.0
68.2
CBraMod probe, per channel
58.2
62.5
Riemannian pooling
+ healthy donors
78.9
84.3
+ LesionSim donors (population)
79.7
84.2
+ LesionSim donors (patient-matched)
78.6
83.5
+ other patients' data
84.0
86.1
50
60
70
80
90
held-out accuracy (%), mean and 95 % CI