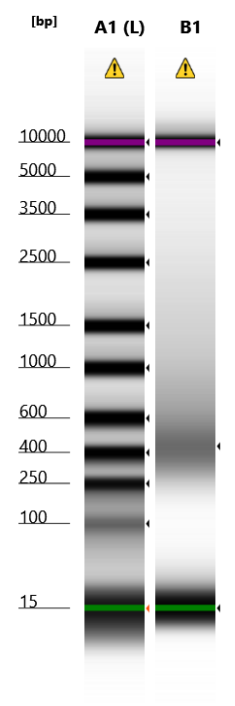


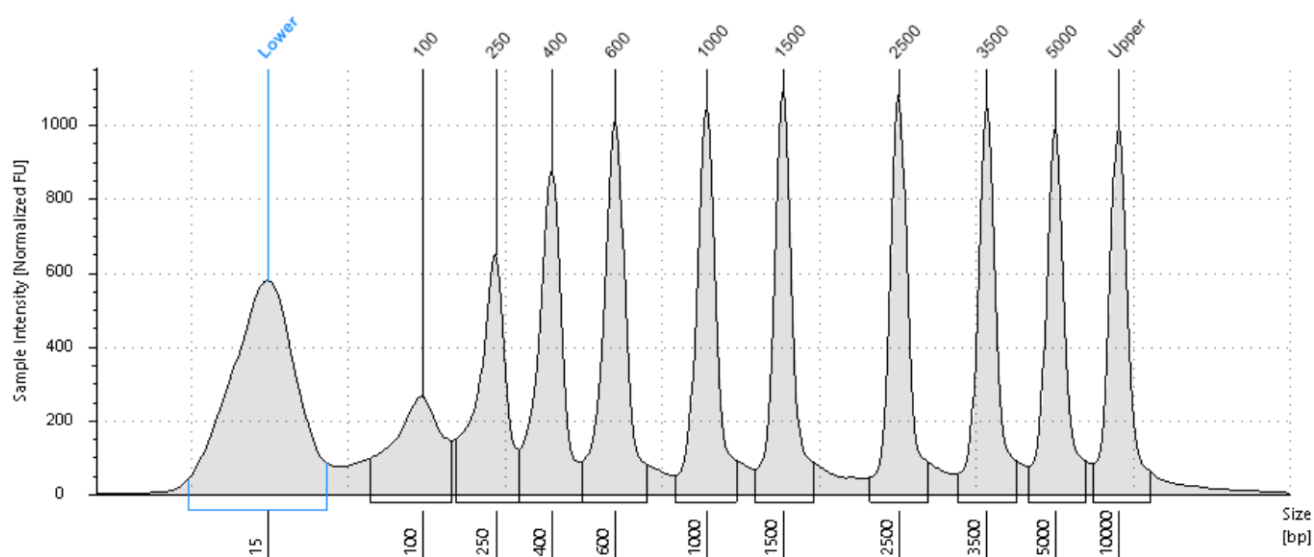
Filename: 2023-02-01 - 13.31.56.HSD5000



Default image (Contrast 100%)

Sample Info

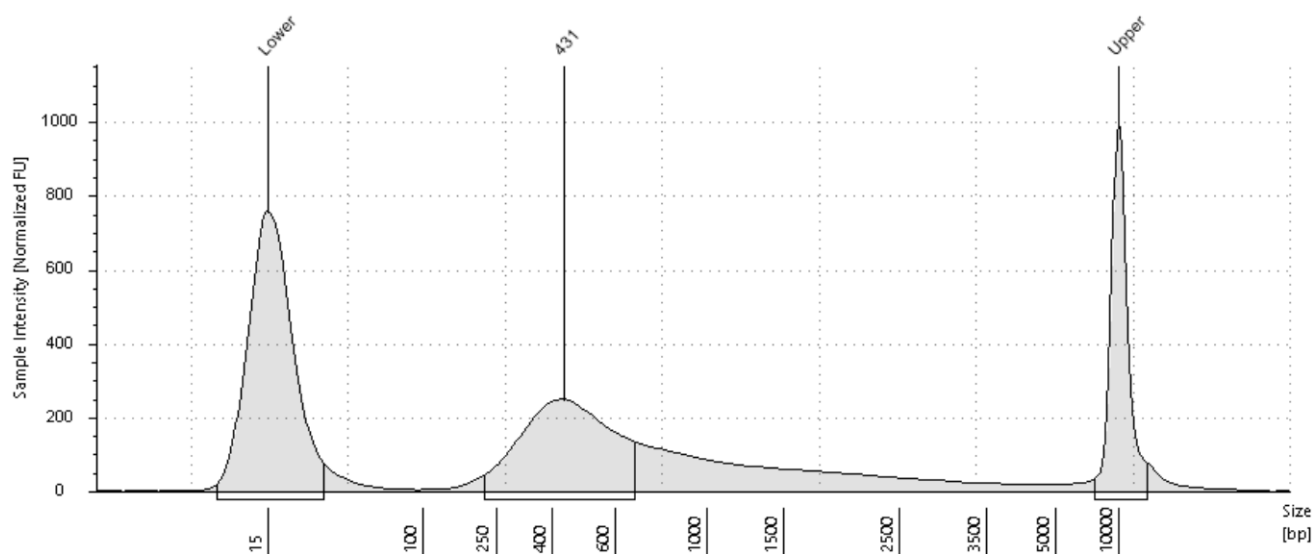
Well	Conc. [pg/ul]	Sample Description	Alert	Observations
A1	2080	Ladder		Caution! Expired ScreenTape device; Ladder
B1	295	Final LIB_01.02.23		Caution! Expired ScreenTape device

A1: Ladder**Sample Table**

Well	Conc. [pg/ul]	Sample Description	Alert	Observations
A1	2080	Ladder		Caution! Expired ScreenTape device; Ladder

Peak Table

Size [bp]	Calibrated Conc. [pg/ul]	Assigned Conc. [pg/ul]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
15	350	-	35900	-		Lower Marker
100	152	-	2340	7.31		
250	213	-	1310	10.24		
400	244	-	940	11.74		
600	269	-	690	12.92		
1000	253	-	389	12.15		
1500	247	-	254	11.88		
2500	235	-	145	11.31		
3500	238	-	105	11.43		
5000	229	-	70.6	11.02		
10000	180	180	27.7	-		Upper Marker

B1: Final LIB_01.02.23**Sample Table**

Well	Conc. [pg/ul]	Sample Description	Alert	Observations
B1	295	Final LIB_01.02.23		Caution! Expired ScreenTape device

Peak Table

Size [bp]	Calibrated Conc. [pg/ul]	Assigned Conc. [pg/ul]	Peak Molarity [pmol/l]	% Integrated Area	Peak Comment	Observations
15	384	-	39400	-		Lower Marker
431	295	-	1050	100.00		
10000	180	180	27.7	-		Upper Marker