

NOTES

Tanit Medical Engineering does not take responsibility for any damages resulting from changes on drawings made by others. Errors may occur by not referring to the complete set of final issue drawing.

Tanit Medical Engineering cannot accept responsibility for any damage due to the partial use of final issue drawings, however caused.

All dimensions are in millimeters unless otherwise specified. Do not scale from printed pdf files.

Tanit Medical Engineering accepts no responsibility or liability for defective work due to scaling from these drawings.

LEGEND

- 1. FOR SYMBOLS, LEGEND AND GENERAL NOTES, REFER TO DWG # E-001.
- 2. FOR GENERAL ELECTRICAL DETAILS, REFER TO DWG # E-501 AND E-502.
- 3. ALL EMERGENCY AND EXIT LIGHTING ARE WIRED ON NON SWITCHED CIRCUIT TO THE PANEL BOARD IN THE RESPECTIVE ZONE.

REV	MODIFICATIONS	DATE
00	ISSUED FOR APPROVAL	31/12/2023
01	REVISED BASED ON GE COMMENTS	13/01/2024
02	REVISED BASED ON GE COMMENTS	08/02/2024

CONTRACTOR:
FOMEX Ltd.

TANIT
MEDICAL ENGINEERING

TANIT MEDICAL ENGINEERING
9 Ade Adedeji Close,
Lekki Phase 1 Lagos, Nigeria
TEL: +234 803 525 1436
Email: info@tanitgroup.com
www.tanitgroup.com

Distribution and Storage of Pharmaceuticals Equipment Contracting
Building and Medical Infrastructure Project Development Advisory

PROJECT TITLE:
STELLA OBASANJO HOSPITAL

CLIENT:
BMC Ltd.

SHEET TITLE:
**Ground Floor Plan
GE EQUIPMENT LAYOUT**

Revision: 02



Scale: 1/150

Drawn by: A.H Date: 08/02/2024

Checked by: A.H Date: 08/02/2024


Approved by: I.K Date: 08/02/2024

PROJECT NO:
20/SOH-01 SHEET NO:
GE-100

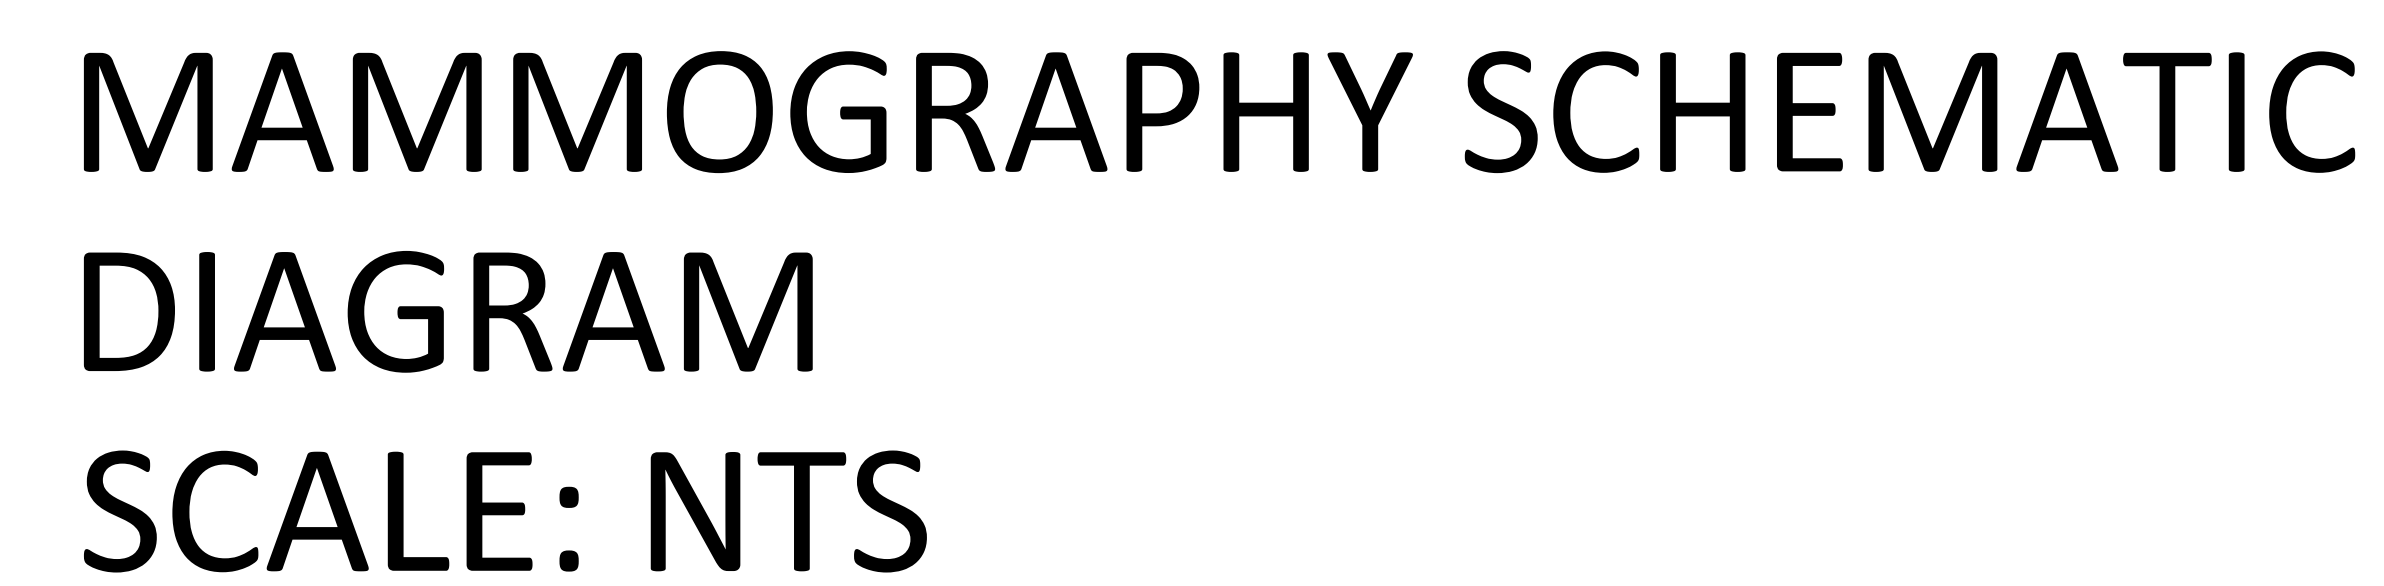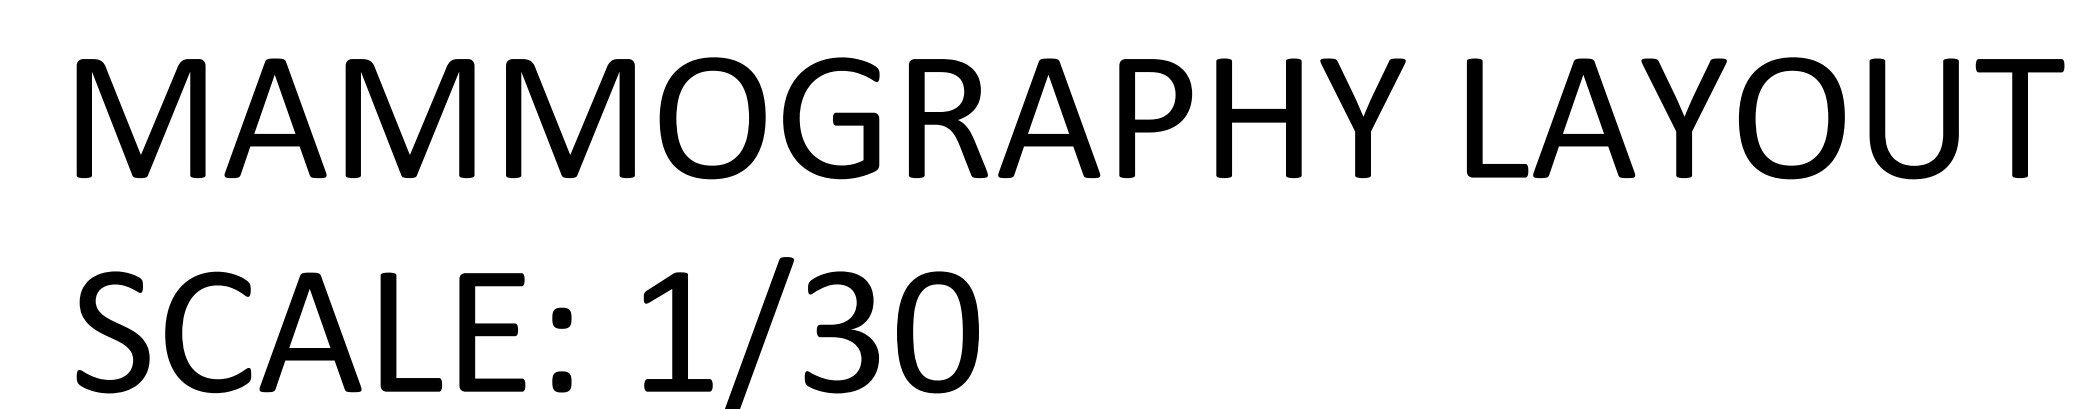


PROJECT NO: 20/SOH-01	SHEET NO: GF-101
--------------------------	----------------------------

SHEET NO:
GE-101

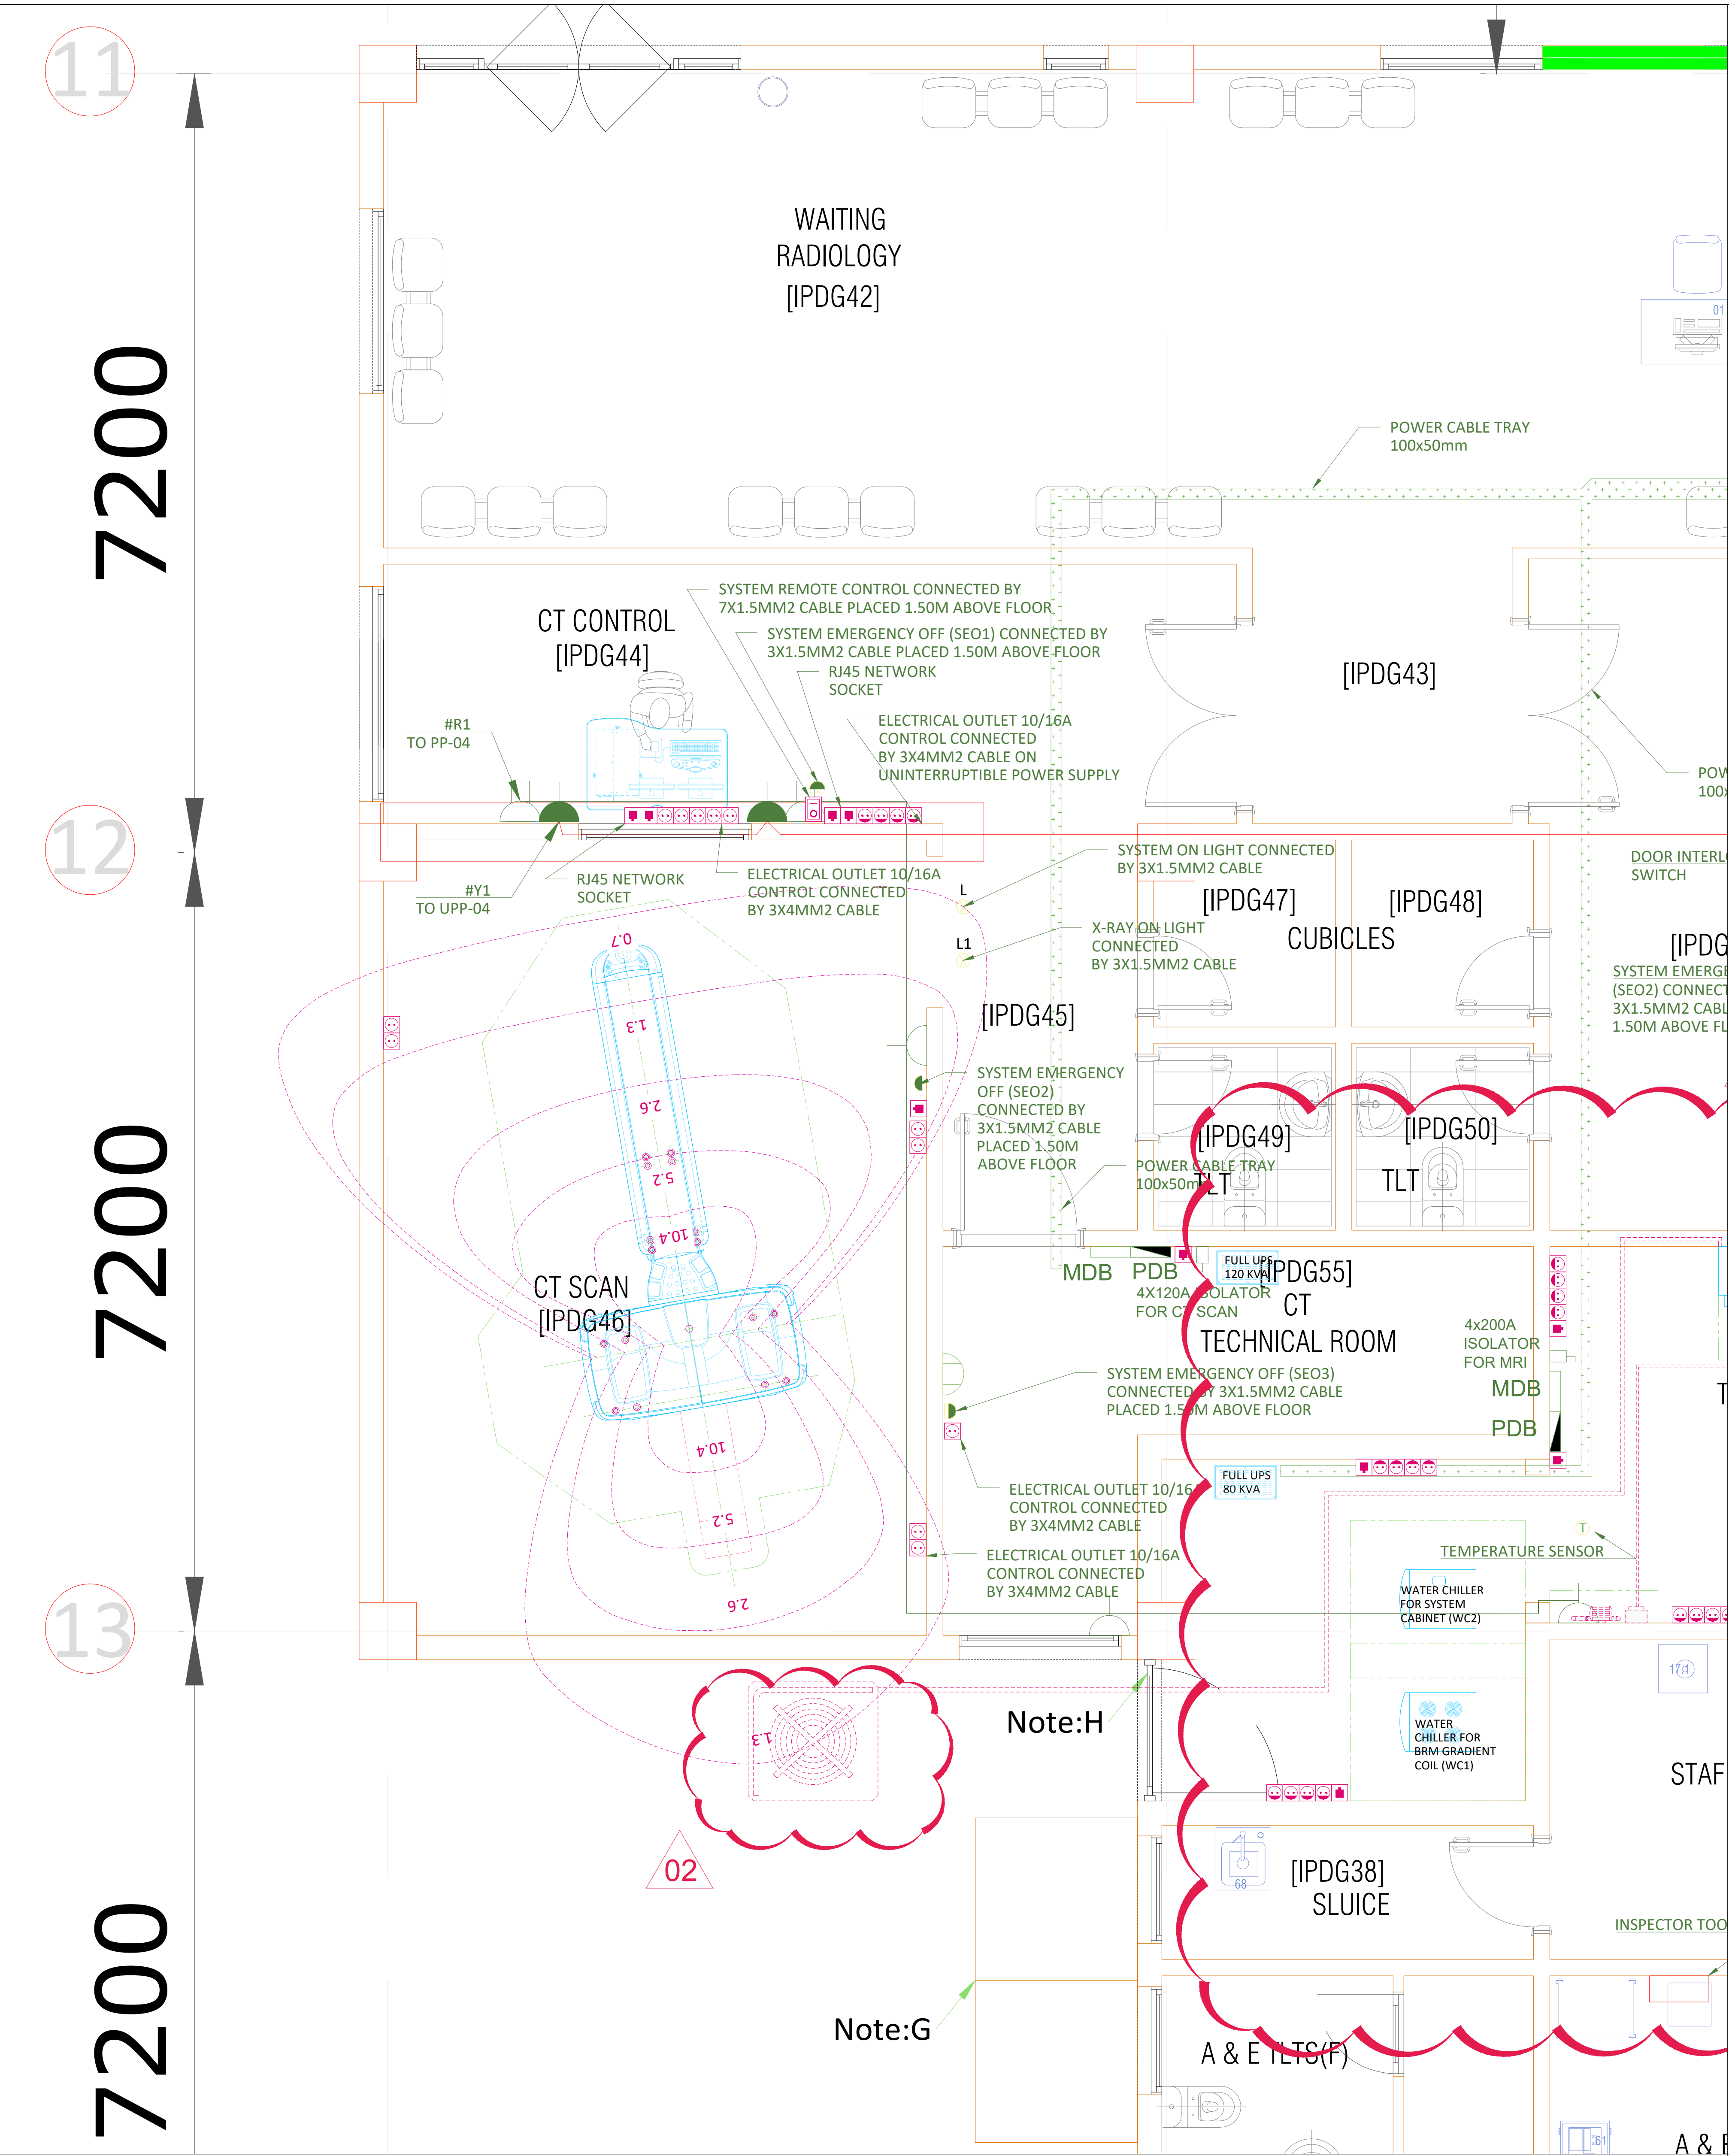

CT SCANNER LAYOUT
SCALE: 1/30

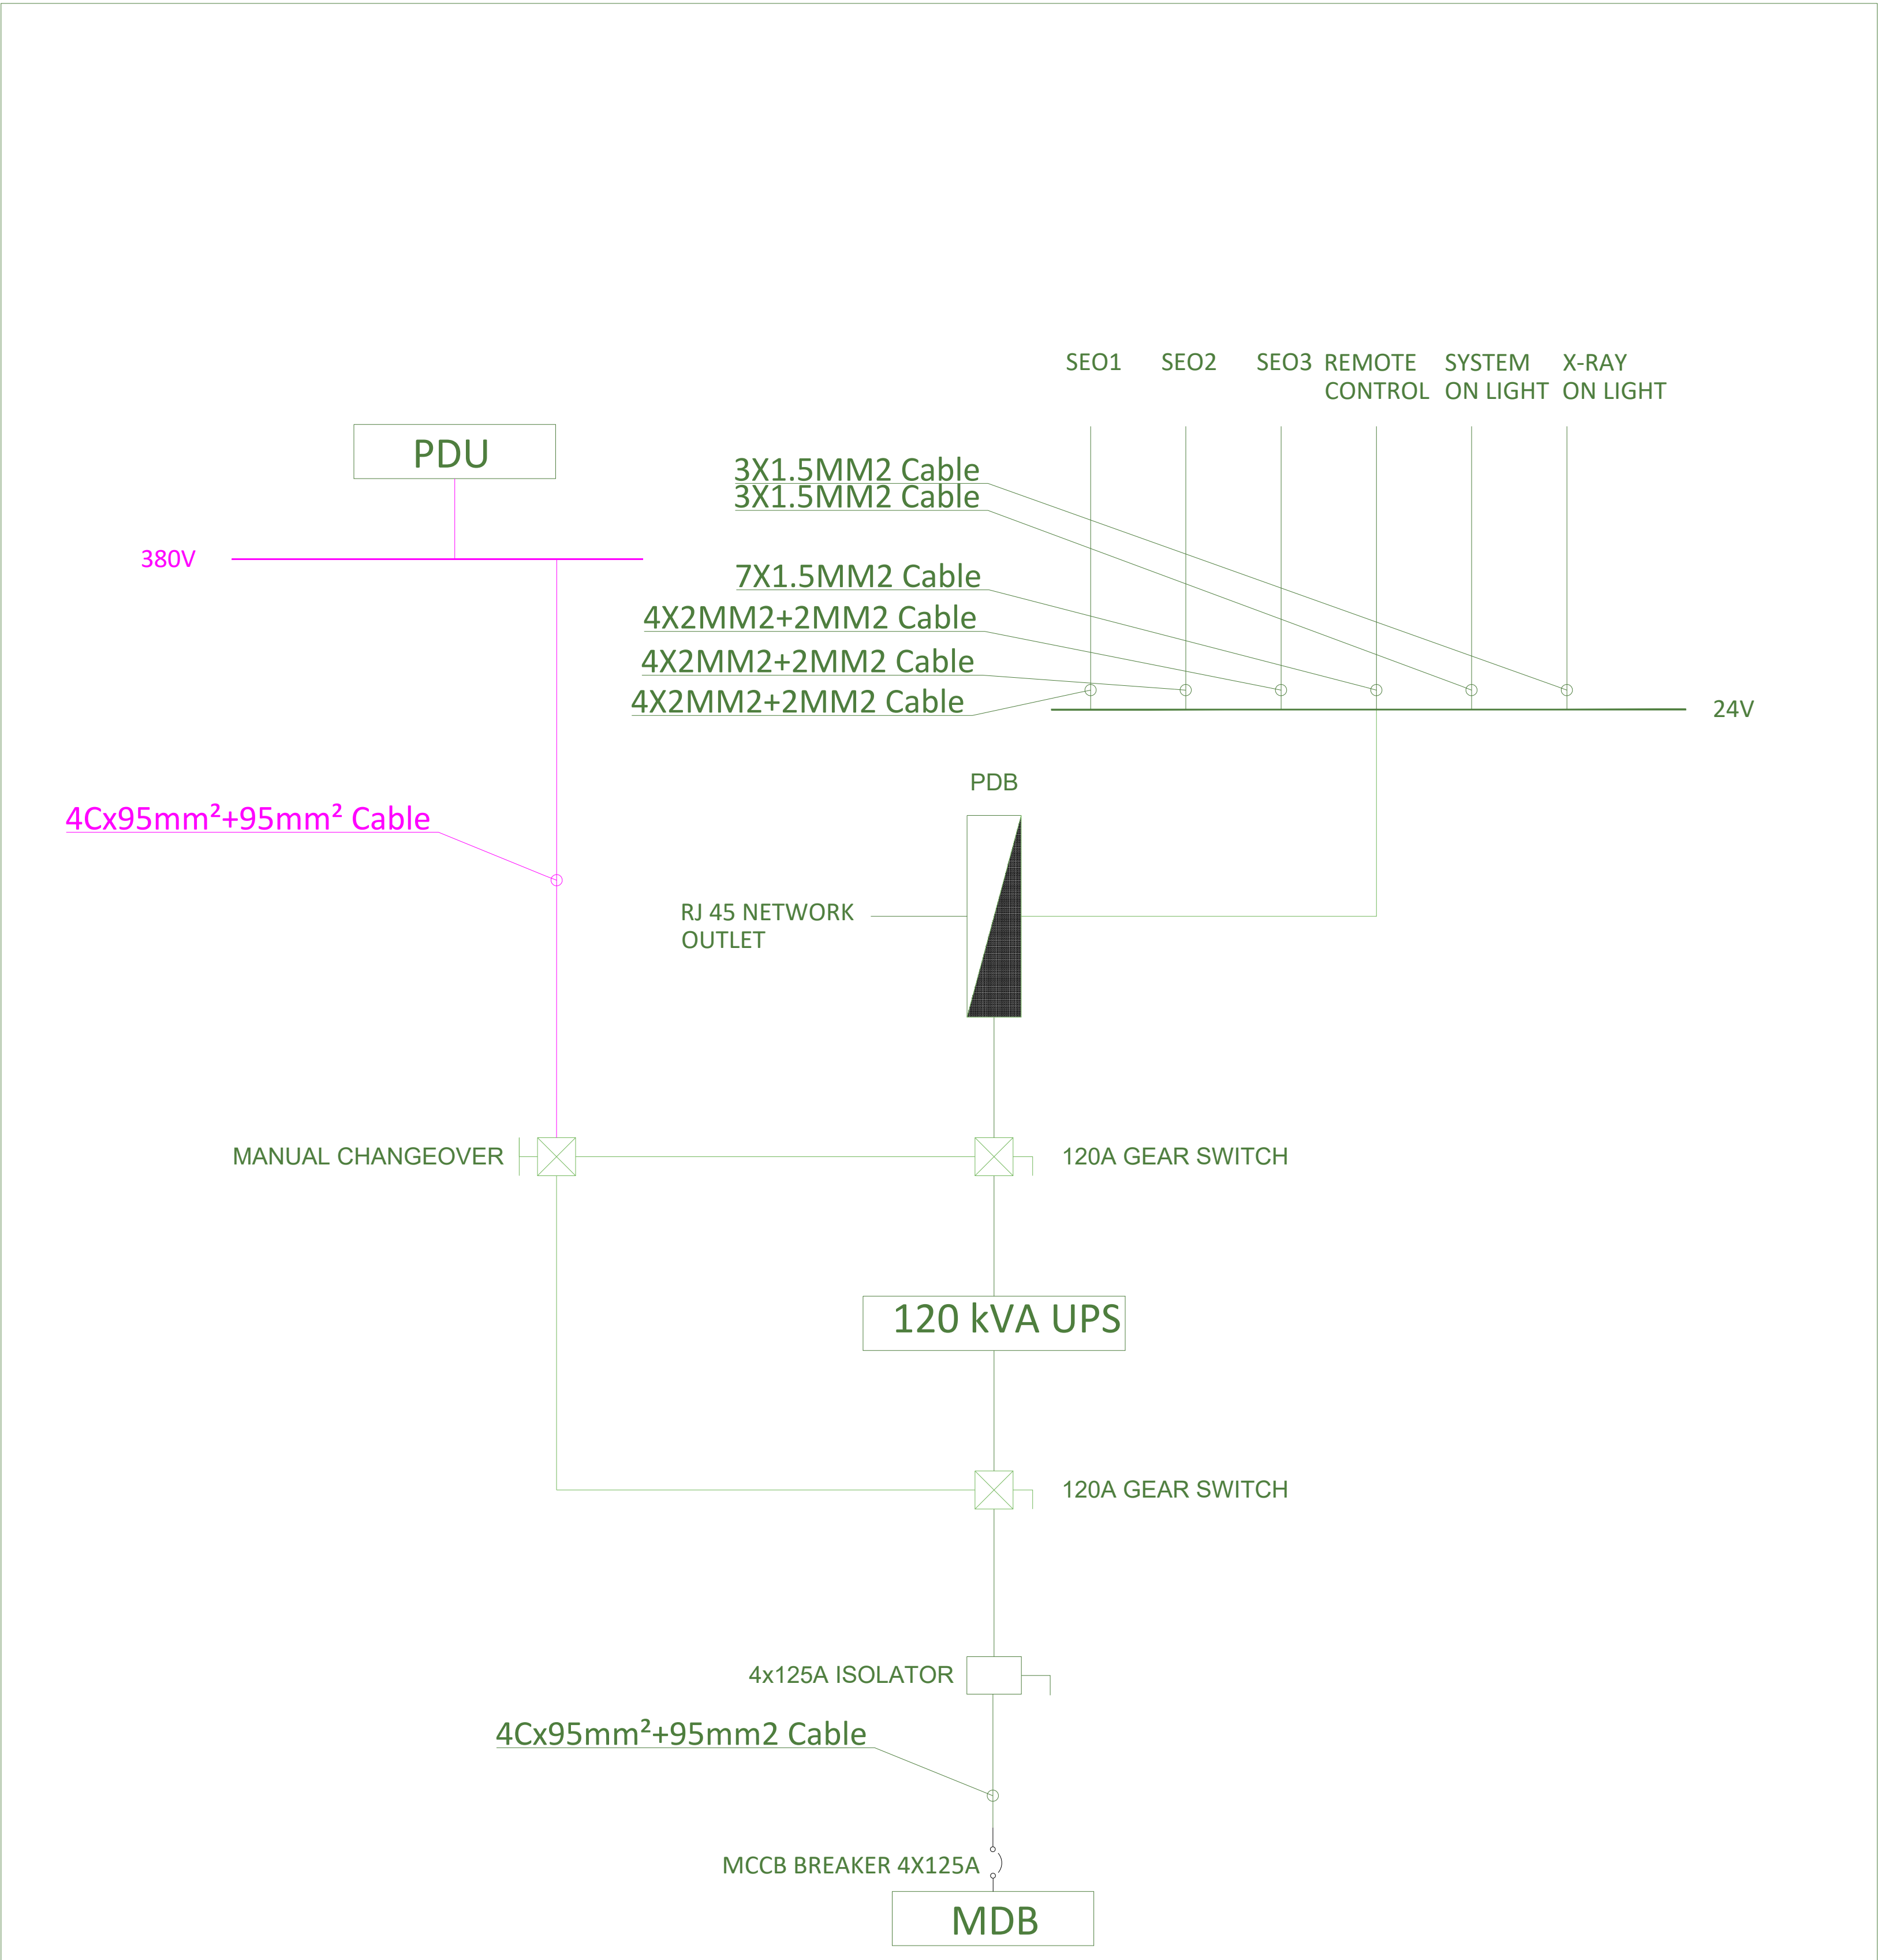

CT SCANNER SCHEMATIC
DIAGRAM
SCALE: NTS

NOTES

Tanit Medical Engineering does not take responsibility for any damages resulting from changes on drawings made by others. Errors may occur by not referring to the complete set of final issue drawing.

Tanit Medical Engineering cannot accept responsibility for any damage due to the partial use of final issue drawings, however caused.

All dimensions are in millimeters unless otherwise specified. Do not scale from printed pdf files.

Tanit Medical Engineering accepts no responsibility or liability for defective work due to scaling from these drawings.

LEGEND

1. FOR SYMBOLS, LEGEND AND GENERAL NOTES, REFER TO DWG # E-001.

2. FOR GENERAL ELECTRICAL DETAILS, REFER TO DWG # E-501 AND E-502.

3. ALL EMERGENCY AND EXIT LIGHTING ARE WIRED ON NON SWITCHED CIRCUIT TO THE PANEL BOARD IN THE RESPECTIVE ZONE.

REV	MODIFICATIONS	DATE
00	ISSUED FOR APPROVAL	31/12/2023
01	REVISED BASED ON GE COMMENTS	13/01/2024
02	REVISED BASED ON GE COMMENTS	08/02/2024

CONTRACTOR:

FOMEX Ltd.

TANIT

TANIT MEDICAL ENGINEERING

9 Ade Adedeji Close,
Lekki Phase 1 Lagos, Nigeria
TEL: +234 803 525 1436
Email: info@tanitgroup.com
www.tanitgroup.com

Distribution and Storage of Pharmaceuticals
Building and Medical Infrastructure

Equipment Contracting
Project Development Advisory

PROJECT TITLE:

STELLA OBASANJO HOSPITAL

CLIENT:

BMC Ltd.

SHEET TITLE:

Ground Floor Plan
CT SCANNER LAYOUT

Revision: 02

Scale: 1/150

Drawn by: A.H

Date: 08/02/2024

Checked by: A.H



Date: 08/02/2024

Approved by: I.K


Date: 08/02/2024

PROJECT NO:
20/SOH-01


SHEET NO:
GE-102

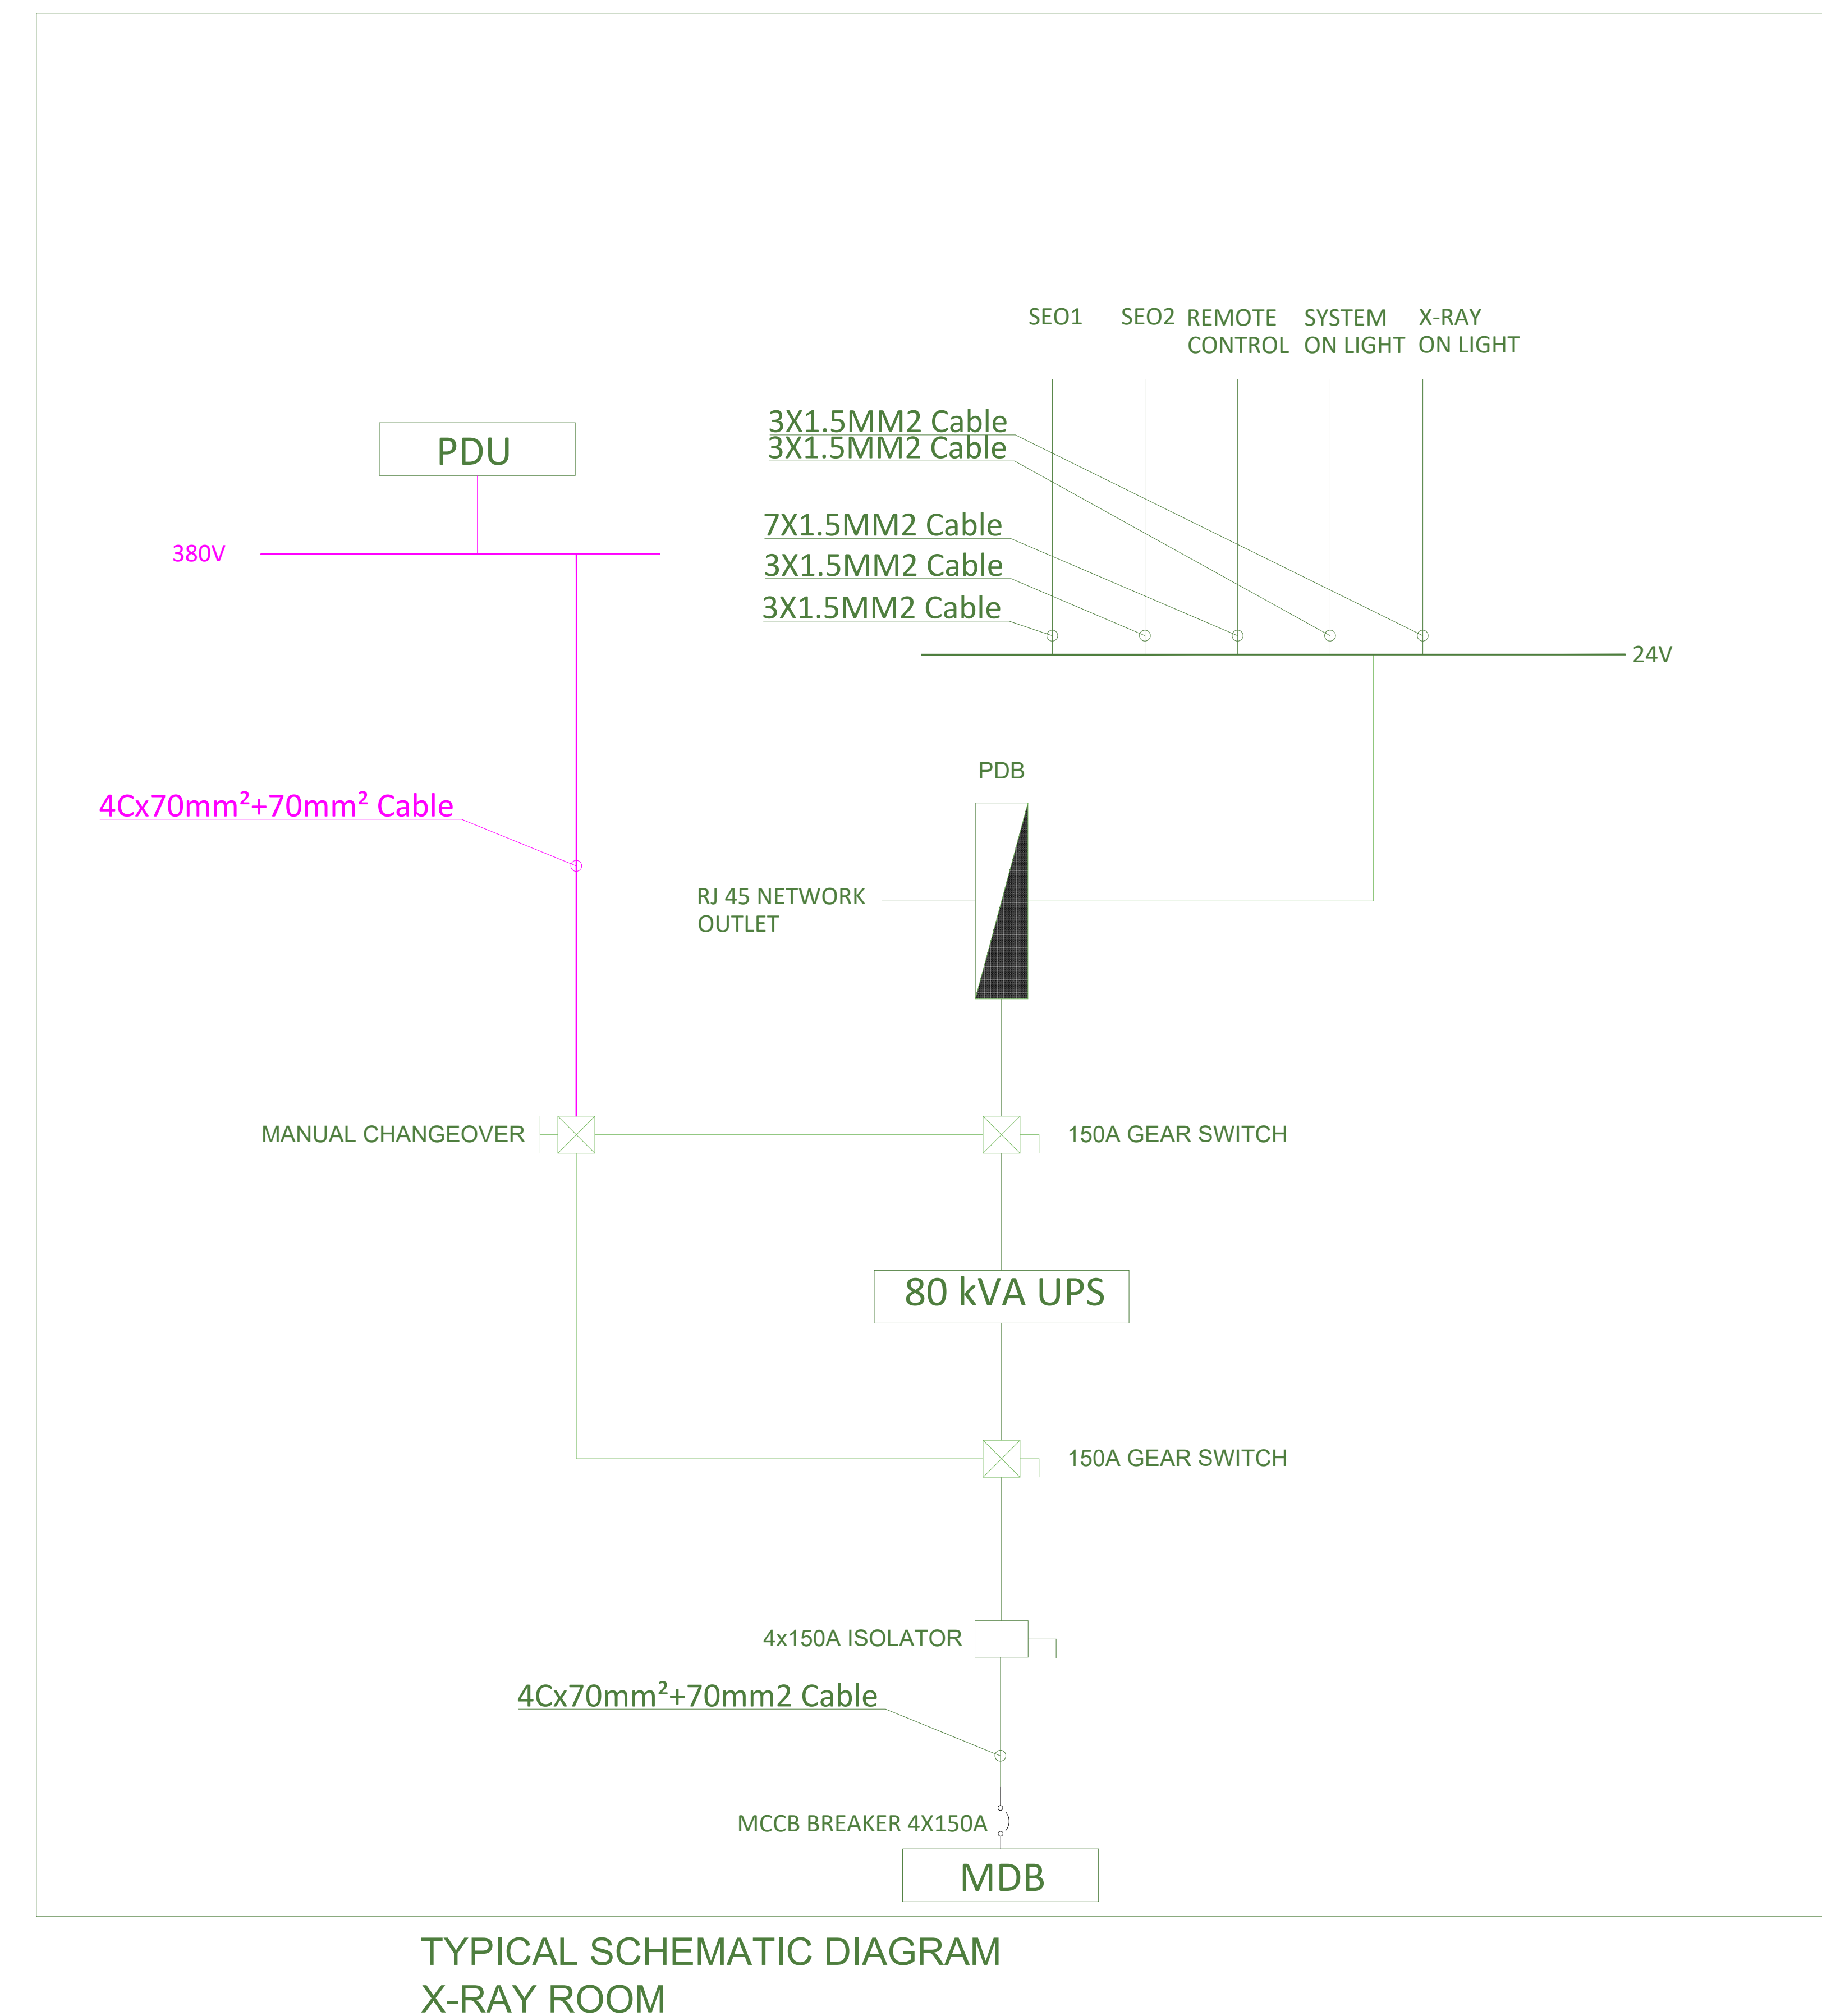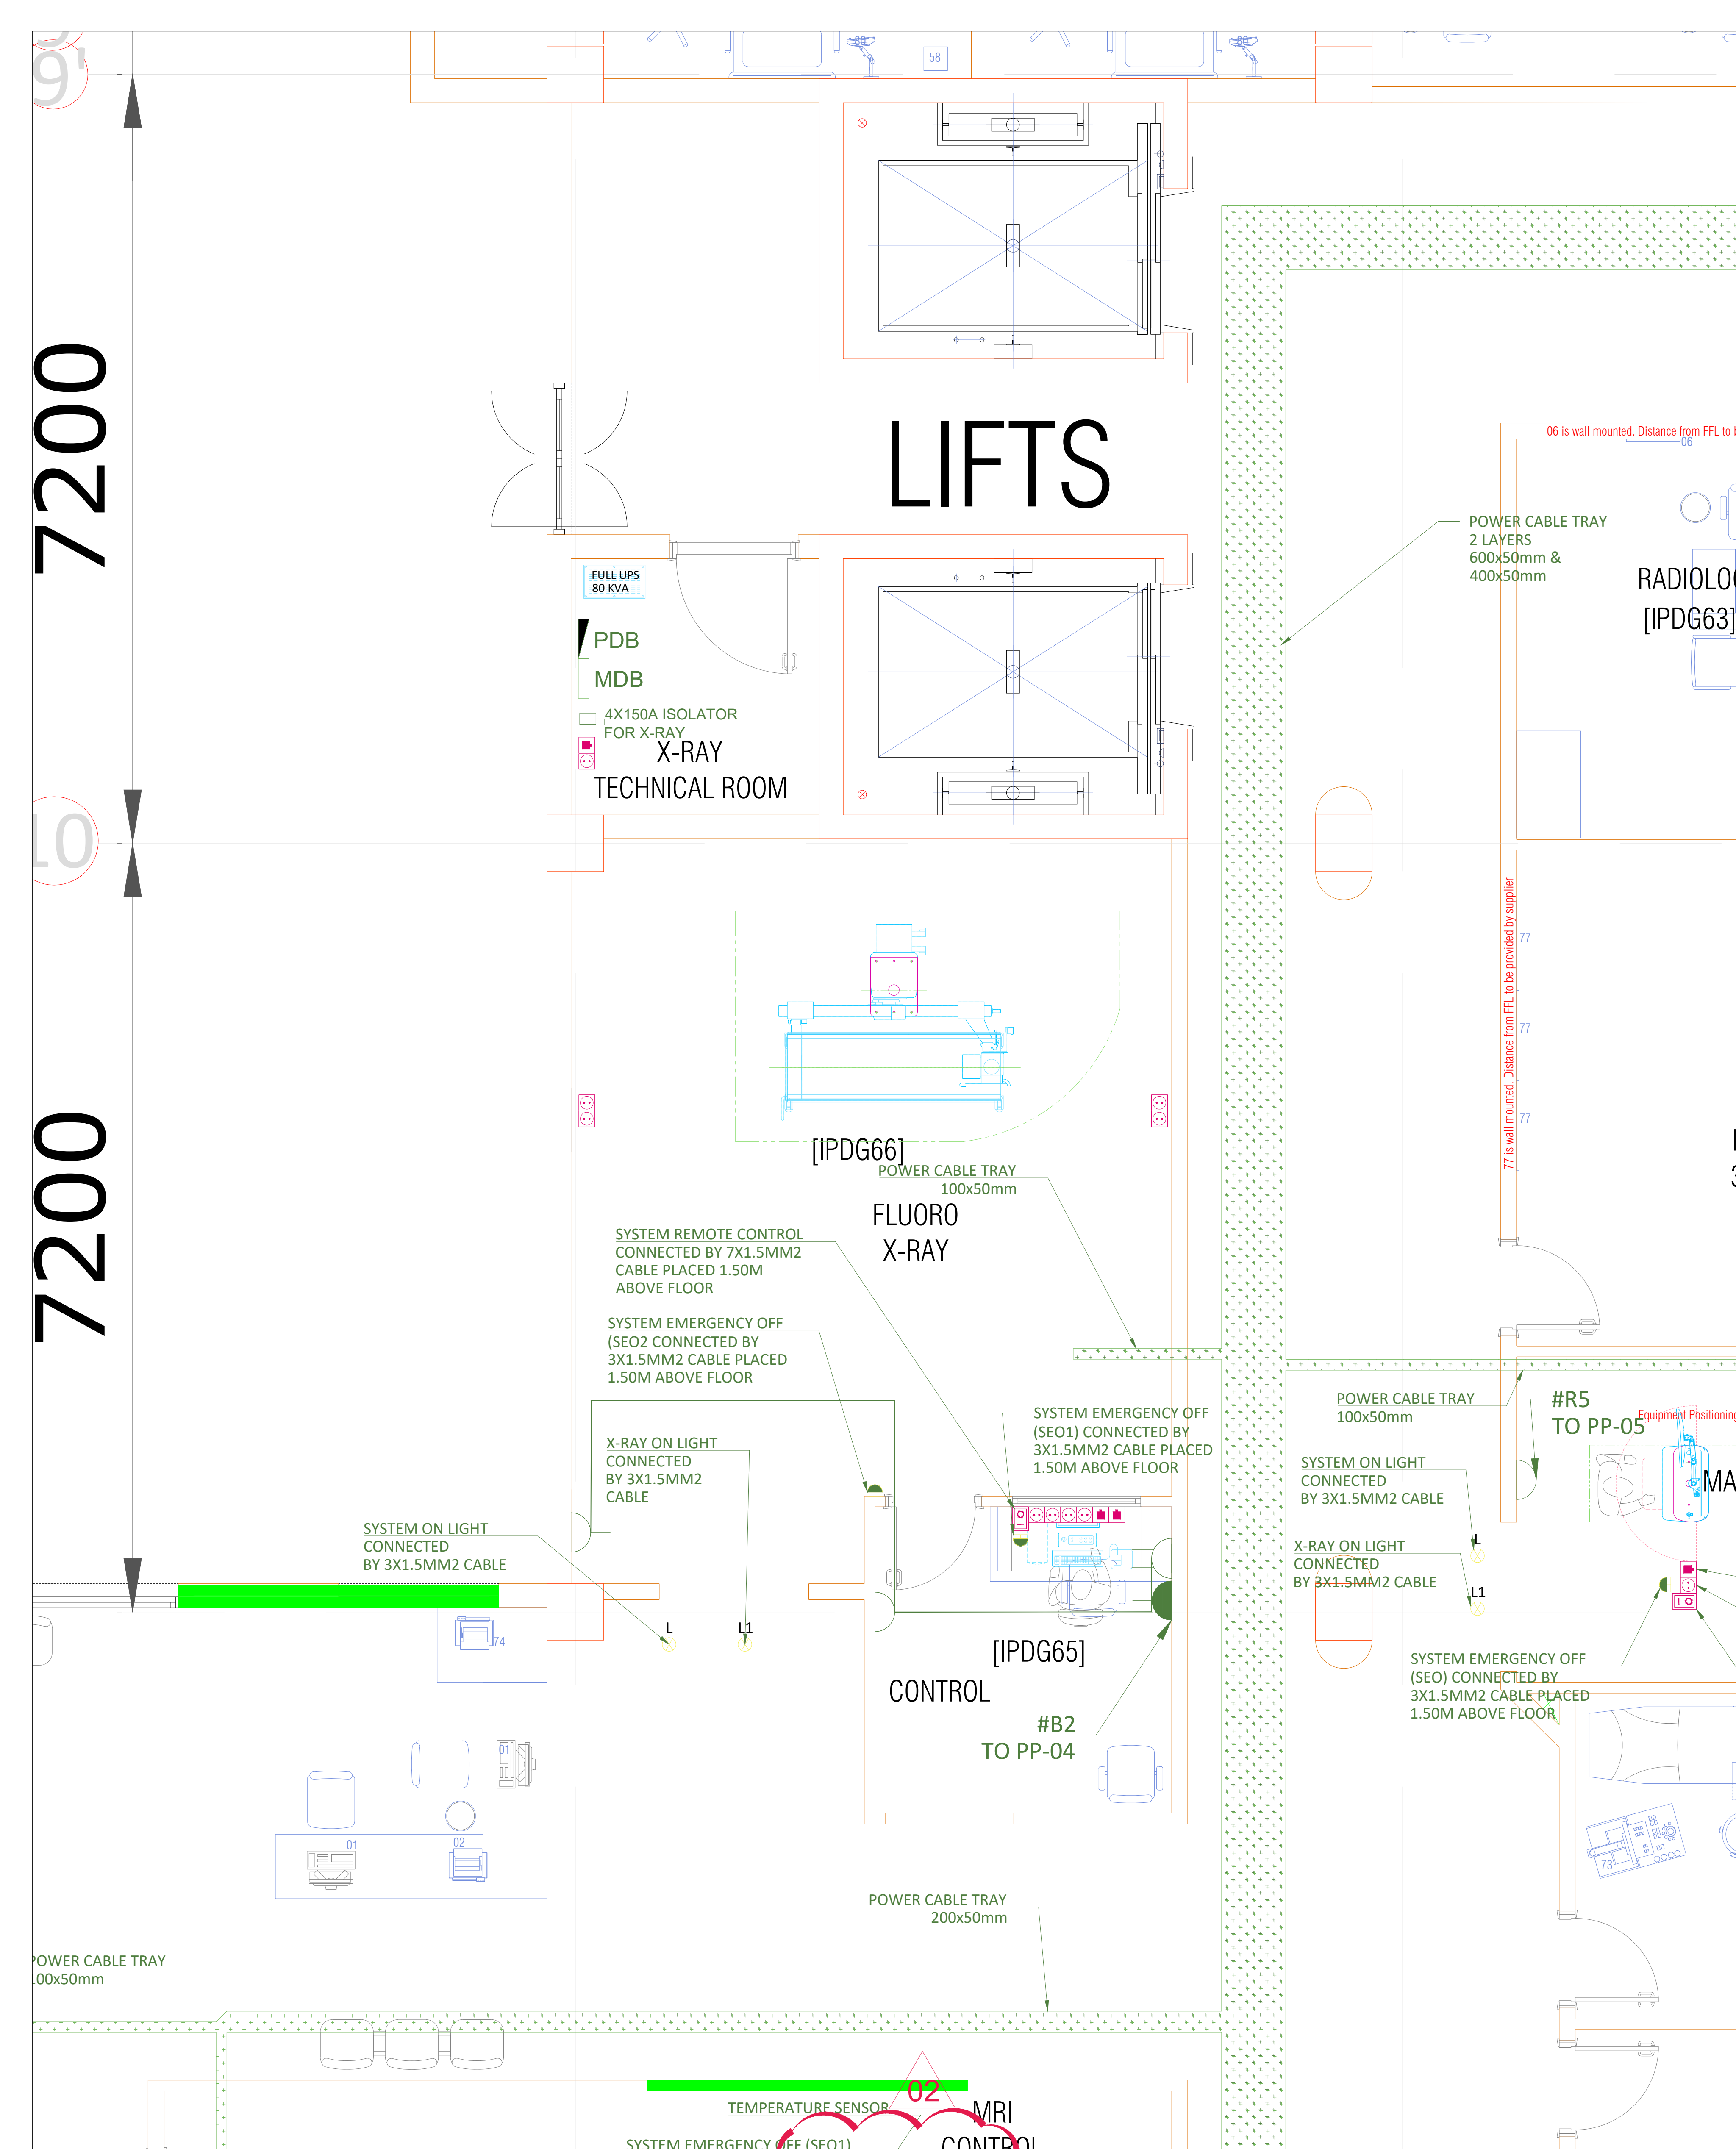

<div>NOTES</div> <p>Tanit Medical Engineering does not take responsibility for any damages resulting from changes on drawings made by others. Errors may occur by not referring to the complete set of final issue drawing.</p> <p>Tanit Medical Engineering cannot accept responsibility for any damage due to the partial use of final issue drawings, however caused.</p> <p>All dimensions are in millimeters unless otherwise specified. Do not scale from printed pdf files.</p> <p>Tanit Medical Engineering accepts no responsibility or liability for defective work due to scaling from these drawings.</p>		
<div>LEGEND</div> <div><div>1.</div><div>FOR SYMBOLS, LEGEND AND GENERAL NOTES, REFER TO DWG # E-001.</div></div> <div><div>2.</div><div>FOR GENERAL ELECTRICAL DETAILS, REFER TO DWG # E-501 AND E-502.</div></div> <div><div>3.</div><div>ALL EMERGENCY AND EXIT LIGHTING ARE WIRED ON NON SWITCHED CIRCUIT TO THE PANEL BOARD IN THE RESPECTIVE ZONE.</div></div>		
REV	MODIFICATIONS	DATE
00	ISSUED FOR APPROVAL	31/12/2023
01	REVISED BASED ON GE COMMENTS	13/01/2024
02	REVISED BASED ON GE COMMENTS	08/02/2024
<div>CONTRACTOR:</div> <div>FOMEX Ltd.</div>		
<div><div><div>TANIT</div><div>MEDICAL ENGINEERING</div></div><div><div>9 Ade Adedeji Close, Lekki Phase 1 Lagos, Nigeria TEL: +234 803 525 1436. Email: info@tanitgroup.com www.tanitgroup.com</div><div><div>TANIT MEDICAL ENGINEERING</div><div>Distribution and Storage of Pharmaceuticals Equipment Contracting Building and Medical Infrastructure Project Development Advisory</div></div></div></div>		
<div>PROJECT TITLE:</div> <div>STELLA OBASANJO HOSPITAL</div>		
<div>CLIENT:</div> <div>BMC Ltd.</div>		
<div>SHEET TITLE:</div> <div>Ground Floor Plan X-RAY LAYOUT</div>		
<div>Revision: 02</div>		
<div>Scale: 1/150</div>		
<div>Drawn by: A.H</div>		<div>Date: 08/02/2024</div>
<div>Checked by: A.H</div>		<div>Date: 08/02/2024</div>
<div>Approved by: I.K</div>		<div>Date: 08/02/2024</div>
<div>PROJECT NO: 20/SOH-01</div>		<div>SHEET NO: GE-103</div>

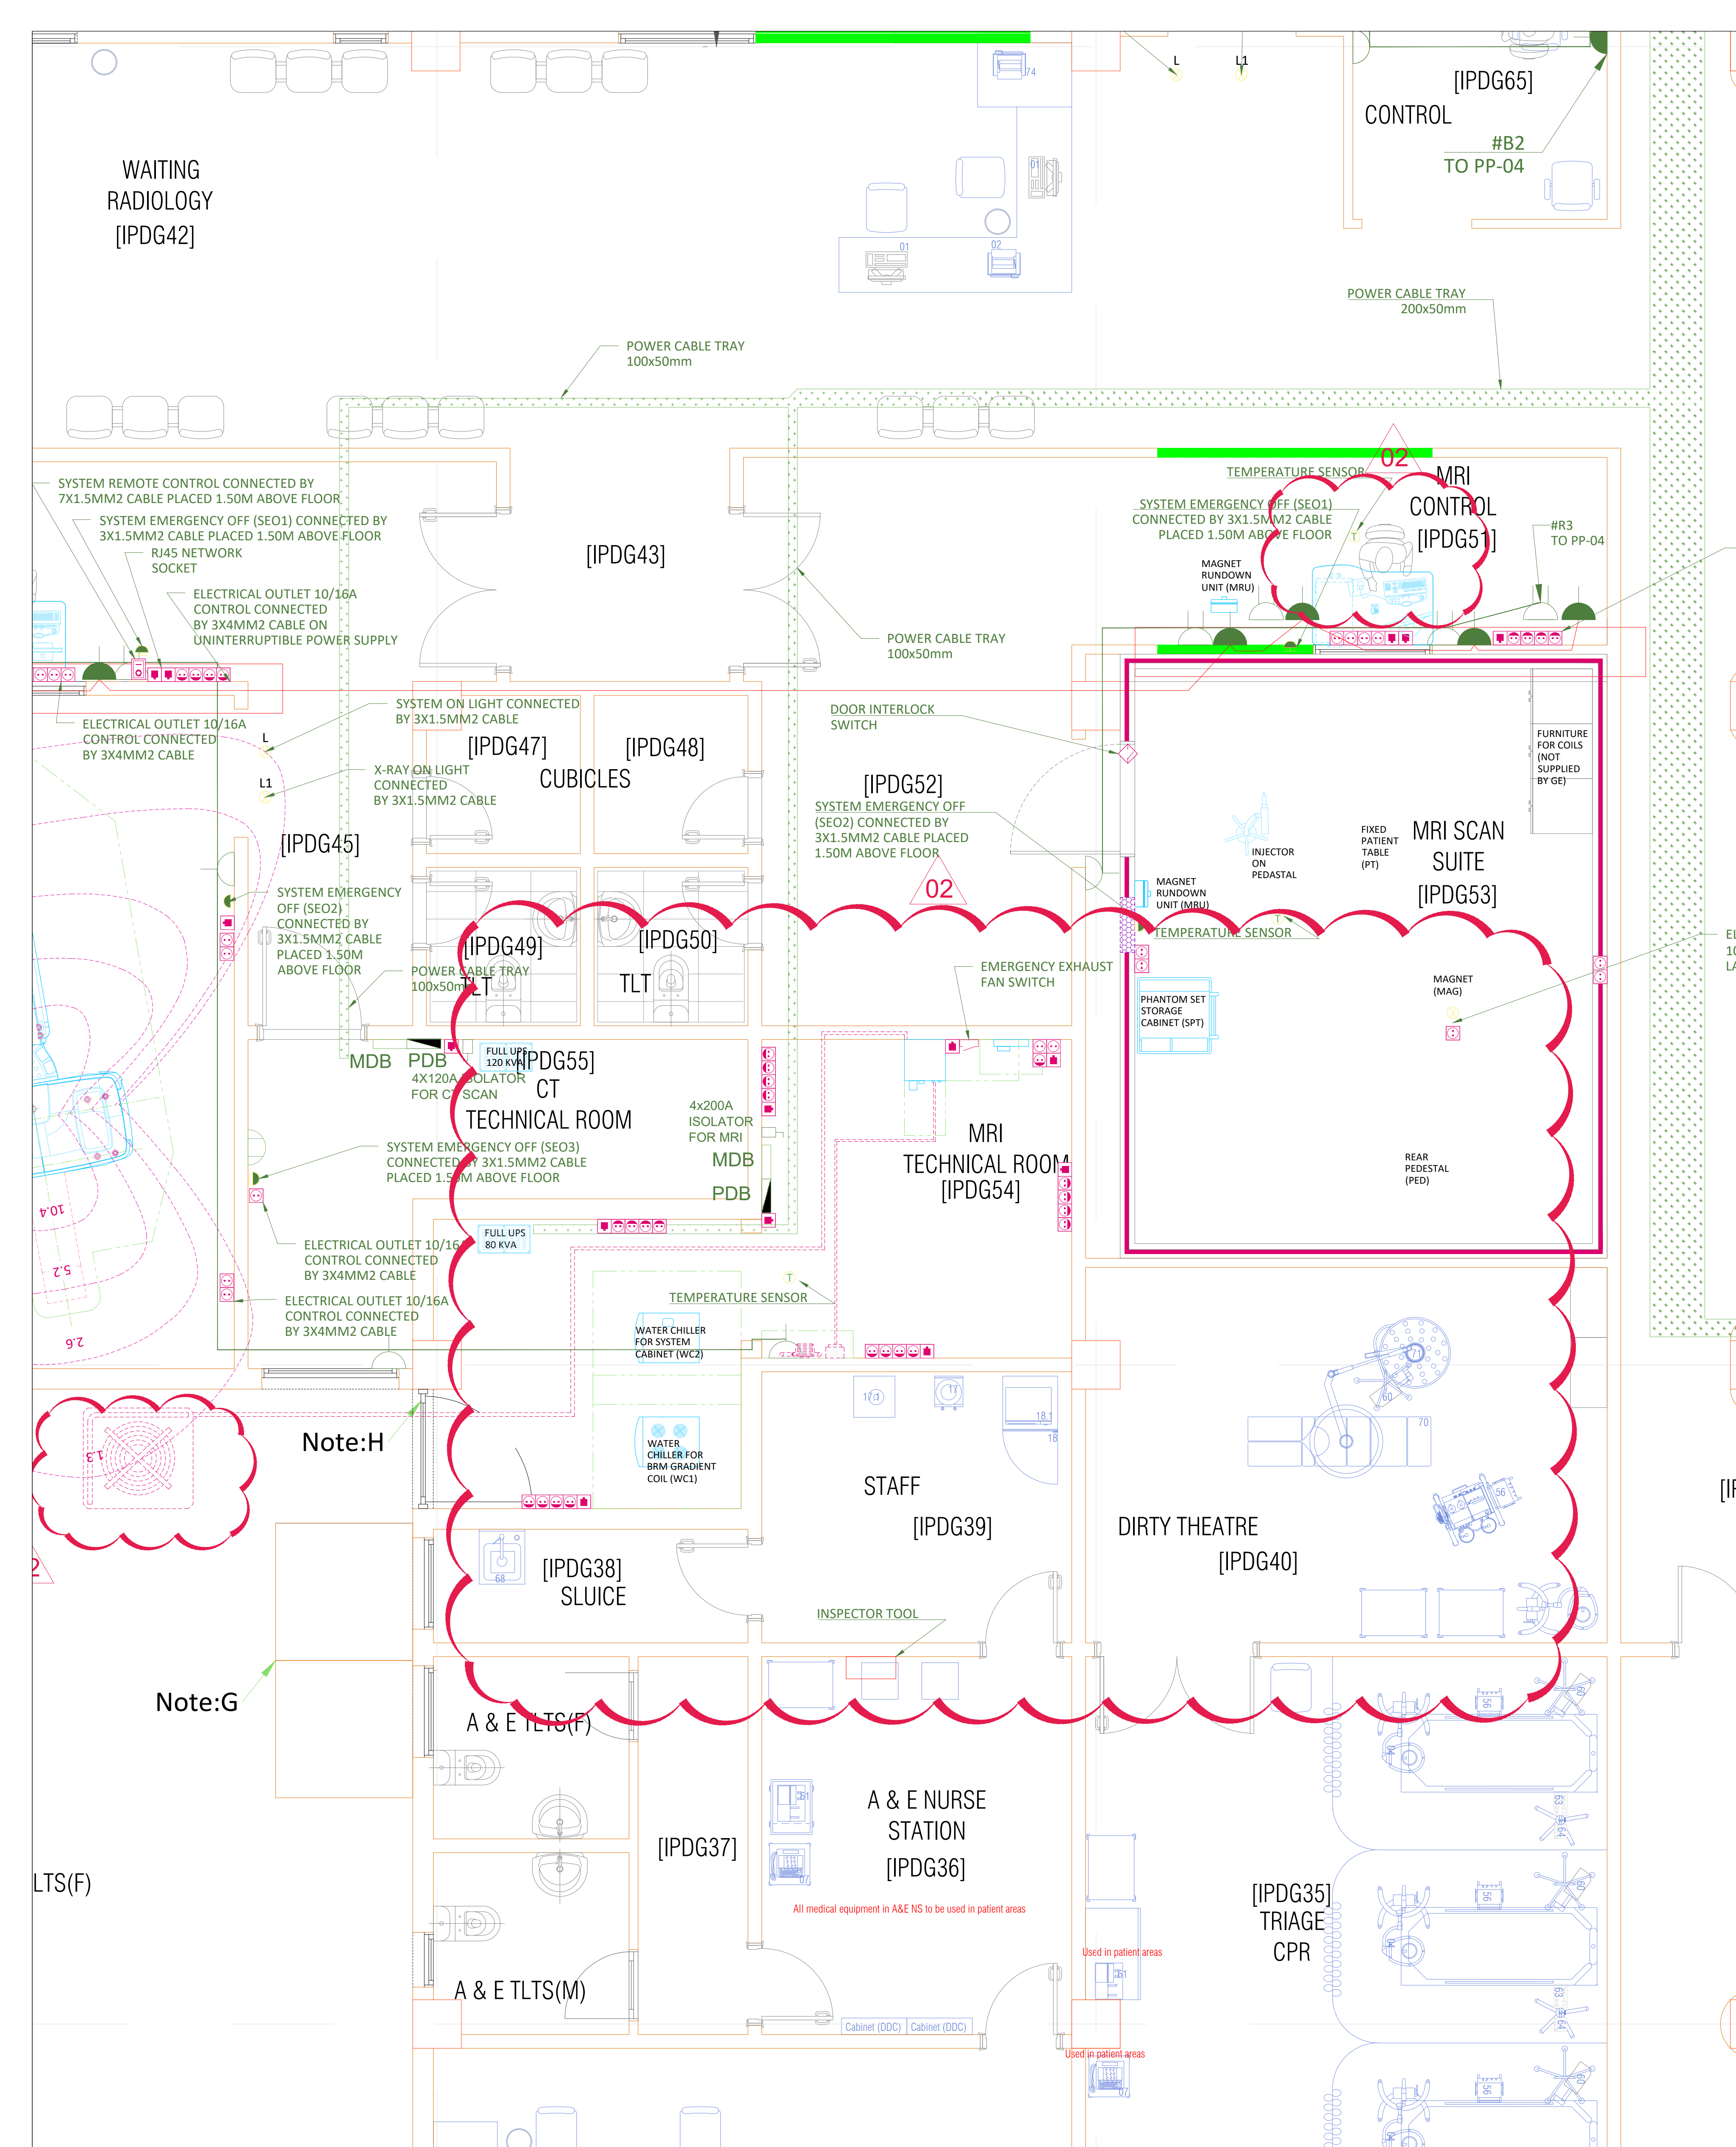

MRI SCANNER LAYOUT
SCALE: 1/35

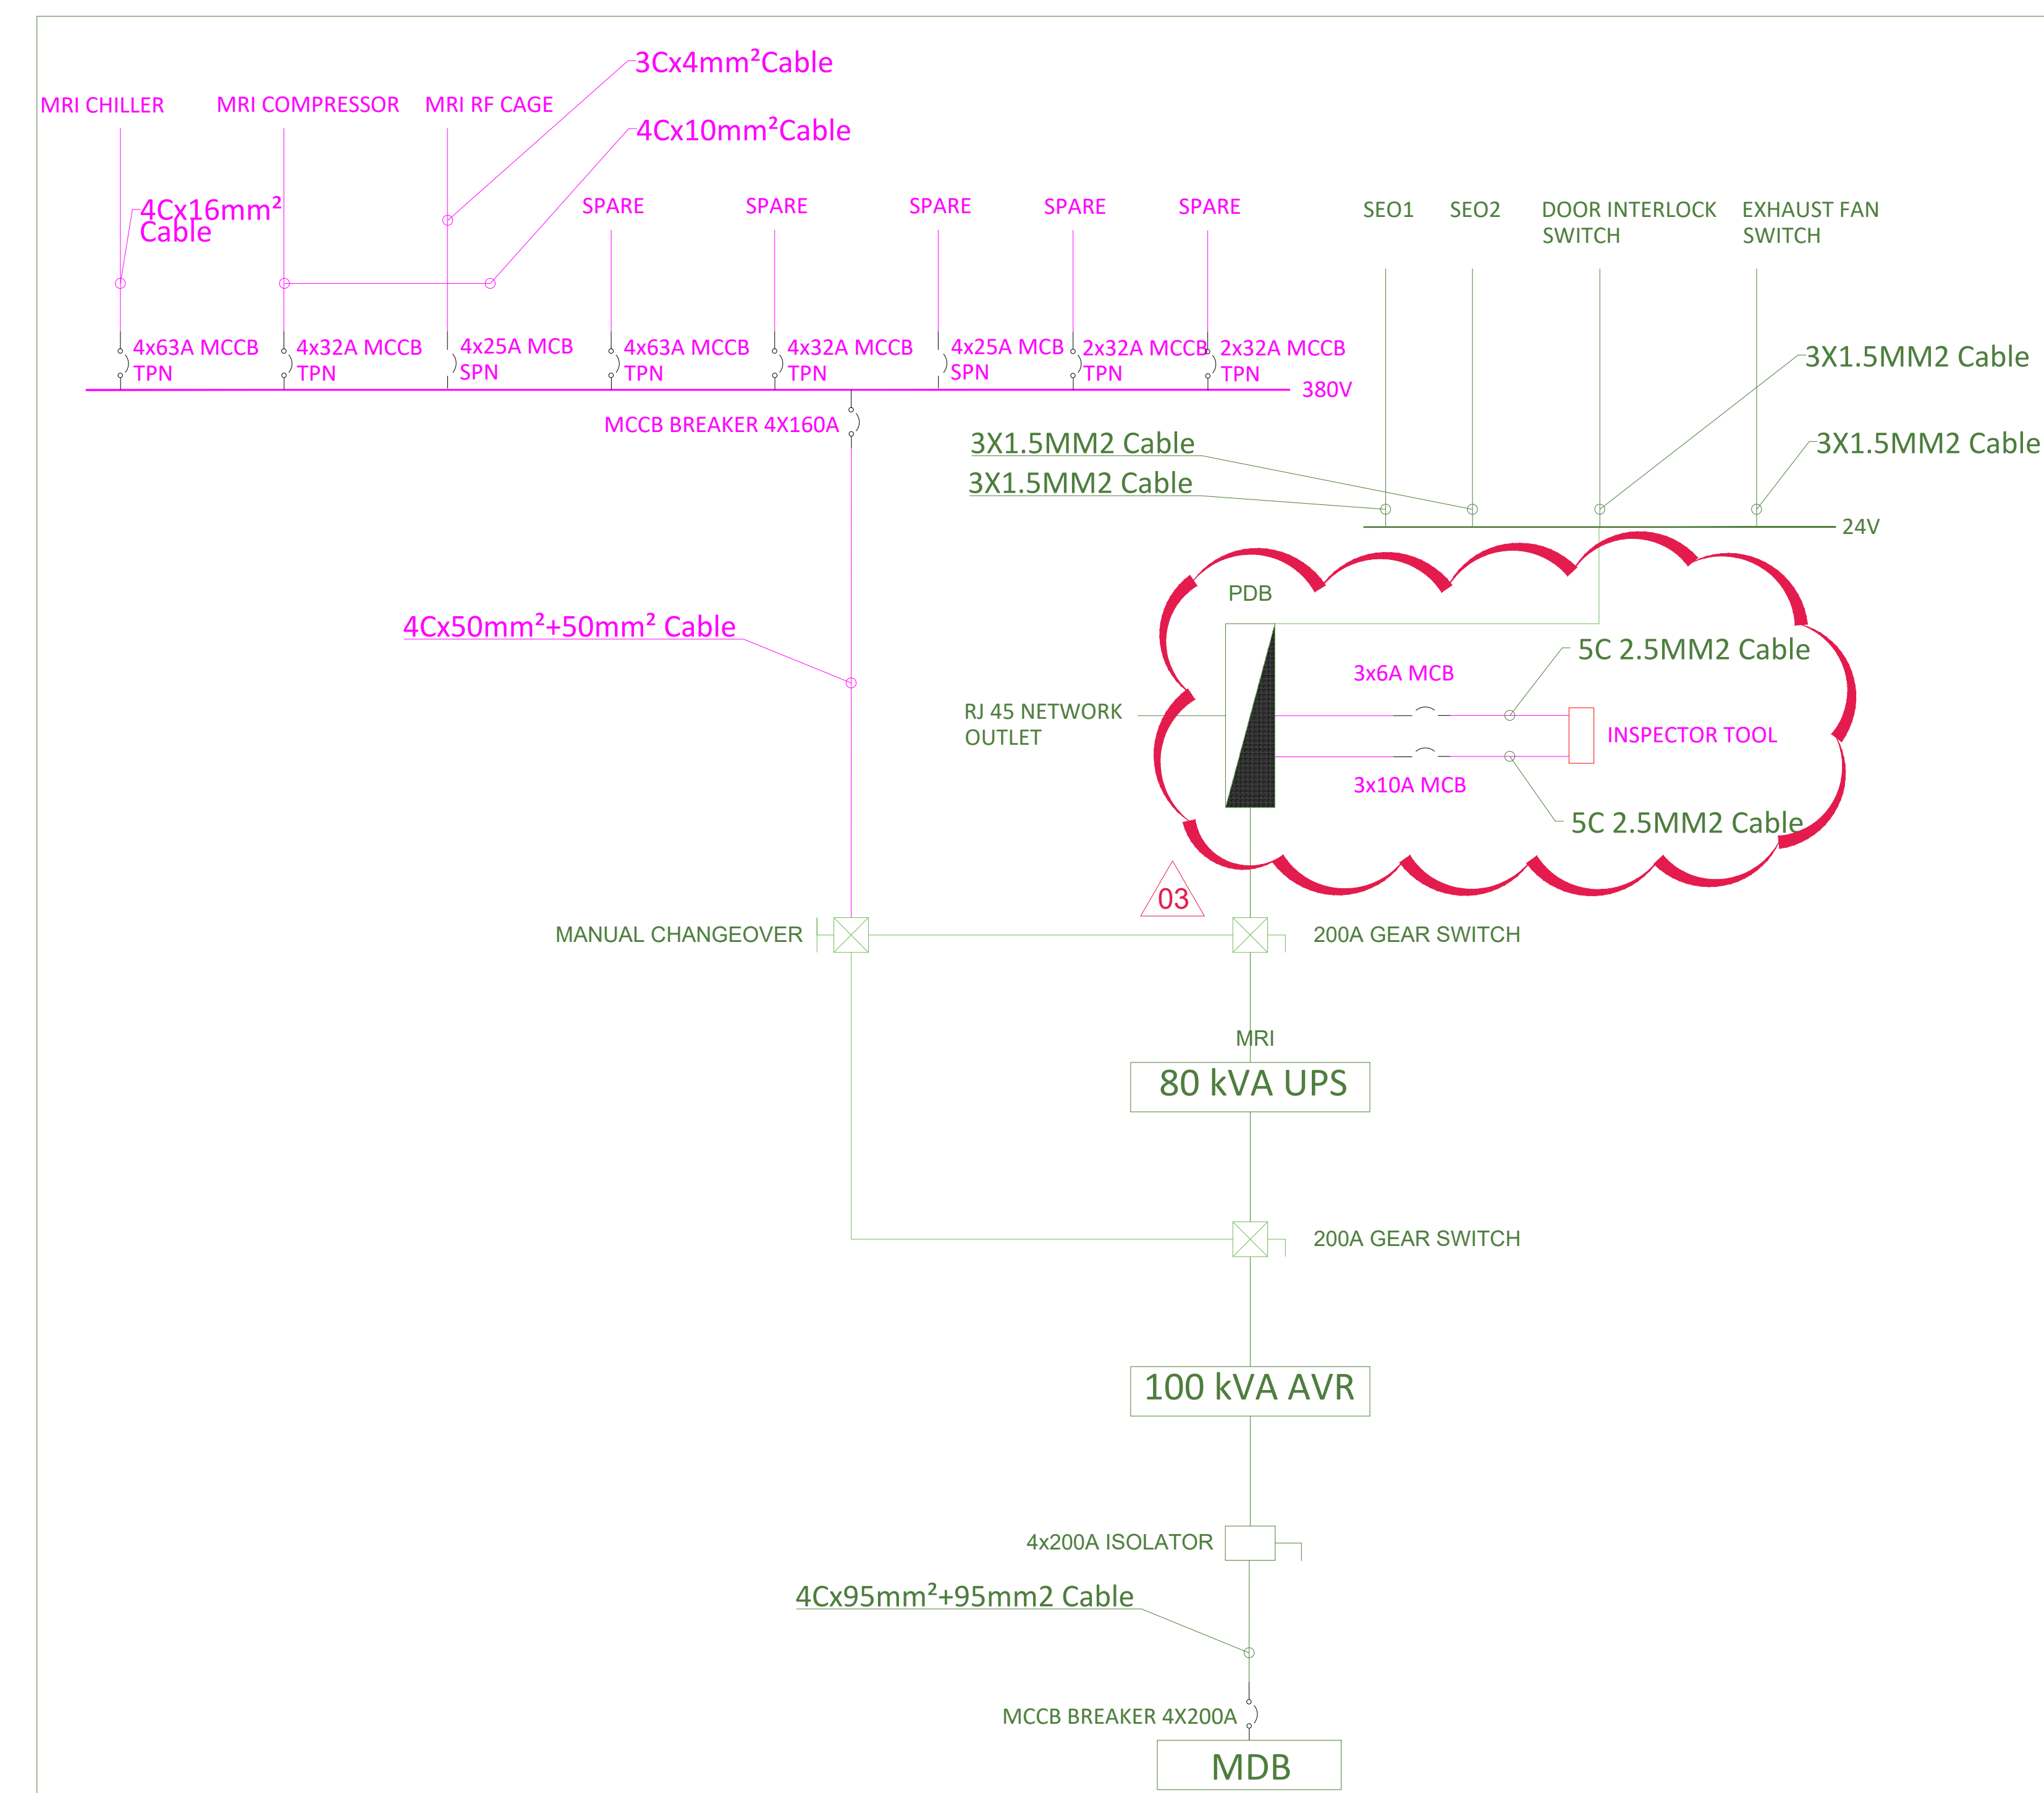

TYPICAL SCHEMATIC DIAGRAM
MRI ROOM

MRI SCANNER SCHEMATIC
DIAGRAM
SCALE: NTS

NOTES

Tanit Medical Engineering does not take responsibility for any damages resulting from changes on drawings made by others. Errors may occur by not referring to the complete set of final issue drawing.

Tanit Medical Engineering cannot accept responsibility for any damage due to the partial use of final issue drawings, however caused.

All dimensions are in millimeters unless otherwise specified. Do not scale from printed pdf files.

Tanit Medical Engineering accepts no responsibility or liability for defective work due to scaling from these drawings.

LEGEND

1. FOR SYMBOLS, LEGEND AND GENERAL NOTES, REFER TO DWG # E-001.
2. FOR GENERAL ELECTRICAL DETAILS, REFER TO DWG # E-501 AND E-502.
3. ALL EMERGENCY AND EXIT LIGHTING ARE WIRED ON NON SWITCHED CIRCUIT TO THE PANEL BOARD IN THE RESPECTIVE ZONE.

REV	MODIFICATIONS	DATE
00	ISSUED FOR APPROVAL	31/12/2023
01	REVISED BASED ON GE COMMENTS	13/01/2024
02	REVISED BASED ON GE COMMENTS	08/02/2024

CONTRACTOR:
FOMEX Ltd.

TANIT
MEDICAL ENGINEERING

TANIT MEDICAL ENGINEERING
9 Ade Adedeji Close,
Lekki Phase 1 Lagos, Nigeria
TEL: +234 803 525 1436.
Email: info@tanitgroup.com
www.tanitgroup.com

Distribution and Storage of Pharmaceuticals	Equipment Contracting
Building and Medical Infrastructure	Project Development Advisory

PROJECT TITLE:
STELLA OBASANJO HOSPITAL

CLIENT:
BMC Ltd.

SHEET TITLE:

Ground Floor Plan
MRI SCANNER LAYOUT

Revision: 02

Scale: 1/150

Drawn by: A.H	Date: 08/02/2024
---------------	------------------

Checked by: A.H	Date: 08/02/2024
-----------------	------------------

Approved by: I.K	Date: 08/02/2024
------------------	------------------

PROJECT NO:
20/SOH-01

SHEET NO:
GE-104