



1 ▼

Dec 15, 2021

Hemocytometer use to quantify concentration of cells' suspensions V.1

abotero¹¹University of Alberta

1



protocol .

Plant pathology

abotero

DISCLAIMER – FOR INFORMATIONAL PURPOSES ONLY; USE AT YOUR OWN RISK

The protocol content here is for informational purposes only and does not constitute legal, medical, clinical, or safety advice, or otherwise; content added to protocols.io is not peer reviewed and may not have undergone a formal approval of any kind. Information presented in this protocol should not substitute for independent professional judgment, advice, diagnosis, or treatment. Any action you take or refrain from taking using or relying upon the information presented here is strictly at your own risk. You agree that neither the Company nor any of the authors, contributors, administrators, or anyone else associated with protocols.io, can be held responsible for your use of the information contained in or linked to this protocol or any of our Sites/Apps and Services.

This protocol presents the procedures to estimate the concentration of cells' suspensions using an hemocytometer

abotero 2021. Hemocytometer use to quantify concentration of cells' suspensions. **protocols.io**
<https://protocols.io/view/hemocytometer-use-to-quantify-concentration-of-cel-b2vcqe2w>



Hemocytometer

protocol ,

Dec 15, 2021

Dec 15, 2021

55940

The lower limit for accurate counting of cells in a hemocytometer is usually considered to be $2.5 \times 10^5/\text{ml}$.

For cell numbers greater than $2.5 \times 10^6/\text{ml}$, it is generally recommended that the sample be diluted.

Hemocytometer
Microscope
Vortex (optional)
Micropipette 10-100 μl
Pipette tips

:

DISCLAIMER – FOR INFORMATIONAL PURPOSES ONLY; USE AT YOUR OWN RISK


The protocol content here is for informational purposes only and does not constitute legal, medical, clinical, or safety advice, or otherwise; content added to protocols.io is not peer reviewed and may not have undergone a formal approval of any kind. Information presented in this protocol should not substitute for independent professional judgment, advice, diagnosis, or treatment. Any action you take or refrain from taking using or relying upon the information presented here is strictly at your own risk. You agree that neither the Company nor any of the authors, contributors, administrators, or anyone else associated with protocols.io, can be held responsible for your use of the information contained in or linked to this protocol or any of our Sites/Apps and Services.

- 1 Wash the hemocytometer with a washer bottle and dry it using a paper towel
- 2 Cover the hemocytometer with the coverslip and place it on a flat surface
- 3 Vortex briefly the cell suspension whose concentration will be calculated
- 4 Using a micropipette collect 10-100 μl of the previously agitated suspension

- 5 Place the micropipette tip on the hemocytometer edge near the coverslip
- 6 Empty the spore suspension slowly into the chamber of the hemocytometer
- 7 Place the hemocytometer in the microscope's mechanical stage and secure it using the stage clip
- 8 Turn on the microscope and focus on the hemocytometer
- 9 Look out for the first square to be counted
- 10 Count the number of cells on each square

If the cells are touching the upper or the left lines of the square, cells are to be counted, but if they are touching the lower or right line they should not be counted

- 11 Count all the squares following a zig-zag

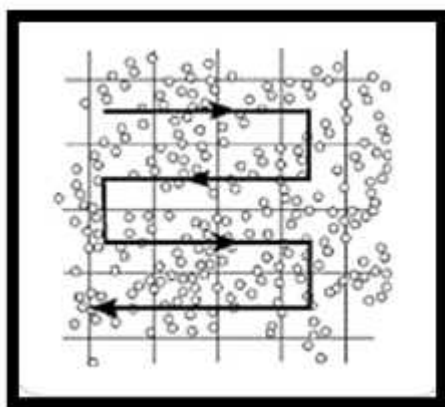

12 Write down the number of cells on each square


The lower limit for accurate counting of cells in a hemocytometer is usually considered to be $2.5 \times 10^5/\text{ml}$.

For cell numbers greater than $2.5 \times 10^6/\text{ml}$, it is generally recommended that the sample be diluted.

Count the number of cells on at least five squares. Ideally, repeat the procedure twice for higher accuracy

13 Estimation of the concentration

According to the cell's size cells can be counted on squares 1, 2 or 3

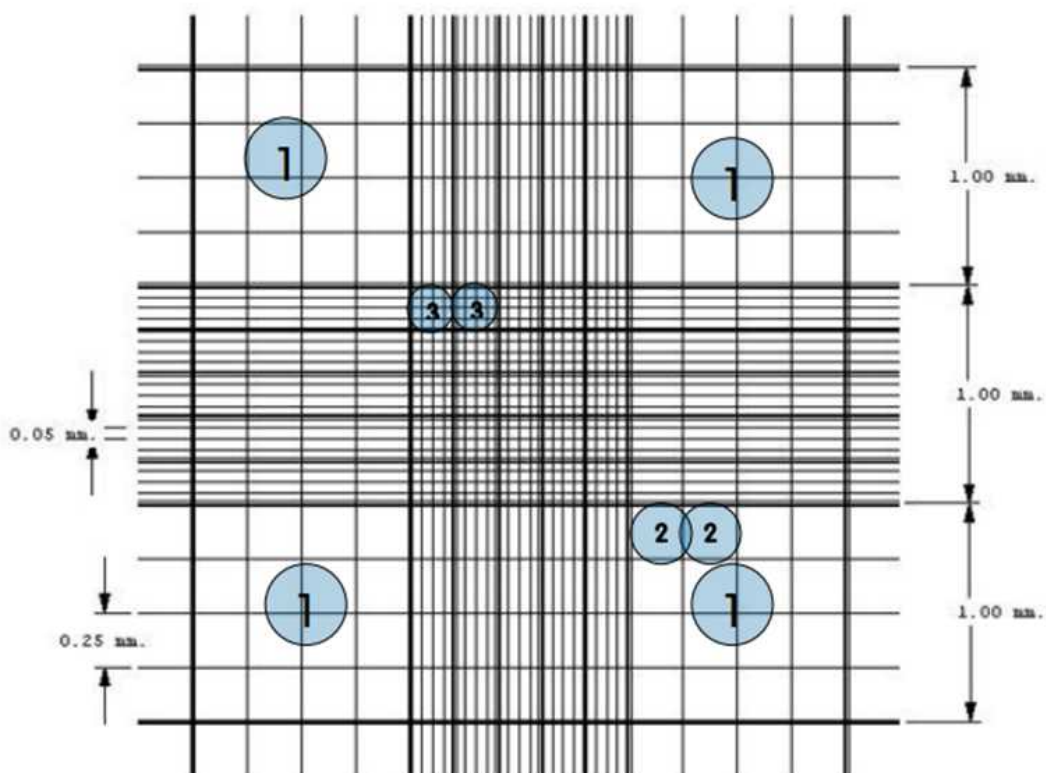

13.1 If cells were counted on squares of size 1

Concentration (cells/ml)= Number of counted cells*10,000/Number of squares counted

If the cells' suspension has been diluted the formula should be adjusted to:

*Concentration (cells/ml)= Number of counted cells*10,000/Number of squares counted*dilution*

13.2 If cells were counted on squares of size 2

Concentration (cells/ml)= Number of counted cells*160,000/Number of squares counted

If the cells' suspension has been diluted the formula should be adjusted to:

Concentration (cells/ml)= Number of counted cells*160,000/Number of squares counted*dilution

13.3 If cells were counted on squares of size 3

Concentration (cells/ml)= Number of counted cells*250,000/Number of squares counted

This square size is typically used to count *Plasmodiophora brassicae* resting spores

If the cells' suspension has been diluted the formula should be adjusted to:

Concentration (cells/ml)= Number of counted cells*250,000/Number of squares counted*dilution