

Version 2 ▾

Aug 14, 2020

⌚ V.2 - Direct wastewater RNA capture and purification via the "Sewage, Salt, Silica and SARS-CoV-2 (4S)" method V.2

Oscar N Whitney¹, Basem Al-Shayeb², Alex Crits-Cristoph³, Mira Chaplin⁴, Vinson Fan¹, Hannah Greenwald⁴, Adrian Hinkle⁴, Rose Kantor⁴, Lauren Kennedy⁴, Anna Maurer¹, Robert Tjian⁵, Kara L. Nelson⁶, UC Berkeley Wastewater-based epidemiology consortium⁶

¹University of California, Berkeley, Tjian & Darzacq laboratory; ²University of California, Berkeley, Banfield & Doudna laboratory;

³University of California, Berkeley, Banfield laboratory; ⁴University of California, Berkeley, Nelson laboratory;

⁵University of California, Berkeley, HHMI; ⁶University of California, Berkeley

 Works for me dx.doi.org/10.17504/protocols.io.bjr9km96

Coronavirus Method Development Community




Oscar Whitney

University of California, Berkeley, Tjian & Darzacq Laborato...

ABSTRACT

This protocol describes the procedure of the "4S" (Sewage, Salt, Silica and SARS-CoV-2) method for SARS-CoV-2 RNA extraction from wastewater. Offering a highly efficient, modular and economical alternative to existing wastewater RNA purification methods, this procedure lowers the barrier to entry for SARS-CoV-2 wastewater-based epidemiology. This procedure is intended to be carried out in a BSL2+ laboratory space, with precautions when handling raw wastewater samples.

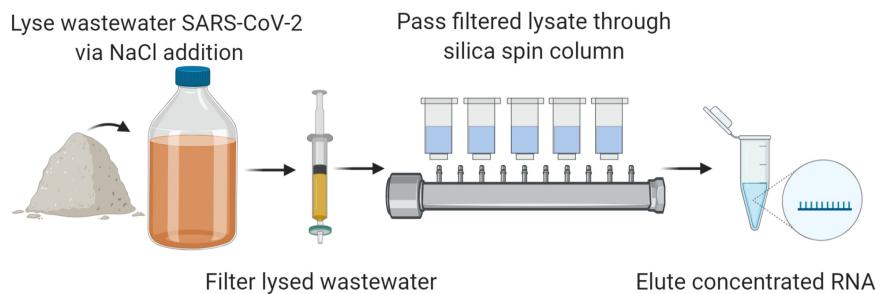

DOI

dx.doi.org/10.17504/protocols.io.bjr9km96

PROTOCOL CITATION

Oscar N Whitney, Basem Al-Shayeb, Alex Crits-Cristoph, Mira Chaplin, Vinson Fan, Hannah Greenwald, Adrian Hinkle, Rose Kantor, Lauren Kennedy, Anna Maurer, Robert Tjian, Kara L. Nelson, UC Berkeley Wastewater-based epidemiology consortium 2020. V.2 - Direct wastewater RNA capture and purification via the "Sewage, Salt, Silica and SARS-CoV-2 (4S)" method. **protocols.io**
<https://dx.doi.org/10.17504/protocols.io.bjr9km96>

KEYWORDS

SARS-CoV-2, Wastewater-based epidemiology, Direct capture, RNA extraction, COVID-19

LICENSE

This is an open access protocol distributed under the terms of the [Creative Commons Attribution License](https://creativecommons.org/licenses/by/4.0/), which permits unrestricted use, distribution, and reproduction in any medium, provided the original author and source are credited

IMAGE ATTRIBUTION

Figures created with BioRender.com

CREATED

Aug 14, 2020

LAST MODIFIED

Aug 14, 2020

PROTOCOL INTEGER ID

40481

GUIDELINES**DISCLAIMER – FOR INFORMATIONAL PURPOSES ONLY; USE AT YOUR OWN RISK**

The protocol content here is for informational purposes only and does not constitute legal, medical, clinical, or safety advice, or otherwise; content added to [protocols.io](#) is not peer reviewed and may not have undergone a formal approval of any kind. Information presented in this protocol should not substitute for independent professional judgment, advice, diagnosis, or treatment. Any action you take or refrain from taking using or relying upon the information presented here is strictly at your own risk. You agree that neither the Company nor any of the authors, contributors, administrators, or anyone else associated with [protocols.io](#), can be held responsible for your use of the information contained in or linked to this protocol or any of our Sites/Apps and Services.

MATERIALS

NAME	CATALOG #	VENDOR
Tris		
EDTA		
Sodium Chloride	PubChem CID: 5234	
Microcentrifuge		
Ethanol		
Zymo III-P column	C1040-5	Zymo Research
EZ-Vac Vacuum Manifold	S7000	Zymo Research
Durapore® Membrane Filter 5.0 µm	SVLP04700	Millipore Sigma
Magnetic Funnel 300mL 47mm	4242	Pall
Bovilis Coronavirus Calf Vaccine	16445	Merck Animal Health
Swinnex Filter Holder	SX0004700	Millipore Sigma
ZymoPURE Elution Buffer	D4200-7-30	Zymo Research

STEPS MATERIALS

NAME	CATALOG #	VENDOR
Durapore® Membrane Filter 5.0 µm	SVLP04700	Millipore Sigma
Swinnex Filter Holder	SX0004700	Millipore Sigma
Magnetic Funnel 300mL 47mm	4242	Pall
EZ-Vac Vacuum Manifold	S7000	Zymo Research
Zymo III-P column	C1040-5	Zymo Research
ZymoPURE Elution Buffer	D4200-7-30	Zymo Research
TE buffer		
Bovilis Coronavirus Calf Vaccine	16445	Merck Animal Health

SAFETY WARNINGS

Wastewater is intrinsically hazardous, so we advise handling wastewater samples in a biosafety cabinet in a BSL2+ laboratory space.

BEFORE STARTING

We developed this procedure to provide a highly efficient, economical and rapid method for extraction of SARS-CoV-2 RNA from wastewater. Using this procedure at the University of California Berkeley, we have captured and quantified SARS-CoV-2 and pepper mild mottle virus (PMMoV) present in a variety of San Francisco Bay Area raw wastewater influent samples and samples collected upstream of wastewater treatment plants. Results may vary depending on wastewater sample type and laboratory setting.

This procedure relies on vacuum column processing, which can be performed with a vacuum manifold and vacuum pump or central vacuum line. In our laboratory, this procedure yields concentrated and purified wastewater RNA in less than 3 hours.

In our laboratory, this purification method enables the detection of SARS-CoV-2 N and E gene RNA as well as PMMoV RNA via RT-qPCR probe-mediated detection. Depending on sample origin, we are able to recover an average of 35 ng RNA/mL of purified wastewater sample (min = 9.33 ng/mL, max = 95 ng/mL).

Preparing RNA wash buffers

- 1 Prepare **1 L** each of two wash buffers - Wash buffer #1 (4S-WB1) and #2 (4S-WB2), for later use during cleanup of RNA bound to silica columns.

1.1 4S-WB1 composition:

Reagent	Original molarity/%	Final molarity/%	Volume per liter of buffer
NaCl	5 M	1.5 M	300 mL
Ethanol	100%	20%	200 mL
TRIS pH 7.2	1 M	10 mM	10 mL
Pure water (MilliQ or distilled)	NA	NA	490 mL

Add **490 mL** water to sterile bottle

Add **300 mL** of **[M]5 Molarity (M)** NaCl

Add **200 mL** of **[M]100 % volume** Ethanol

Add **10 mL** of **[M]1 Molarity (M)** **pH 7.2** TRIS

Agitate to fully mix buffer solution

1.2 4S-WB2 composition:

Reagent	Original molarity/%	Final molarity/%	Volume per liter of buffer
NaCl	5 M	100 mM	20mL
Ethanol	100%	80%	800mL
TRIS pH 7.2	1 M	10 mM	10mL
Pure water (MilliQ or distilled)	NA	NA	170mL

Add **170 mL** water to sterile bottle

Add **20 mL** of **[M]5 Molarity (M)** NaCl

Add **800 mL** of **[M]100 % volume** Ethanol

Add **10 mL** of **[M]1 Molarity (M)** **pH 7.2** TRIS

Agitate to fully mix buffer solution

Sample preparation, RNA preservation and particle lysis

- 2 Obtain a **40 mL** wastewater sample in a sterile sample collection tube. Maintain at **4 °C** during transport to the lab.



Sodium chloride and TE buffer (Go to step 4) can be added to sample immediately after collection. Our unpublished analysis demonstrates that Sodium chloride & TE buffer preserve RNA present in wastewater.

- 3 Resuspend dry bovine coronavirus stock (Bovilis Coronavirus Calf Vaccine) in **2 mL** of PBS. Dilute this resuspended stock into PBS at a dilution of 1:10 (**100 µl** of stock into **900 µl** PBS). Spike 50uL of diluted bCoV into the wastewater sample as a recovery efficiency control. Agitate sample to fully mix bCoV or other spiked-in controls with the wastewater sample.



Bovilis Coronavirus Calf Vaccine

by Merck Animal Health

Catalog #: 16445



Other recovery controls can be used instead of bCoV. Some candidates include Phi6 bacteriophage and coronavirus OC43. In addition, purified RNAs can be used to quantify the extraction efficiency of "free RNA".

- 4 Add **9.5 g** of sodium chloride to **40 mL** wastewater sample.

Make **pH 7.2** TE buffer (**1 Molarity (M)** TRIS, **100 Milimolar (mM)** EDTA).

Add **400 µl** of TE buffer to **40 mL** wastewater sample.




Here, NaCl lyses lipid-protein envelopes, denatures proteins and disrupts RNA-protein interactions. EDTA inhibits the enzymatic degradation of RNA by RNases present in wastewater and TRIS provides optimal buffering conditions for nucleic acids.

- 4.1 Agitate sample until all NaCl dissolves in the wastewater. Vortex or shake sample for **00:00:30** to promote lysis.



Raw wastewater containing NaCl, TRIS & EDTA.

- 5 (OPTIONAL) Heat inactivate sample at Δ **70 °C** for **00:30:00**. Our unpublished analyses have shown that this step will not affect SARS-CoV-2 RNA enrichment and detection.
- 6 Filter the sample through a 5-um PVDF filter via syringe filtration or funnel top vacuum.

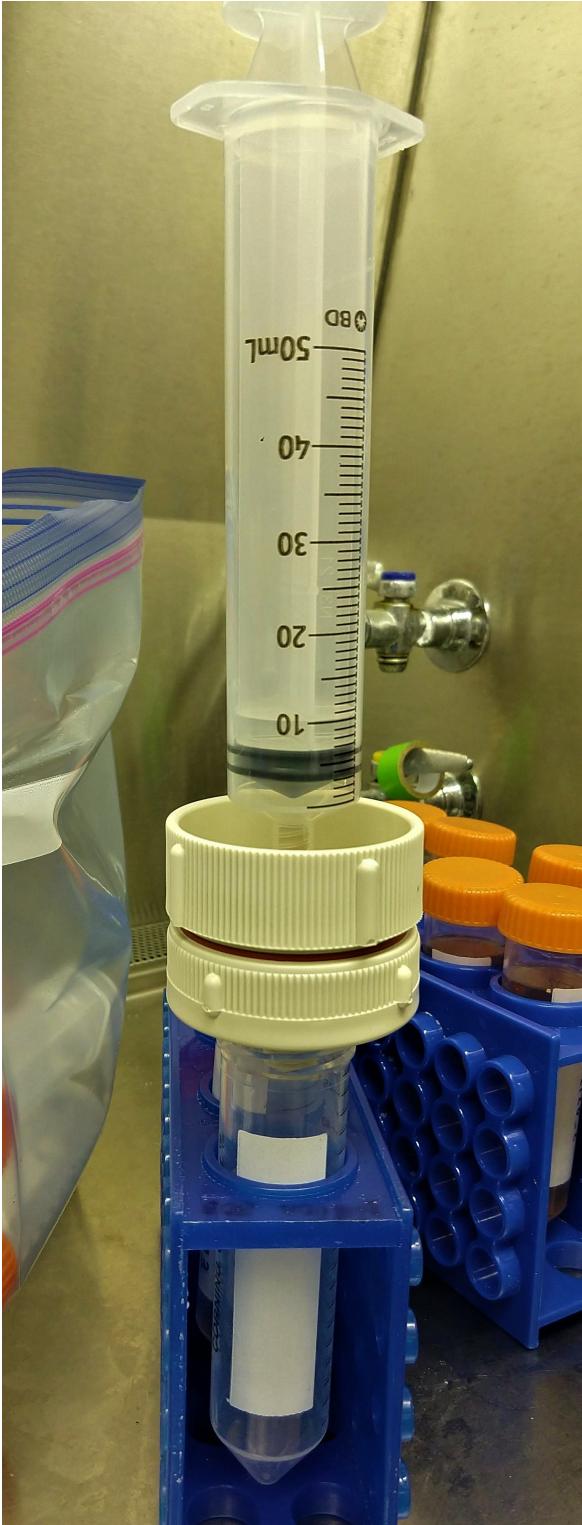

Syringe filter setup: Wastewater is filtered through a 47-mm reusable filter membrane holder.



Durapore® Membrane Filter 5.0 μ m

by Millipore Sigma

Catalog #: SVLP04700



Swinnex Filter Holder
by Millipore Sigma
Catalog #: SX0004700




Magnetic Funnel 300mL 47mm
by Pall
Catalog #: 4242



Wastewater filtering through a 5-um PVDF filter in a Pall filter holder.

Direct RNA extraction (RNA Binding, Washing, Eluting)

- 7 Aliquot **40 mL** filtrate into two **20 mL** aliquots. Add **20 mL** of **[M]70 % volume** ethanol to each **20 mL** sample filtrate aliquot.

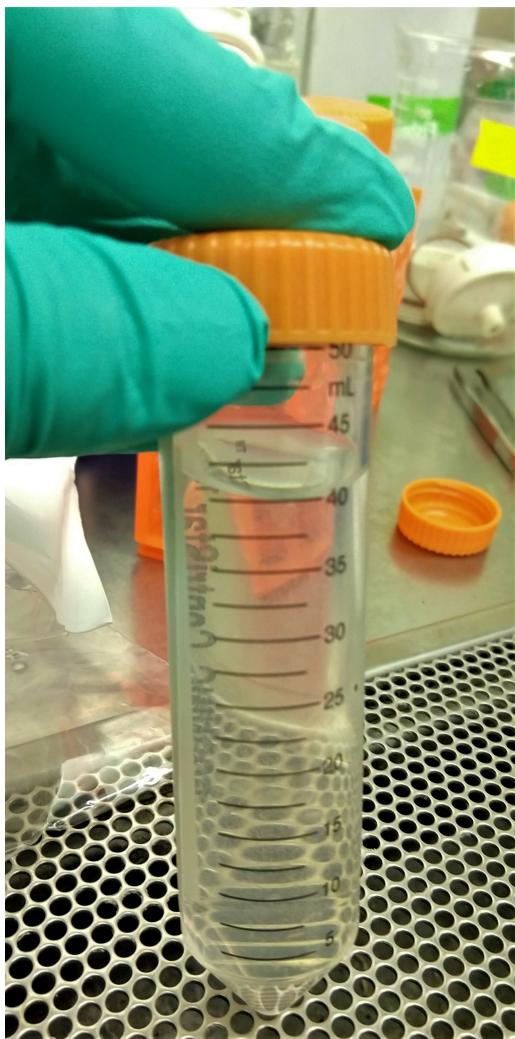


Filtered sample before ethanol addition. Filtrate should be semi-clear.

7.1 Agitate sample to mix ethanol and wastewater lysate.


- 8 Attach Zymo III-P (or other) silica spin column to a vacuum manifold. Vacuum the full **80 mL** volume (both aliquots) of wastewater lysate & ethanol through the spin column.



Commercial silica spin columns vary in their silica membrane packing tightness, changing the flow rate of lysed wastewater. We advise the use of the Zymo III-P column to avoid column clogging issues, but columns such as the Qiagen RNeasy, QIAamp Mini Spin and Zymogen II-CR can act as substitutes, depending on vacuum strength and sample particulate content. Large-format "maxiprep" style columns are also able to purify wastewater RNA, but require a large volume RNA elution up to 20mL (Step 13) and a downstream precipitation-concentration step (Isopropanol precipitation, see [companion protocol](#), Step 12).

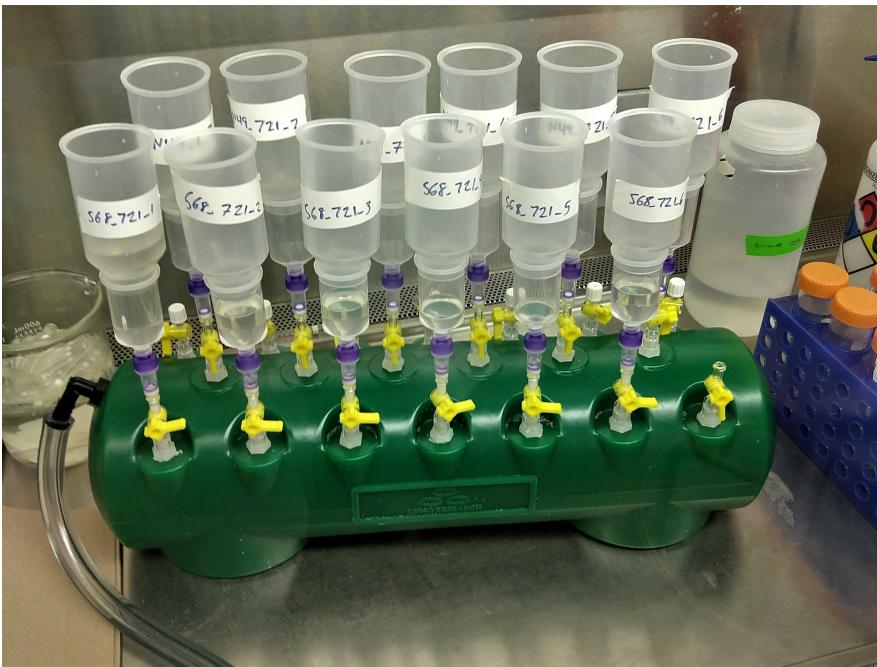

Passing lysed & filtered samples through Zymo III-P columns for direct RNA capture.

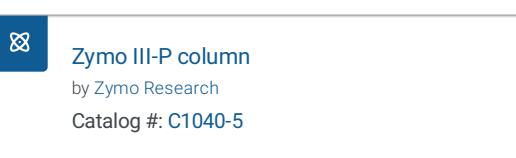

9 Vacuum **5 mL** wash buffer #1 (4S-WB1) through the silica spin column.

10 Vacuum **10 mL** wash buffer #2 (4S-WB2) through the silica spin column.


RNA elution

11 Detach silica spin column from vacuum manifold, remove any attached reservoirs/funnels and place column into a 1.5-mL centrifugation-compatible flowthrough collection tube.

12 Centrifuge silica spin column in tube at **10000 x g, 4°C 00:02:00** to remove any residual 4S-WB2 present in the column.

12.1 Discard the collection tube and place silica column into a new 1.5-mL centrifugation-compatible flowthrough collection tube.

13 Pre-warm **200 µl** of ZymoPURE elution buffer or **200 µl pH 8** TE buffer per RNA sample to **50 °C** in a heat block, waterbath or incubator.



13.1 Add **200 µl** of pre-warmed elution buffer to each silica spin column. Incubate the elution buffer and column + collection tube assembly in a heat block or incubator warmed to **50 °C** for **00:10:00**.

13.2 Spin at **10000 x g, 37°C 00:05:00** to elute RNA from the column.
The flowthrough present in the collection tube contains the purified RNA.

Storage

14 The eluted RNA is now ready for downstream analysis. Store RNA at **4 °C** for same-day use or freeze at **-80 °C** for later use and storage.