



Figure 4

CC-2343

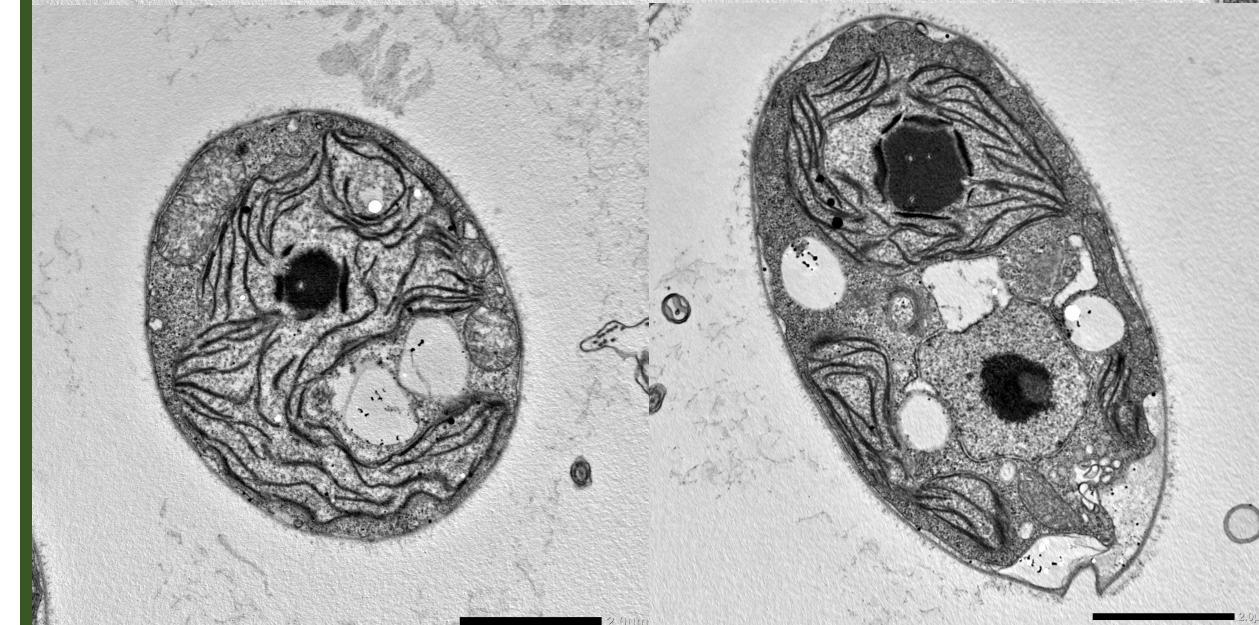

C

Control

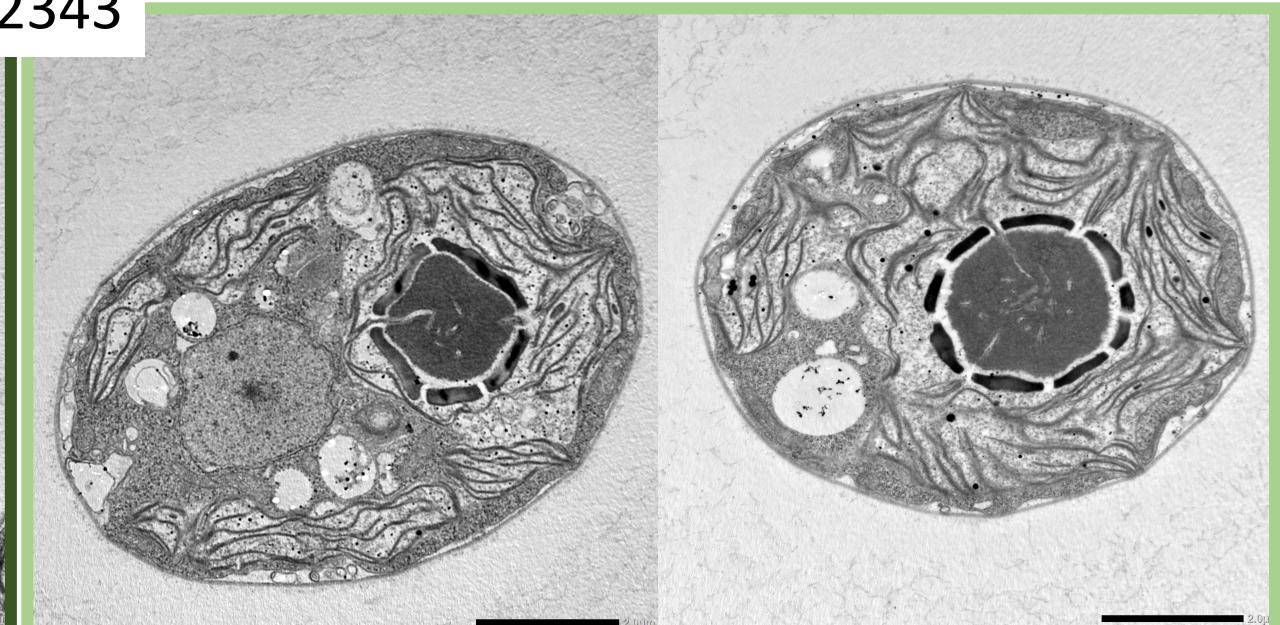

D

H₂O₂ Treatment