


SRL-1109-370 - RawData

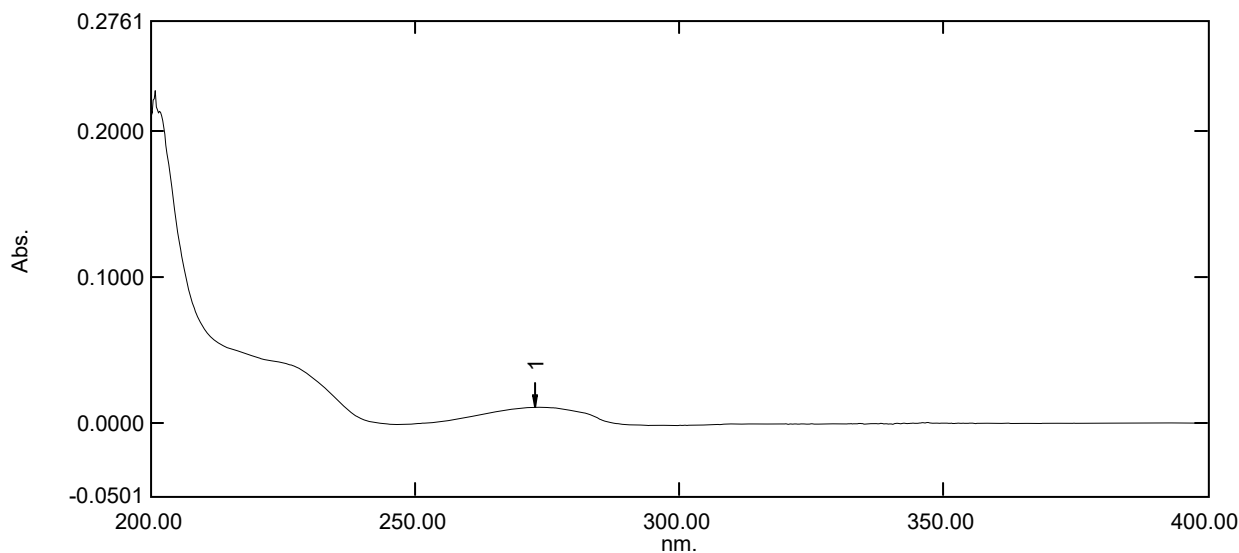

[Measurement Properties]


Wavelength Range (nm.): 200.00 to 400.00  
Scan Speed: Fast  
Sampling Interval: 0.2  
Auto Sampling Interval: Enabled  
Scan Mode: Single

[Instrument Properties]

Instrument Type: UV-1900 Series  
Measuring Mode: Absorbance  
Slit Width: 1.0 nm  
Light Source Change Wavelength: 340.8 nm  
S/R Exchange: Normal

.....

Peak Pick Table

No.	P/V	Wavelength	Abs.	Descriptio
1		272.80	0.0104	

Note - This data is for the reference purpose only. It does not have any correlation with HPLC wavelength. Selection of wavelength of HPLC report is based on the IN-HOUSE protocol.