

International Conference on Computational Intelligence: Modeling Techniques and Applications
(CIMTA) 2013

An Effective Approach: Image Quality Enhancement for Microaneurysms Detection of Non-Dilated Retinal Fundus Image

Niladri Sekhar Datta^{a*}, Himadri Sekhar Dutta^b, Mallika De^c, Saurajeet Mondal^b

^a*Future Institute of Engg. & Management, Dept. of I.T., Kolkata, PIN-700150, India*

^b*Kalyani Govt. Engg. College, Kalyani, Dept. of E.C.E., Nadia, PIN-741235, India*

^c*University of Kalyani, DETS, Kalyani, Nadia, PIN-741235, India*

Abstract

Microaneurysm (MA), small dark round dots on retinal fundus image is the earliest clinical sign of Diabetic Retinopathy (DR) disease. MA detection at early stage can help to reduce the blindness. In such cases the retinal fundus images produced by fluorescent ophthalmoscope are often noisy and low in contrast. Detecting the Microaneurysms using those fundus images is very difficult for ophthalmologist. In the present paper, we propose a method using location based contrast enhancement process, popularly known as Contrast Limited Adaptive Histogram Equalization (CLAHE) for the detection of retinal changes in DR images. CLAHE is an adaptive extension of Histogram Equalization which helps in dynamic preservation of the local contrast characteristics of an image. The proposed algorithm divides the retinal fundus image into a number of small, non-overlapping contextual tiles. Following CLAHE at each tile separately, median filtering of DR images is carried out in order to smooth the background noise. Results of the proposed algorithm show a considerable improvement in the enhancement of DR image quality. The average sensitivity and specificity of this Diabetes Screening System revealed as 82.64% and 99.98% respectively.

© 2013 The Authors. Published by Elsevier Ltd. Open access under [CC BY-NC-ND license](https://creativecommons.org/licenses/by-nc-nd/4.0/).

Selection and peer-review under responsibility of the University of Kalyani, Department of Computer Science & Engineering

Keywords - Medical Image Processing; Optic Disk; Contrast Limited Adaptive Histogram Equalization (CLAHE); Median Filtering; Microaneurysms; Exudates.

1. Introduction

* Corresponding author. Tel.: +918902622816; fax: +91-33-24345641.

E-mail address: dattaniladri1983@gmail.com

Nowadays Diabetes has emerged as a major health care problem in India. According to the International Diabetes Federation (IDF), there were an estimated 40 million patients with diabetes in India in 2007 and this number is predicted to rise to almost 70 million patients by 2025. The countries with the largest number of Diabetic people will be India, China and USA by 2030 [1]. The ratio of people affected with the disease to the number of eye specialist who can screen these patients is very high. Hence there is a need of automated diagnostic system for detection of Diabetic affected eye so that only diseased persons can be referred to the specialist for further intervention and treatment. According to the expert view Diabetic Retinopathy screening may reduce the risk of blindness in these patients by 50% and can provide considerable cost savings to public health systems [2]. Therefore early detection through regular screening and timely intervention will be highly beneficial in effectively controlling the progress of the disease [2]. Usually, retinal images captured from fluorescence oscilloscope are of poor in contrast as a result of the acquisition process. In medical image analysis, it is already reported that image enhancement techniques improve the quality of retinal images. Enhancement, in the present context, refers to bring out the finer details of the image under test while emphasizing the features of interest. The goal of image enhancement is to extract the important characteristics from which a detailed description of the target is henceforth possible. Such an image can serve either for improved human perception or as an input to further automated image processing technique. Thus, image enhancement technique plays a vital role for DR screening system.

A lot of research work published on early diagnosis of Diabetic Retinopathy. Most of them are based on the detection of microaneurysms at mild stage. T. Spencer et al. [3] proposed a mathematical technique to segment MA within fluorescein angiogram. J.H. Hipwell et al. [4] used Gaussian matched filters to retain candidate MA for classification. D. Fleming et al. [5] proposed a method to detect MA by local contrast normalization. C. Sinthanayothin et al. [6] proposed an automated system for detection of Diabetic Retinopathy using Recursive Region Growing Segmentation (RRGS). Usher et al. [7] employed a combination of Recursive Region Growing adaptive intensity thresholding to detect candidate lesions region and a neural network is used for classification to segment MA candidate regions and k-nearest neighbors (KNN) to classify MA. Miri et al. [8] used multi resolution tools using a non linear function to modify the curvelet coefficients. Techniques based on matched filtering are ideal enhancing low contrast blood vessels over a limited area but the computation becomes complex with larger image size [8, 9]. This process is attractive in enhancing the global contrast of an image, but not readily when features of interest occupy a relatively narrow range of gray scale, especially as those noticed in Non Proliferative Diabetic Retinopathy (NPDR) images.

Most of the techniques reported in literature, used retinal images with dilated pupil where MA and other feature already distinguished and clearly visible. The rest of the sections in the paper are organized as follows: section II presents detailed explanation of proposed method; section III describes the detection of MAs using proposed enhancement process. In section IV, results and discussion are provided. Finally, conclusion is given in section V.

2. Proposed CLAHE Method at Pre-processing Stage

Image enhancement technique increase the quality of image under test and ensure improved comprehend ability. Histogram equalization is one of such methodology adopted for contrast enhancement that expands the pixel intensity distribution in order to utilize the entire dynamic range. It is observed that the input retinal fundus images are often very low in contrast, which is evident from their histograms that are narrow and concentrated only to certain gray level values. However, retinopathic images contain minute details of the lesions that get obscured due to limited contrast and are not easily presented to doctors. This may lead to delayed diagnosis and even wrong treatment. Histogram equalization plays an important role in such cases, however, while leaving local changes in contrast, unconsidered. Recently, CLAHE algorithm has been successfully proposed for biomedical imaging; however, it increases background in-homogeneities and hence calls for some post processing. We present a method for enhancement of DR image based on CLAHE method. The basic idea of the algorithm is to divide the image into a number of small, non-overlapping contextual regions, called “Tiles” as shown in fig. 1. The steps of proposed method are given below:

StepI : Retinal fundus image selected as input.

- StepII : Green layer selected.
 StepIII : Decimate the image into two by two sized contextual regions (Tiles).
 StepIV : Apply CLAHE in each tile separately.
 StepV : Apply median filter in each tile separately.
 StepVI : Apply image catenation method on four Tiles.

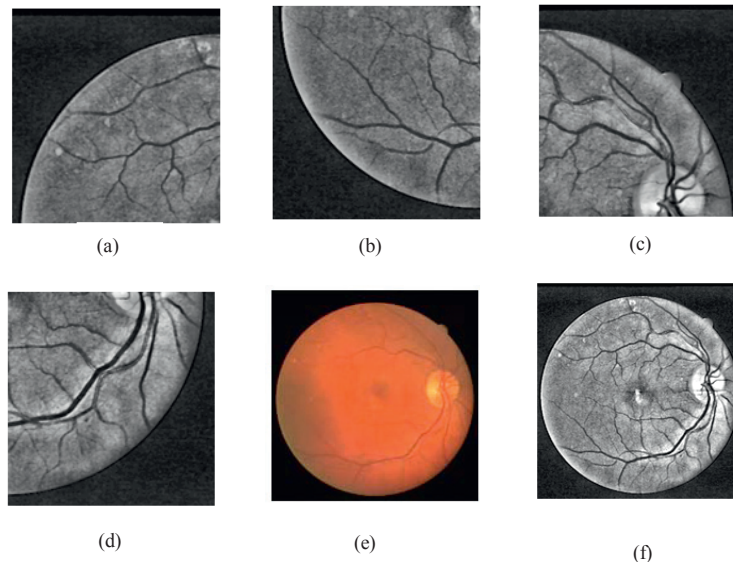


Fig 1. Region based CLAHE followed by median filter (a) Tile1, (b) Tile2, (c) Tile3, (d) Tile4 (e) Original image, (f) Resultant image

In this method median filter is applied for smoothen the enhanced image. A median filter is often chosen as it is proved to be effective in smoothening of the image due to its capability to reduce impulse noise, ability to preserve edge information of resultant image and ability to not create any new unrealistic pixel intensity as the median value is one of the elements present in the neighborhood. The proposed image quality enhancement technique applied on automated Diabetic screening system for classification of normal and Diabetic eye. The next section describes the Microaneurysms detection system.

3. Microaneurysms Detection

In experts point of view detection of MAs become difficult due to low contrast noisy retinal images [11]. In this paper automated software based Diabetes screening system is developed using MATLAB software for calculating the microaneurysms area on given retinal images. In the proposed method the green channel are used to detect the MAs. Next, few subsections describe the intermediate steps for detection of MAs. The overall procedure for MA detection is shown in figure 3.

A. Pre-processing stage

A pre-processing stage is required for improving the image quality prior to the detection stage. Here, the green plane of the original RGB colour image is used as because red lesions have the highest contrast with the background in this colour plane. It is observed that the contrast of the retinal images tends to be bright in the centre and diminish at the side. To equalize the image intensity level, proposed CLAHE method is applied. Then, the image histogram is

examined and also checks the equalization of the intensity level from 0-255.

B. Large Objects Elimination

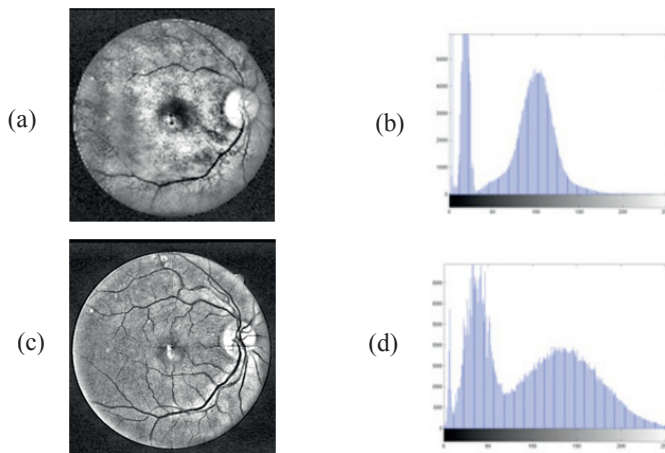


Fig 2. (a) Conventional CLAHE image with (b) Histogram of conventional CLAHE image, (c) Resultant image of proposed method with (d) Histogram of resultant image of proposed method

Canny edge detection method is applied to detect edge and the circular border is obtained after subtracting the dilated image with eroded images. Then, detection and elimination of large object (object size > 100 pixels) of retinal fundus image is carried out. Mathematical morphological methods [12] are applied here for removing large object like exudates, bright lesions etc. The border is eliminated before the image filled up with enclosed area. The area (i.e. MA with noise) obtained by subtracting away the edges with image. Then, the larger objects are removed by morphological operation. The resultant image still contains noise (blood vessels, exudates). As, exudates are the bright yellow-white objects on the retinal image developed due to the leakage of blood, can be traced out by applying proposed CLAHE method. Large objects such as exudates can be removed by applying AND logic.

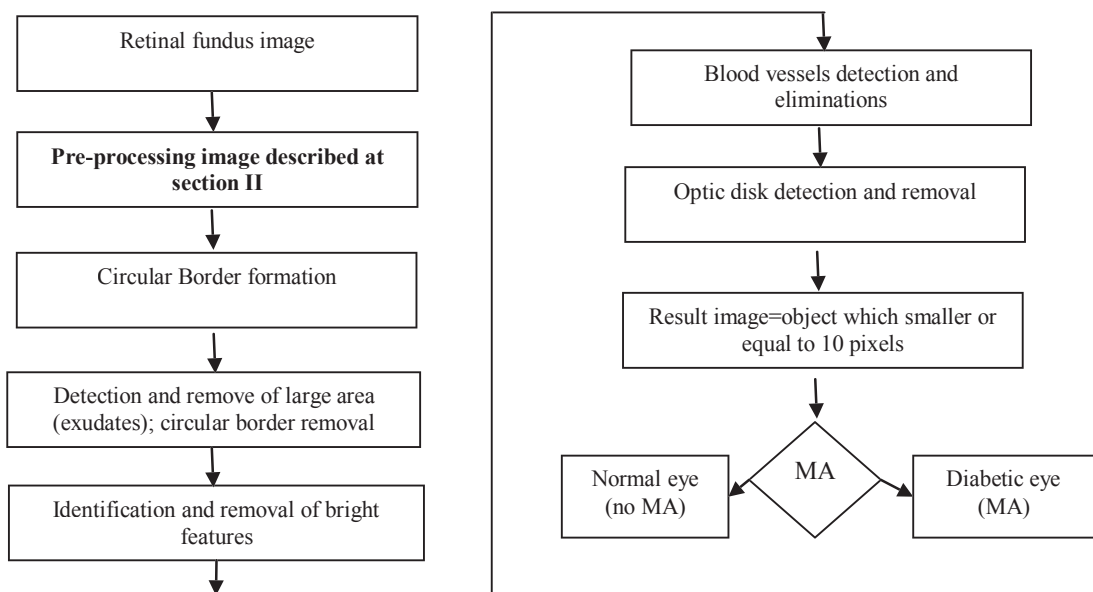


Fig 3. Proposed method for Diabetes detection system

C. Blood Vessel Detection and Eliminations

Blood vessels are detected and extracted by applying morphological operation with image segmentation of threshold value. Removing the small area (object size ≤ 100 pixels) of noise, the clearer blood vessel image is obtained. This image is compared using AND logic with the result from the previous AND logic and remove the blood vessels.

D. Optic Disk Detection and Elimination

Pictorial view of the retinal image illustrates that optic disk is a collection of bright pixels and it is developed in anywhere of the retinal images. So, a mask is created to enclose the optic disk. As m by n matrix (i.e. dimensions of image provided by the user) of retinal input image selected for detection of MA, the maximum value for each of the n columns of the image is first pointed out before locating the largest value. The coordinates (i.e. row and column) of all brightest pixels are determined and median was calculated. Next, the mask is created using the following relation for creating circles:

$$R^2 = (x - h)^2 + (y - k)^2 \quad (1)$$

where h and k are the coordinates (row and column) and R is the radius. Then, created mask is subtracted from the segmented retinal image and obtained the image without optic disk. Microaneurysms area obtained after removing other existing elements.

4. Result and Discussion

The proposed method applied for forty seven retinal images where nine images were abnormal (i.e. damaged for DR) and thirty eight images were normal. The performance of the proposed method is evaluated quantitatively by comparing the resultant extraction with ophthalmologists, hand drawn ground truth images pixel by pixel [13]. The average sensitivity and specificity revealed as 82.64% and 99.98% respectively. The average sensitivity is the percentage of the actual MA pixels that are detected and specificity is the percentage of the non MA pixels that are correctly classified as non MA pixels. In this context the British Diabetic Association (Diabetes UK) has established standards for any Diabetic Retinopathy screening programmed of at least 80% sensitivity and 95% specificity [14]. This research work started with the development of pre-processing techniques to improve image quality using histogram analysis. However, the contrast enhancement technique not only enhances the image quality, but also enhances the noise. Then image processing techniques are applied for identification of normal features such as optic disk, retinal blood vessels and elimination of abnormal features such as Microaneurysms. The overall procedure for MA detection divided into three fundamental steps. The first step consists of image enhancement of the green channel as green channel has most information of image than other channels. The second step detects all possible patterns corresponding to MA. The last step classifies the normal eye and Diabetic eye according to MAs area calculation (i.e. for zero area revealed as normal eye) based on the proposed method.

5. Conclusion

The development of automated Diabetic Retinopathy screening system becomes a highly effective way of reducing the burden of eye specialist, i.e. only Diabetic eye send for further diagnoses. This has major implementation for the reduction of the cost of the public health systems. The proposed method enhances the quality of the DR image while preserving the sharpness and minute of the details. Finally, proposed Diabetic screening system shows the satisfactorily results for classifying normal and Diabetic eye. In view of its modest computational requirements and simplicity, the proposed method may be directly implemented in any image processing engine both for large and high resolution Diabetic Retinopathy images.

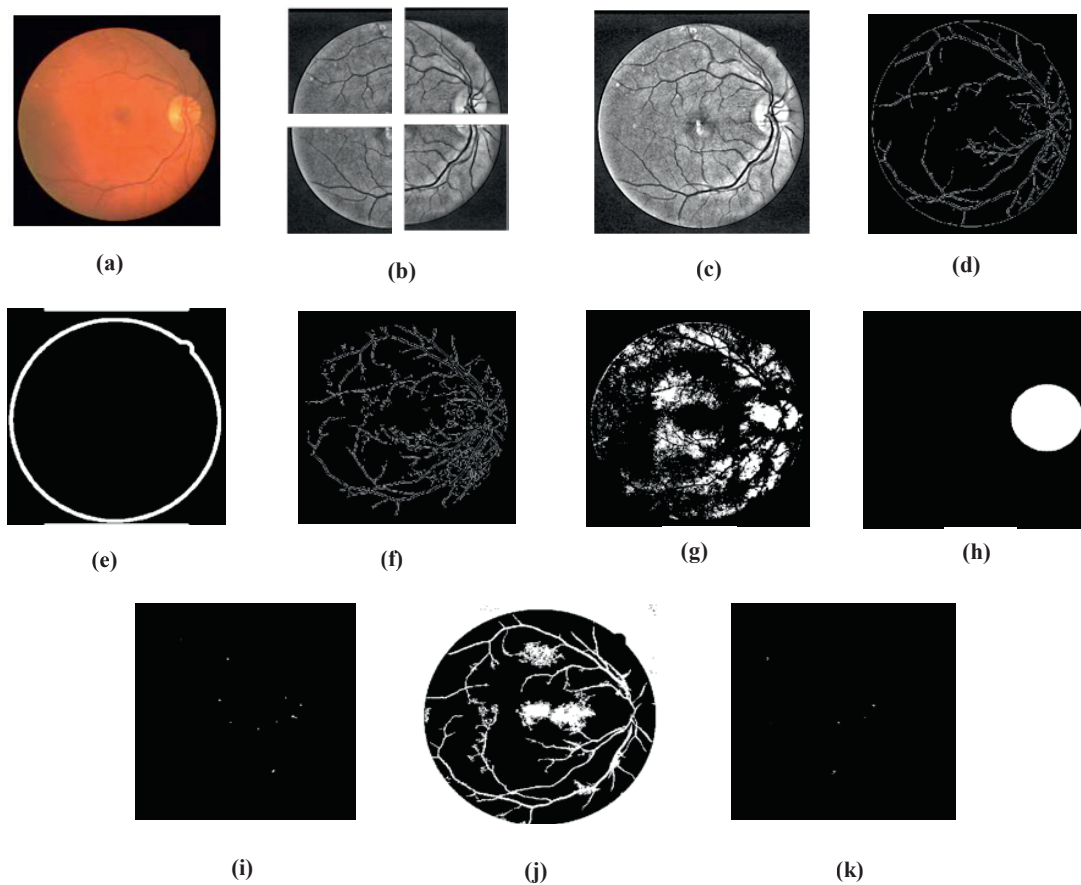


Fig.4. Experimental results:(a) Retinal image as input,(b) Decimate the image into two by two sized contextual regions (c)pre-processing image using proposed method (d) CANNY edge detection, (e) Circular border, (f) Edge without circular border, (g) Bright features of retinal image, (g) Mask for optical disk, (h) MA with noise, (i) Blood vessels with small objects, (j) MA detected after removing blood vessels and noise

Acknowledgements

The authors express their deep sense of gratitude to the faculty members of the Department of Engineering & Technological Studies, University of Kalyani, West Bengal, India, where the research work has been carried out.

References

1. S. Wild, G. Roglic, A. Green, R. Sicree, and H. King "Global prevalence of diabetes: estimates for the year 2000 and projections for 2030" *Diabetes care*. 27 (2004) 1047–1053.
2. H. J. Jelinek, M. J. Cree, D. Worsley, A. Luckie, and P. Nixon "An automated microaneurysm detector as a tool for identification of diabetic retinopathy in rural optometric practice" *Clinical and Experimental Optometry*. 89 (2006) 299–305.
3. T. Spencer, J.A.Olson, M.C. Hardy, P.F.Sharp and J.V. Forrester "An image processing strategy for the segmentation and quantification of microaneurysms in fluorescein angiograms of the ocular fundus " *comp Biomed Res*. 29 (1996) 284-302.
4. J.H. Hipwell, F.Strachan, J.A.Olson, and K.C.MCHardy, P.F.Sharp and J.V.Forrester "Automated detection of microaneurysms in digital red-free photographs: a diabetic retinopathy screening tool" *Diabetic Medicine*. 17 (2000) 588–594.

5. D. Fleming, S. Philip, K.A. Goatman, and J.A.Olson “Automated microaneurysm detection using local contrast normalization and local vessel detection” *IEEE Transactions on Medical Imaging*. 9 (2006) 1223–1232.
6. C.Sinthanayothin, J.Boyce and T.H.Williamson “Automated Detection of Diabetic Retinopathy on Digital Fundus Image” *Diabetic Medicine*. 19 (2002) 105–112.
7. D. Usher, M. Dumskyj and M. Himaga “Automated Detection of Diabetic Retinopathy in Digital Retinal Images: A Tool for Diabetic Retinopathy Screening” *Diabetic Medicine*. 21 (2002) 84–90.
8. M.S.Miri, and A. Mahloojifar “A Comparison Study to Evaluate Retinal Image Enhancement Techniques” *ICSIPA* (2009) 90 – 94.
9. A.Hoover, V. Kouznetsova, and M. Goldbaum "Locating blood vessels in retinal images by piecewise threshold probing of a matched filter response" *IEEE Trans. Med. Imaging*. 19 (2000) 203-210.
10. J. A. Stark “Adaptive Image Contrast Enhancement Using Generalizations of Histogram Equalization” *IEEE Transactions On Image Processing*. 9 (2000) 889-894.
11. W. Hsu, P. M. D. S. Pallawala, M. L. Lee and K.G. A. Eong “The Role of Domain Knowledge in the Detection of Retinal Hard Exudates” *CVPR*. (2001) 246-251.
12. R. C.Gonzalez, R. E.Woods, and S. L. Eddins “Digital Image processing using MATLAB”, 2nd Indian ed., Pearson Education 2005.
13. N.S.Datta, R.Sarkar,H.S.Dutta, and M.Dey “Software based automated early detection of diabetic retinopathy on non dilated retinal image through mathematical morphological process” *IJCA*. 60 (2012) 20-24.
14. A.Mead, S. Burnett, and C.Davey “Diabetic Retinopathy screen in the UK” *Journal of the Royal Society of medicine*. 94 (2001) 127-129.