


รายงานผลการดำเนินการ  
บำรุงรักษาเชิงป้องกันและสอบเทียบเครื่องมือแพทย์

โรงพยาบาลพญาไท พหลโยธิน

รอบเดือน เมษายน 2567


## สรุปผลการดำเนินการ

ลำดับ	รายละเอียด	จำนวน (เครื่อง)	หมายเหตุ
1	จำนวนเครื่องมือทั้งหมด	446	ตามเอกสารแนบ 1
2	ผลการสอบเทียบ		
	PASS	408	
	OUT OF RANGE	1	ตามเอกสารแนบ 2
3	ไม่สามารถดำเนินการ		ตามเอกสารแนบ 3
	DEFECTIVE	15	
	ยกเลิกออกจากแผนชั่วคราว	1	
	ยกเลิกการใช้งาน	3	
	หาเครื่องไม่พบ	18	
ดำเนินการแล้วทั้งหมด		446	




สรุปผลเครื่องมือที่ไม่ผ่านเกณฑ์การสอบเทียบ จำแนกตามเครื่องมือ

ชื่อเครื่องมือ	จำนวน
INFUSION PUMPS	1
ผลรวมทั้งหมด	1




สรุปผลเครื่องมือที่ไม่ผ่านเกณฑ์การสอบเทียบ จำแนกตามแผนก

ชื่อแผนก	จำนวน
Patient Wards 15	1
ผลรวมทั้งหมด	1

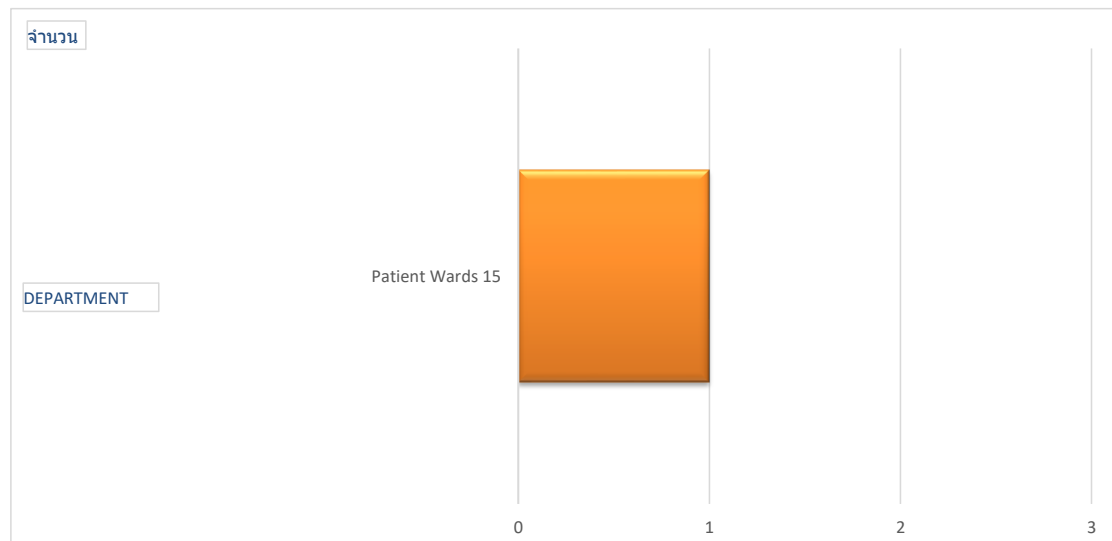

## สรุปผลเครื่องที่ไม่สามารถดำเนินการ จำแนกตามสถานะ

ชื่อสถานะ	จำนวน
DEFECTIVE	15
หาเครื่องไม่พบ	213
ยกเลิกการใช้งาน	22
บริษัทภายนอกดำเนินการ	94
BME	19
ติดใช้งาน	1
<b>ผลรวมทั้งหมด</b>	<b>364</b>



No.	ID CODE	Cer.No	PM.No	MEDICAL EQUIPMENT	BRAND	MODEL	S/N	DEPARTMENT	STATUS	REMARK
1	PTP02203	24PTP_0104240010	24PTP_01PM04240010	VENTILATORS, TRANSPORT	CAREFUSION	LTV 1200	E69078	Ambulance	PASS	
2	PTP02204	24PTP_0104240027	24PTP_01PM04240027	DEFIBRILLATORS, EXTERNAL, MANUAL	PHILIPS	HeartStart MRx (M3535A)	US00566825	Ambulance	PASS	Carbon Dioxide Concentration 5% (36.8 mmHg) ±2.6 mmHg = 37 mmHg Carbon Dioxide Concentration 10% (73.6 mmHg) ±5.2 mmHg = 75 mmHg
3	PTP02231	24PTP_0103240003	24PTP_01PM03240003	ASPIRATORS, EMERGENCY	OSCAR BOSCAROL	OB 2012	1101511782	Ambulance	PASS	
4	PTP02823	24PTP_0104240014	24PTP_01PM04240013	ASPIRATORS, EMERGENCY	OSCAR BOSCAROL	OB 2012	1101210862	Ambulance	PASS	
5	PTP00630	24PTP_0104240274	24PTP_01PM04240275	WARMING UNITS, PATIENT, RADIANT, INFANT	ATOM	V-3200N	2022864	Anesthesia	PASS	
6	PTP00680	24PTP_0104240342	24PTP_01PM04240344	ANESTHESIA UNITS	DATEX-OHMEDA	S/5 Aespire	AMXJ01250	Anesthesia	PASS	
7	PTP00680(VEN)	24PTP_0104240341	24PTP_01PM04240345	VENTILATORS, ANESTHESIA	DATEX-OHMEDA	S/5 Aespire	AMXJ01250	Anesthesia	PASS	
8	PTP00696	24PTP_0104240265	24PTP_01PM04240266	ANESTHESIA UNITS	DATEX-OHMEDA	S/5 Aespire	AMXK00324	Anesthesia	PASS	
9	PTP00696(VEN)	24PTP_0104240266	24PTP_01PM04240265	VENTILATORS, ANESTHESIA	DATEX-OHMEDA	S/5 Aespire	AMXK00324	Anesthesia	PASS	
10	PTP00697	24PTP_0104240299	24PTP_01PM04240299	MONITORS, BEDSIDE, PHYSIOLOGIC	NIHON KOHDEN	BSM-2303K	1369	Anesthesia	PASS	
11	PTP00727	24PTP_0104240349	24PTP_01PM04240352	MONITORS, BEDSIDE, PHYSIOLOGIC	NIHON KOHDEN	PVM-2701	103039	Anesthesia	PASS	
12	PTP00740	24PTP_0104240280	24PTP_01PM04240280	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	INTELLIVUE MP70(M8007A)	DE84381179	Anesthesia	PASS	
13	PTP00742	24PTP_0104240373	24PTP_01PM04240376	MODULE, ECG/SPO2/NIBP	PHILIPS	M3001A	DE632F8004	Anesthesia	PASS	MODULE OF ID Code : PTP00762
14	PTP00743	24PTP_0104240284	24PTP_01PM04240284	MODULE, IBP	PHILIPS	M1006B	3604G12969	Anesthesia	PASS	MODULE OF ID Code :PTP00740
15	PTP00748	-	-	MONITORS, PATIENT TRANSPORT	PHILIPS	INTELLIVUE X2(M3002A)	DE037A3403	Anesthesia	หาเครื่องมือไม่พบ	
16	PTP00749	24PTP_0104240283	24PTP_01PM04240283	MONITORS, PATIENT TRANSPORT	PHILIPS	INTELLIVUE X2(M3002A)	DE315C9789	Anesthesia	PASS	
17	PTP00759	24PTP_0104240291	24PTP_01PM04240294	MONITORS, BEDSIDE, PHYSIOLOGIC	NIHON KOHDEN	PVM-2701	4706	Anesthesia	PASS	
18	PTP00760	24PTP_0104240305	24PTP_01PM04240305	MONITORS, BEDSIDE, PHYSIOLOGIC	NIHON KOHDEN	PVM-2701	4710	Anesthesia	PASS	ไม่มีสาย EKG
19	PTP00761	24PTP_0104240304	24PTP_01PM04240304	MONITORS, BEDSIDE, PHYSIOLOGIC	NIHON KOHDEN	PVM-2701	4709	Anesthesia	PASS	
20	PTP00762	24PTP_0104240372	24PTP_01PM04240375	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	INTELLIVUE MP20(M8001A)	DE50406378	Anesthesia	PASS	ปุ่ม silence ข้างหู

No.	ID CODE	Cer.No	PM.No	MEDICAL EQUIPMENT	BRAND	MODEL	S/N	DEPARTMENT	STATUS	REMARK
21	PTP00764	24PTP_0104240293	24PTP_01PM04240292	MONITORS, BEDSIDE, PHYSIOLOGIC	NIHON KOHDEN	BSM-2303K	1126	Anesthesia	PASS	
22	PTP00765	24PTP_0104240374	24PTP_01PM04240377	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	INTELLIVUE MP20(M8001A)	DE50406334	Anesthesia	PASS	สาย SpO2 เป็อย
23	PTP00766	24PTP_0104240375	24PTP_01PM04240378	MODULE, ECG/SPO2/NIBP	PHILIPS	M3001A	DE51282425	Anesthesia	PASS	MODULE OF ID Code : PTP00765
24	PTP00767	24PTP_0104240370	24PTP_01PM04240373	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	INTELLIVUE MP20(M8001A)	DE50406324	Anesthesia	PASS	ปั้ม silence เริ่มเสื่อมสภาพ
25	PTP00768	24PTP_0104240371	24PTP_01PM04240374	MODULE, ECG/SPO2/NIBP	PHILIPS	M3001A	DE51282892	Anesthesia	PASS	MODULE OF ID Code : PTP00767
26	PTP00769	24PTP_0104240301	24PTP_01PM04240301	WARMING UNITS, PATIENT, FORCED-AIR	BAIR HUGGER	505	74895	Anesthesia	PASS	
27	PTP00770	24PTP_0104240300	24PTP_01PM04240300	WARMING UNITS, PATIENT, FORCED-AIR	BAIR HUGGER	505	74894	Anesthesia	PASS	
28	PTP00771	24PTP_0104240264	24PTP_01PM04240264	WARMING UNITS, PATIENT, FORCED-AIR	BAIR HUGGER	775	85703	Anesthesia	PASS	
29	PTP02945	-	-	INFUSION PUMPS, ANALGESIC, PATIENT-CONTROLLED	AITECS	SP-14S	7907	Anesthesia	ยกเลิกการใช้งาน	
30	PTP03459	-	-	MODULE, CO2/TEMP	PHILIPS	M3014A	DE61414205	Anesthesia	หาเครื่องไม่พบ	
31	PTP03472	24PTP_0104240361	24PTP_01PM04240363	MODULE, ECG/SPO2/NIBP	PHILIPS	M3001A	DE632E9412	Anesthesia	PASS	MODULE OF ID Code :PTP01162
32	PTP03488	24PTP_0104240096	24PTP_01PM04240096	INFUSION PUMPS, ANALGESIC, PATIENT-CONTROLLED	B BRAUN	PERFUSOR SPACE	472033	Anesthesia	PASS	
33	PTP03489	24PTP_0104240095	24PTP_01PM04240095	INFUSION PUMPS, ANALGESIC, PATIENT-CONTROLLED	B BRAUN	PERFUSOR SPACE	472039	Anesthesia	PASS	
34	PTP03566	24PTP_0104240287	24PTP_01PM04240287	OXIMETERS, PULSE	COVIDIEN	PM10N	-	Anesthesia	PASS	
35	PTP03567	24PTP_0104240289	24PTP_01PM04240289	OXIMETERS, PULSE	COVIDIEN	PM10N	-	Anesthesia	PASS	
36	PTP00204	24PTP_0104240345	24PTP_01PM04240350	OXIMETERS, PULSE	NOVAMETRIX	515A	79-1538TPR	BME-PTP	PASS	
37	PTP03286	24PTP_0104240323	24PTP_01PM04240326	SPHYGMOMANOMETERS, ELECTRONIC, AUTOMATIC	OMRON	HEM-907	20071100093AF	BME-PTP	PASS	
38	PTP03563	-	-	MONITORS, PHYSIOLOGIC, VITAL SIGNS	CRITICARE	506DN	113054816	BME-PTP	หาเครื่องไม่พบ	
39	PTP04021	24PTP_0104240327	24PTP_01PM04240330	OXIMETERS, PULSE	-	-	-	BME-PTP	PASS	
40	PTP04035	24PTP_0104240393	24PTP_01PM04240396	OXIMETERS, PULSE	-	-	-	BME-PTP	PASS	
41	PTP04072	24PTP_0104240085	24PTP_01PM04240085	OXIMETERS, PULSE	-	-	-	BME-PTP	PASS	
42	PTP04144	24PTP_0104240385	24PTP_01PM04240388	OXIMETERS, PULSE	-	-	-	BME-PTP	PASS	
43	PTP04165	24PTP_0104240384	24PTP_01PM04240387	OXIMETERS, PULSE	-	-	-	BME-PTP	PASS	
44	PTP04209	-	-	OXIMETERS, PULSE	-	-	-	BME-PTP	หาเครื่องไม่พบ	
45	PTP04211	-	-	OXIMETERS, PULSE	-	-	-	BME-PTP	หาเครื่องไม่พบ	
46	PTP04228	-	-	OXIMETERS, PULSE	-	-	-	BME-PTP	หาเครื่องไม่พบ	
47	PTP04627	24PTP_0104240197	24PTP_01PM04240196	ASPIRATORS, EMERGENCY	SOLIDA	9E-B	MA23020460053	BME-PTP	PASS	

No.	ID CODE	Cer.No	PM.No	MEDICAL EQUIPMENT	BRAND	MODEL	S/N	DEPARTMENT	STATUS	REMARK
48	PTP01955	24PTP_0104240199	24PTP_01PM04240192	MONITORS, PHYSIOLOGIC, VITAL SIGNS	CASMED	740 SELECT	CFD01304	Bone & Joint	PASS	
49	PTP03736	24PTP_0104240313	24PTP_01PM04240316	CENTRIFUGES, TABLETOP, LOW-SPEED	YINGTAI	TD5	24122010687	Bone & Joint	PASS	
50	PTP03868	-	-	OXIMETERS, PULSE	STRONG	703F	703F-8007008	Bone & Joint	หาเครื่องไม่พบ	
51	PTP04619	24PTP_0104240397	24PTP_01PM04240400	MONITORS, PHYSIOLOGIC, VITAL SIGNS	WELCH ALLYN	CONNEX SPOT MONITOR	100073962020	Bone & Joint	PASS	
52	PTP01788	24PTP_0104240381	24PTP_01PM04240384	MONITORS, BEDSIDE, PHYSIOLOGIC	NIHON KOHDEN	BSM-6301K	4872	Cardio-Neuro Vascular Intervention	PASS	
53	PTP01789	24PTP_0104240382	24PTP_01PM04240385	MODULE, ECG/SPO2/NIBP/IBP/TEMP	NIHON KOHDEN	AY-661P	3180	Cardio-Neuro Vascular Intervention	PASS	MODULE OF ID Code :PTP01788
54	PTP01795	-	-	ANESTHESIA UNITS	DATEX-OHMEDA	AESPIRE	AMX10110153WA	Cardio-Neuro Vascular Intervention	DEFECTIVE	ค่า PEEP ที่ตั้งกับค่าที่เครื่องจ่ายต่างกันเกิน 10%
55	PTP01798	-	-	INJECTORS, CONTRAST MEDIA	LIEBEL-FLARSHEIM	LF	C10111C011	Cardio-Neuro Vascular Intervention	ยกเลิกการใช้งาน	
56	PTP03902	24PTP_0104240383	24PTP_01PM04240386	PACEMAKERS, CARDIAC, EXTERNAL	ST. JUDE MEDICAL	3077	206147	Cardio-Neuro Vascular Intervention	PASS	
57	PTP01707	24PTP_0104240008	24PTP_01PM04240009	MONITORS, PHYSIOLOGIC, VITAL SIGNS	KTMED	KTPM-1000	ZH1100157	Check Up Center	PASS	
58	PTP01723	24PTP_0104240335	24PTP_01PM04240338	MONITORS, PHYSIOLOGIC, VITAL SIGNS	CASMED	740 SELECT	1526308	Check Up Center	PASS	
59	PTP02981	24PTP_0104240258	24PTP_01PM04240258	THERMOMETERS, ELECTRONIC, INFRARED, SKIN	MICROLIFE	FR1MF1	04160881	Check Up Center	PASS	
60	PTP03305	24PTP_0104240394	24PTP_01PM04240397	THERMOMETERS, ELECTRONIC, INFRARED, SKIN	MICROLIFE	FR1DL1	-	Check Up Center	PASS	
61	PTP03477	24PTP_0104240004	24PTP_01PM04240004	MONITORS, PHYSIOLOGIC, VITAL SIGNS	WELCH ALLYN	CONNEX SPOT MONITOR	100085383617	Check Up Center	PASS	
62	PTP03478	24PTP_0104240209	24PTP_01PM04240209	MONITORS, PHYSIOLOGIC, VITAL SIGNS	WELCH ALLYN	CONNEX SPOT MONITOR	100085673617	Check Up Center	PASS	
63	PTP03479	24PTP_0104240219	24PTP_01PM04240220	MONITORS, PHYSIOLOGIC, VITAL SIGNS	WELCH ALLYN	CONNEX SPOT MONITOR	100082643617	Check Up Center	PASS	
64	PTP03490	-	-	MONITORS, PHYSIOLOGIC, VITAL SIGNS	KTMED	KTPM-1000	-	Check Up Center	หาเครื่องไม่พบ	
65	PTP03788	24PTP_0104240333	24PTP_01PM04240335	MONITORS, PHYSIOLOGIC, VITAL SIGNS	WELCH ALLYN	CONNEX SPOT MONITOR	100073742020	Check Up Center	PASS	
66	PTP03791	24PTP_0104240222	24PTP_01PM04240223	MONITORS, PHYSIOLOGIC, VITAL SIGNS	WELCH ALLYN	CONNEX SPOT MONITOR	100073822020	Check Up Center	PASS	
67	PTP03849	24PTP_0104240395	24PTP_01PM04240398	MONITORS, PHYSIOLOGIC, VITAL SIGNS	EDAN	M3A	360125-M21505660014	Check Up Center	PASS	



No.	ID CODE	Cer.No	PM.No	MEDICAL EQUIPMENT	BRAND	MODEL	S/N	DEPARTMENT	STATUS	REMARK
68	PTP03850	24PTP_0104240336	24PTP_01PM04240339	MONITORS, PHYSIOLOGIC, VITAL SIGNS	EDAN	M3A	360125-M21505660013	Check Up Center	PASS	
69	PTP03851	-	-	MONITORS, PHYSIOLOGIC, VITAL SIGNS	EDAN	M3A	360125-M21505660012	Check Up Center	หาเครื่องมือพบ	
70	PTP03903	24PTP_0104240309	24PTP_01PM04240310	MONITORS, PHYSIOLOGIC, VITAL SIGNS	KTMED	KTPM-1000	ZC1100111	Check Up Center	PASS	Battery เสื่อมสภาพ
71	PTP04484	24PTP_0104240401	24PTP_01PM04240404	OXIMETERS, PULSE	-	-	-	Check Up Center	PASS	
72	PTP04524	24PTP_0104240334	24PTP_01PM04240337	MONITORS, PHYSIOLOGIC, VITAL SIGNS	WELCH ALLYN	CONNEX SPOT MONITOR	100098351219	Check Up Center	PASS	
73	PTP04525	24PTP_0104240331	24PTP_01PM04240334	MONITORS, PHYSIOLOGIC, VITAL SIGNS	WELCH ALLYN	CONNEX SPOT MONITOR	100098441219	Check Up Center	PASS	
74	PTP04634	24PTP_0104240378	24PTP_01PM04240381	SPHYGMOMANOMETERS, ELECTRONIC, AUTOMATIC	OMRON	HEM-907	20141000086AF	Check Up Center	PASS	
75	PTP04802	24PTP_0104240271	24PTP_01PM04240271	MONITORS, PHYSIOLOGIC, VITAL SIGNS	CRITICARE	506DN	113054323	Check Up Center	PASS	สาย SpO2 เกือบเสื่อมสภาพ
76	PTP02122	24PTP_0104240306	24PTP_01PM04240307	STERILIZING UNITS, STEAM, TABLETOP	EURONDA	E9 MED	EHD160786	Dental & Implant Center	PASS	
77	PTP02123	24PTP_0104240307	24PTP_01PM04240308	STERILIZING UNITS, STEAM, TABLETOP	EURONDA	E9 MED	EHD160782	Dental & Implant Center	PASS	
78	PTP03481	24PTP_0104240221	24PTP_01PM04240222	MONITORS, PHYSIOLOGIC, VITAL SIGNS	WELCH ALLYN	CONNEX SPOT MONITOR	100019052317	Dental & Implant Center	PASS	
79	PTP04700	24PTP_0104240319	24PTP_01PM04240321	OXIMETERS, PULSE	-	SO911	-	Dental & Implant Center	PASS	
80	PTP04701	24PTP_0104240317	24PTP_01PM04240320	OXIMETERS, PULSE	-	SO911	-	Dental & Implant Center	PASS	
81	PTP04702	24PTP_0104240320	24PTP_01PM04240322	OXIMETERS, PULSE	-	SO911	-	Dental & Implant Center	PASS	
82	PTP03287	24PTP_0104240386	24PTP_01PM04240389	OXIMETERS, PULSE	KTMED	OXYPLAM	LK1401902	Diabetes Mellitus & Endocrine Center	PASS	
83	PTP02177	24PTP_0104240006	24PTP_01PM04240005	DEFIBRILLATORS, EXTERNAL, MANUAL	PHILIPS	HeartStart MRx (M3535A)	US00568018	Emergency & Ambulance	PASS	Carbon Dioxide Concentration 5% (36.8 mmHg) ±2.6 mmHg = 35 mmHg Carbon Dioxide Concentration 10% (73.6 mmHg) ±5.2 mmHg = 77 mmHg
84	PTP02178	24PTP_0104240015	24PTP_01PM04240014	VENTILATORS, TRANSPORT	CAREFUSION	LTV 1200	E71822	Emergency & Ambulance	PASS	
85	PTP02179	24PTP_0104240012	24PTP_01PM04240011	VENTILATORS, TRANSPORT	CAREFUSION	LTV 1200	E71849	Emergency & Ambulance	PASS	
86	PTP02188	24PTP_0104240009	24PTP_01PM04240008	DEFIBRILLATORS, EXTERNAL, AUTOMATED	ZOLL	AED PLUS	X151784217	Emergency & Ambulance	PASS	
87	PTP02189	24PTP_0104240007	24PTP_01PM04240006	DEFIBRILLATORS, EXTERNAL, AUTOMATED	ZOLL	AED PLUS	X151784468	Emergency & Ambulance	PASS	
88	PTP02196	-	-	MONITORS, PHYSIOLOGIC, VITAL SIGNS	CRITICARE	506DN	113054331	Emergency & Ambulance	DEFECTIVE	ส่งซ่อม
89	PTP02197	24PTP_0104240058	24PTP_01PM04240057	INFUSION PUMPS, SYRINGE	TERUMO	TE-331	1212000306	Emergency & Ambulance	PASS	

No.	ID CODE	Cer.No	PM.No	MEDICAL EQUIPMENT	BRAND	MODEL	S/N	DEPARTMENT	STATUS	REMARK
90	PTP02200	24PTP_0104240026	24PTP_01PM04240026	MONITORS, PHYSIOLOGIC, VITAL SIGNS	CRITICARE	506DN	113054335	Emergency & Ambulance	PASS	
91	PTP02323	-	-	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	INTELLIVUE MP20(M8001A)	DE62221474	Emergency & Ambulance	DEFECTIVE	ส่งซ่อมกับทางบริษัท
92	PTP02324	24PTP_0104240029	24PTP_01PM04240029	MODULE, ECG/SPO2/NIBP	PHILIPS	M3001A	DE632F7996	Emergency & Ambulance	PASS	MODULE OF ID Code :PTP00317
93	PTP02330	24PTP_0104240013	24PTP_01PM04240015	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	INTELLIVUE MP20(M8001A)	DE62221470	Emergency & Ambulance	PASS	
94	PTP02331	24PTP_0104240354	24PTP_01PM04240356	MODULE, ECG/SPO2/NIBP	PHILIPS	M3001A	DE717L8969	Emergency & Ambulance	PASS	MODULE OF ID Code :PTP00403
95	PTP02335	24PTP_0104240022	24PTP_01PM04240023	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	INTELLIVUE MP20(M8001A)	DE62221532	Emergency & Ambulance	PASS	
96	PTP02336	24PTP_0104240025	24PTP_01PM04240025	MODULE, ECG/SPO2/NIBP	PHILIPS	M3001A	DE632F8007	Emergency & Ambulance	PASS	MODULE OF ID Code :PTP02335
97	PTP02338	24PTP_0104240030	24PTP_01PM04240065	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	INTELLIVUE MP20(M8001A)	DE62221450	Emergency & Ambulance	PASS	
98	PTP02339	24PTP_0104240066	24PTP_01PM04240066	MODULE, ECG/SPO2/NIBP	PHILIPS	M3001A	DE717L8995	Emergency & Ambulance	PASS	MODULE OF ID Code :PTP02338
99	PTP02343	24PTP_0104240020	24PTP_01PM04240020	MODULE, ECG/SPO2/NIBP	PHILIPS	M3001A	DE9070C8M0	Emergency & Ambulance	PASS	MODULE OF ID Code :PTP02344
100	PTP02344	24PTP_0104240018	24PTP_01PM04240018	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	INTELLIVUE MP20(M8001A)	DE62221543	Emergency & Ambulance	PASS	
101	PTP02352	24PTP_0104240033	24PTP_01PM04240032	INFUSION PUMPS	TOP	TOP-2200	ELZ8612S	Emergency & Ambulance	PASS	Battery เสื่อมสภาพ
102	PTP02353	24PTP_0104240063	24PTP_01PM04240062	INFUSION PUMPS	B BRAUN	INFUSOMAT SPACE P	338499	Emergency & Ambulance	PASS	
103	PTP02354	24PTP_0104240065	24PTP_01PM04240064	INFUSION PUMPS	B BRAUN	INFUSOMAT SPACE P	304466	Emergency & Ambulance	PASS	
104	PTP02355	24PTP_0104240062	24PTP_01PM04240061	INFUSION PUMPS	B BRAUN	INFUSOMAT SPACE P	306228	Emergency & Ambulance	PASS	
105	PTP02356	24PTP_0104240061	24PTP_01PM04240060	INFUSION PUMPS, SYRINGE	B BRAUN	PERFUSOR SPACE	295121	Emergency & Ambulance	PASS	
106	PTP01385	24PTP_0104240105	24PTP_01PM04240105	MONITORS, PHYSIOLOGIC, VITAL SIGNS	Heal Force	CLASSIC-90	J2600JG00498	Eye Ear Nose Throat Clinic	PASS	
107	PTP03495	24PTP_0104240352	24PTP_01PM04240354	ELECTROSURGICAL UNITS, MONOPOLAR/BIPOLAR	MEYER-HAAKE	RADIOSURG 2200	3480	Eye Ear Nose Throat Clinic	PASS	
108	PTP01092	24PTP_0104240355	24PTP_01PM04240358	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	INTELLIVUE MP20(M8001A)	DE62221524	Gastrointestinal & Liver Center	PASS	
109	PTP01093	24PTP_0104240366	24PTP_01PM04240369	MONITORS, PHYSIOLOGIC, VITAL SIGNS	PHILIPS	SURESIGNS VM4	US90328518	Gastrointestinal & Liver Center	PASS	ไม่มีสาย EKG
110	PTP01094	24PTP_0104240365	24PTP_01PM04240368	MONITORS, PHYSIOLOGIC, VITAL SIGNS	PHILIPS	SURESIGNS VM4	US90328541	Gastrointestinal & Liver Center	PASS	ไม่มีสาย EKG, หน้าจอเป็นเส้น
111	PTP01122	24PTP_0104240362	24PTP_01PM04240365	MONITORS, BEDSIDE, PHYSIOLOGIC	NIHON KOHDEN	PVM-2701	6932	Gastrointestinal & Liver Center	PASS	


No.	ID CODE	Cer.No	PM.No	MEDICAL EQUIPMENT	BRAND	MODEL	S/N	DEPARTMENT	STATUS	REMARK
112	PTP01123	-	-	ELECTROSURGICAL UNITS	ERBE	ICC 200	D-2193	Gastrointestinal & Liver Center	DEFFECTIVE	ค่า HF Leakage สูงกว่าเกณฑ์, Mode Bipolar ตั้งแต่ค่า 50 ลงมาต่ำกว่าเกณฑ์
113	PTP01136	24PTP_0104240367	24PTP_01PM04240370	ELECTROSURGICAL UNITS, MONOPOLAR, ARGON-ENHANCED COAGULATION	ERBE	APC 2	11362015	Gastrointestinal & Liver Center	PASS	
114	PTP01162	24PTP_0104240359	24PTP_01PM04240362	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	INTELLIVUE MP20(M8001A)	DE72832658	Gastrointestinal & Liver Center	PASS	ปุ่ม Silence ชำรุด
115	PTP01163	-	-	MODULE, ECG/SPO2/NIBP	PHILIPS	M3001A	DE632F7960	Gastrointestinal & Liver Center	หาเครื่องไม่พบ	
116	PTP03458	24PTP_0104240357	24PTP_01PM04240360	MODULE, ECG/SPO2/NIBP/IBP/TEMP	PHILIPS	M3001A	DE632F7999	Gastrointestinal & Liver Center	PASS	MODULE OF ID Code :PTP01092
117	PTP01650	24PTP_0104240005	24PTP_01PM04240007	MONITORS, PHYSIOLOGIC, VITAL SIGNS	MINDRAY	VS-900	FV-63010443	General Medicine	PASS	
118	PTP01651	24PTP_0104240325	24PTP_01PM04240327	MONITORS, PHYSIOLOGIC, VITAL SIGNS	PHILIPS	SURESIGNS VSI	CN42718758	General Medicine	PASS	
119	PTP01769	24PTP_0104240067	24PTP_01PM04240067	MONITORS, PHYSIOLOGIC, VITAL SIGNS	KTMED	KTPM-1000	ZD1100125	General Medicine	PASS	
120	PTP01779	24PTP_0104240038	24PTP_01PM04240037	INFUSION PUMPS	TOP	TOP-2200	JLY5014S	General Medicine	PASS	
121	PTP01782	24PTP_0104240068	24PTP_01PM04240068	MONITORS, PHYSIOLOGIC, VITAL SIGNS	KTMED	KTPM-1000	ZB1200215	General Medicine	PASS	
122	PTP01783	24PTP_0104240232	24PTP_01PM04240233	MONITORS, PHYSIOLOGIC, VITAL SIGNS	PHILIPS	SURESIGNS VSI	CN42717207	General Medicine	PASS	
123	PTP03082	24PTP_0104240377	24PTP_01PM04240380	THERMOMETERS, ELECTRONIC, INFRARED, SKIN	MICROLIFE	FR1DL1	-	General Medicine	PASS	
124	PTP03473	24PTP_0104240235	24PTP_01PM04240236	MONITORS, PHYSIOLOGIC, VITAL SIGNS	WELCH ALLYN	CONNEX SPOT MONITOR	100091401717	General Medicine	PASS	
125	PTP03480	24PTP_0104240011	24PTP_01PM04240012	MONITORS, PHYSIOLOGIC, VITAL SIGNS	WELCH ALLYN	CONNEX SPOT MONITOR	100015354217	General Medicine	PASS	
126	PTP03482	24PTP_0104240003	24PTP_01PM04240003	MONITORS, PHYSIOLOGIC, VITAL SIGNS	WELCH ALLYN	CONNEX SPOT MONITOR	100019092317	General Medicine	PASS	
127	PTP04587	24PTP_0104240002	24PTP_01PM04240002	OXIMETERS, PULSE	CONTEC	CMS50D1	21050201004	General Medicine	PASS	
128	PLP03861	24PTP_0104240322	24PTP_01PM04240324	VASCULAR SCREENING UNIT (ABI)	FUKUDA DENSHI	VASERA VS-2000	50300417	General Surgery	PASS	
129	PTP01899	24PTP_0104240358	24PTP_01PM04240361	MONITORS, PHYSIOLOGIC, VITAL SIGNS	KTMED	KTPM-1000	ZD1100127	General Surgery	PASS	
130	PTP01900	24PTP_0104240339	24PTP_01PM04240342	MONITORS, PHYSIOLOGIC, VITAL SIGNS	KTMED	KTPM-1000	ZD1100128	General Surgery	PASS	
131	PTP01915	24PTP_0104240312	24PTP_01PM04240315	ELECTROSURGICAL UNITS, MONOPOLAR	WEM	SS-501E	174	General Surgery	PASS	

No.	ID CODE	Cer.No	PM.No	MEDICAL EQUIPMENT	BRAND	MODEL	S/N	DEPARTMENT	STATUS	REMARK
132	PTP02184	-	24PTP_01PM04240219	SCANNING SYSTEMS, ULTRASONIC, GENERAL-PURPOSE	GE HEALTHCARE	VIVID I	020279V1	General Surgery	PASS	
133	PTP03700	24PTP_0104240234	24PTP_01PM04240235	OXIMETERS, PULSE	FINGER PULSE OXIMETER	703F	703F8GA00688	General Surgery	PASS	
134	PTP04580	24PTP_0104240233	24PTP_01PM04240234	MONITORS, PHYSIOLOGIC, VITAL SIGNS	WELCH ALLYN	CONNEX SPOT MONITOR	21100098411219	General Surgery	PASS	
135	PTP00991	24PTP_0104240230	24PTP_01PM04240231	DEFIBRILLATORS, EXTERNAL, MANUAL	PHILIPS	HeartStart XL (M4735A)	US00466991	Heart Center	PASS	
136	PTP00994	24PTP_0104240369	24PTP_01PM04240372	EXERCISERS, AEROBIC, TREADMILL	QUINTON	Q-STRESS TM55	QS006616	Heart Center	PASS	
137	PTP00997	24PTP_0104240060	24PTP_01PM04240059	INFUSION PUMPS	TOP	TOP-2200	GLY2351S	Heart Center	PASS	
138	PTP01000	24PTP_0104240231	24PTP_01PM04240232	MONITORS, PHYSIOLOGIC, VITAL SIGNS	PHILIPS	SURESIGNS VSI	CN42717094	Heart Center	PASS	
139	PTP01006	24PTP_0104240332	24PTP_01PM04240336	EXERCISERS, AEROBIC, TREADMILL	QUINTON	Q-STRESS TM55	QS007226	Heart Center	PASS	
140	PTP01016	24PTP_0104240218	24PTP_01PM04240218	MONITORS, PHYSIOLOGIC, VITAL SIGNS	COLIN	DUXEO BX-10	11509	Heart Center	PASS	ปุ่มวัด NIBP ขาด, หน้าจอเสื่อมสภาพ, Battery เสื่อมสภาพ
141	PTP01041	24PTP_0104240216	24PTP_01PM04240216	MONITORS, PHYSIOLOGIC, VITAL SIGNS	KTMED	KTPM-1000	ZC1100110	Heart Center	PASS	สาย SpO2 เสื่อมสภาพ
142	PTP03896	24PTP_0104240368	24PTP_01PM04240371	MONITORING SYSTEMS, PHYSIOLOGIC, STRESS EXERCISE, CARDIAC	QUINTON	Q-STRESS	121110000831	Heart Center	PASS	
143	PTP04523	24PTP_0104240217	24PTP_01PM04240217	MONITORS, PHYSIOLOGIC, VITAL SIGNS	WELCH ALLYN	CONNEX SPOT MONITOR	100098421219	Heart Center	PASS	
144	PLP02512	24PTP_0104240182	24PTP_01PM04240182	MODULE, ECG/SPO2/NIBP	PHILIPS	M3001A	DE83753521	I.C.U	PASS	MODULE OF ID Code : PTP00311
145	PTP00077	24PTP_0104240184	24PTP_01PM04240184	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	INTELLIVUE MP20(M8001A)	DE62221467	I.C.U	PASS	
146	PTP00217	24PTP_0104240165	24PTP_01PM04240167	VENTILATORS, TRANSPORT	FLIGHT MEDICAL	FLIGHT 60	V61-0012	I.C.U	PASS	
147	PTP00218	24PTP_0104240111	24PTP_01PM04240111	VENTILATORS, INTENSIVE CARE	CAREFUSION	VELA	BDT02140	I.C.U	PASS	
148	PTP00255	24PTP_0104240054	24PTP_01PM04240053	INFUSION PUMPS, SYRINGE	TERUMO	TE-311	1111000499	I.C.U	PASS	Battery เสื่อมสภาพ
149	PTP00258	24PTP_0104240114	24PTP_01PM04240114	VENTILATORS, INTENSIVE CARE	CAREFUSION	VELA	BFT01867	I.C.U	PASS	
150	PTP00259	24PTP_0104240127	24PTP_01PM04240125	VENTILATORS, INTENSIVE CARE	CAREFUSION	VELA	BFT02392	I.C.U	PASS	
151	PTP00260	24PTP_0104240113	24PTP_01PM04240113	VENTILATORS, INTENSIVE CARE	CAREFUSION	VELA	BFT01674	I.C.U	PASS	O2 sensor failed
152	PTP00261	24PTP_0104240321	24PTP_01PM04240325	VENTILATORS, INTENSIVE CARE	PURITAN BENNETT	840	3512123690	I.C.U	PASS	


No.	ID CODE	Cer.No	PM.No	MEDICAL EQUIPMENT	BRAND	MODEL	S/N	DEPARTMENT	STATUS	REMARK
153	PTP00262	24PTP_0104240203	24PTP_01PM04240203	VENTILATORS, INTENSIVE CARE	PURITAN BENNETT	840	3510073348	I.C.U	PASS	
154	PTP00263	24PTP_0104240110	24PTP_01PM04240110	VENTILATORS, INTENSIVE CARE	PURITAN BENNETT	840	3510070748	I.C.U	PASS	
155	PTP00265	24PTP_0104240162	24PTP_01PM04240164	VENTILATORS, INTENSIVE CARE	PURITAN BENNETT	840	3510103598	I.C.U	PASS	
156	PTP00278	24PTP_0104240129	24PTP_01PM04240128	VENTILATORS, INTENSIVE CARE	CAREFUSION	VELA	BFT02553	I.C.U	PASS	O2 sensor failed
157	PTP00279	24PTP_0103240002	24PTP_01PM03240002	VENTILATORS, INTENSIVE CARE	CAREFUSION	VELA	BFT01189	I.C.U	PASS	
158	PTP00280	24PTP_0104240112	24PTP_01PM04240112	VENTILATORS, INTENSIVE CARE	CAREFUSION	VELA	BFT01893	I.C.U	PASS	
159	PTP00287	24PTP_0104240056	24PTP_01PM04240055	INFUSION PUMPS, SYRINGE	TERUMO	TE-331	1207000232	I.C.U	PASS	
160	PTP00288	24PTP_0104240121	24PTP_01PM04240121	INFUSION PUMPS, SYRINGE	TERUMO	TE-331	1207000232	I.C.U	PASS	
161	PTP00293	24PTP_0104240167	24PTP_01PM04240169	INFUSION PUMPS	TOP	TOP-2200	JLY4967	I.C.U	PASS	
162	PTP00294	24PTP_0104240152	24PTP_01PM04240152	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	INTELLIVUE MX450	DE35148458	I.C.U	PASS	
163	PTP00295	24PTP_0104240125	24PTP_01PM04240126	MODULE, ECG/SPO2/NIBP	PHILIPS	M3001A	DE5630FGRY	I.C.U	PASS	MODULE OF ID Code :PTP00454
164	PTP00296	24PTP_0104240188	24PTP_01PM04240188	MODULE, ECG/SPO2/NIBP	PHILIPS	M3001A	DE83732001	I.C.U	PASS	Carbon Dioxide Concentration 5% (36.8 mmHg) ±2.6 mmHg Carbon Dioxide Concentration 10% (73.6 mmHg) ±5.2 mmHg, MODULE OF ID Code :PTP02717
165	PTP00305	-	-	DEFIBRILLATORS, EXTERNAL, MANUAL	PHILIPS	HeartStart XL+ (861290)	US71514172	I.C.U	DEFECTIVE	ส่งซ่อมกับทางบริษัท
166	PTP00306	24PTP_0104240183	24PTP_01PM04240183	DEFIBRILLATORS, EXTERNAL, MANUAL	PHILIPS	EFFICIA DFM100	CN32605631	I.C.U	PASS	
167	PTP00307	24PTP_0104240118	24PTP_01PM04240120	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	INTELLIVUE MP20(M8001A)	DE72876242	I.C.U	PASS	
168	PTP00308	24PTP_0104240159	24PTP_01PM04240160	MODULE, ECG/SPO2/NIBP	PHILIPS	M3001A	DE632F7955	I.C.U	PASS	MODULE OF ID Code : PTP00309
169	PTP00309	24PTP_0104240160	24PTP_01PM04240159	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	INTELLIVUE MP20(M8001A)	DE72832648	I.C.U	PASS	
170	PTP00310	24PTP_0104240171	24PTP_01PM04240173	MODULE, ECG/SPO2/NIBP	PHILIPS	M3001A	DE717L9005	I.C.U	PASS	MODULE OF ID Code :PTP00372
171	PTP00311	24PTP_0104240180	24PTP_01PM04240180	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	INTELLIVUE MP20(M8001A)	DE50406347	I.C.U	PASS	
172	PTP00312	24PTP_0104240193	24PTP_01PM04240194	MODULE, ECG/SPO2/NIBP	PHILIPS	M3001A	DE9070C8LM	I.C.U	PASS	MODULE OF ID Code :PTP00184
173	PTP00314	24PTP_0104240198	24PTP_01PM04240199	MODULE, ECG/SPO2/NIBP	PHILIPS	M3001A	DE4680E2M8	I.C.U	PASS	MODULE OF ID Code :PTP00315
174	PTP00315	24PTP_0104240196	24PTP_01PM04240198	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	INTELLIVUE MP20(M8001A)	DE62221444	I.C.U	PASS	
175	PTP00316	24PTP_0104240187	24PTP_01PM04240187	MODULE, ECG/SPO2/NIBP	PHILIPS	M3001A	DE9070A3GJ	I.C.U	PASS	MODULE OF ID Code :PTP02717
176	PTP00317	24PTP_0104240028	24PTP_01PM04240028	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	INTELLIVUE MP20(M8001A)	DE72832664	I.C.U	PASS	

No.	ID CODE	Cer.No	PM.No	MEDICAL EQUIPMENT	BRAND	MODEL	S/N	DEPARTMENT	STATUS	REMARK
177	PTP00319	24PTP_0104240185	24PTP_01PM04240185	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	INTELLIVUE MP20(M8001A)	DE62221472	I.C.U	PASS	
178	PTP00320	24PTP_0104240201	24PTP_01PM04240201	MODULE, ECG/SPO2/NIBP	PHILIPS	M3001A	DE717M0430	I.C.U	PASS	MODULE OF ID Code :PTP00471
179	PTP00321	24PTP_0104240173	24PTP_01PM04240162	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	INTELLIVUE MP20(M8001A)	DE62221455	I.C.U	PASS	
180	PTP00322	24PTP_0104240330	24PTP_01PM04240333	MODULE, ECG/SPO2/NIBP	PHILIPS	M3001A	DE9070C8LU	I.C.U	PASS	MODULE OF ID Code :PTP02728
181	PTP00323	24PTP_0104240151	24PTP_01PM04240151	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	INTELLIVUE MP20(M8001A)	DE62221442	I.C.U	PASS	
182	PTP00359	24PTP_0104240057	24PTP_01PM04240056	INFUSION PUMPS, SYRINGE	TERUMO	TE-331	1111000517	I.C.U	PASS	
183	PTP00360	24PTP_0104240017	24PTP_01PM04240017	INFUSION PUMPS	TOP	TOP-2300	15A0039	I.C.U	PASS	
184	PTP00361	24PTP_0104240092	24PTP_01PM04240092	INFUSION PUMPS	B BRAUN	INFUSOMAT SPACE P	370070	I.C.U	PASS	
185	PTP00362	24PTP_0104240119	24PTP_01PM04240119	INFUSION PUMPS, SYRINGE	B BRAUN	PERFUSOR SPACE	305925	I.C.U	PASS	
186	PTP00363	24PTP_0104240090	24PTP_01PM04240090	INFUSION PUMPS, SYRINGE	B BRAUN	PERFUSOR SPACE	311447	I.C.U	PASS	
187	PTP00365	-	24PTP_01PM04240311	SCANNING SYSTEMS, ULTRASONIC, GENERAL-PURPOSE	GE HEALTHCARE	VIVID S5	0197VS5	I.C.U	PASS	
188	PTP00368	24PTP_0104240194	24PTP_01PM04240195	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	INTELLIVUE MP20(M8001A)	DE72876246	I.C.U	PASS	
189	PTP00369	24PTP_0104240116	24PTP_01PM04240116	MODULE, ECG/SPO2/NIBP	PHILIPS	M3001A	DE907L3232	I.C.U	PASS	MODULE OF ID Code :PTP02485
190	PTP00370	24PTP_0104240153	24PTP_01PM04240153	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	INTELLIVUE MP20(M8001A)	DE72832656	I.C.U	PASS	
191	PTP00371	24PTP_0104240149	24PTP_01PM04240149	MODULE, ECG/SPO2/NIBP	PHILIPS	M3001A	DE632F7995	I.C.U	PASS	MODULE OF ID Code : PTP01971
192	PTP00372	24PTP_0104240170	24PTP_01PM04240172	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	INTELLIVUE MP20(M8001A)	DE62221515	I.C.U	PASS	
193	PTP00373	24PTP_0104240128	24PTP_01PM04240129	MODULE, ECG/SPO2/NIBP	PHILIPS	M3001A	DE632F7985	I.C.U	PASS	MODULE OF ID Code :PTP00403
194	PTP00377	24PTP_0104240211	24PTP_01PM04240211	INFUSION PUMPS	TOP	TOP-2200	JLX4915	I.C.U	PASS	
195	PTP00379	24PTP_0104240046	24PTP_01PM04240045	INFUSION PUMPS	TOP	TOP-2300	15A0144	I.C.U	PASS	
196	PTP00380	24PTP_0104240158	24PTP_01PM04240157	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	INTELLIVUE MP20(M8001A)	DE72832639	I.C.U	PASS	
197	PTP00381	24PTP_0104240122	24PTP_01PM04240123	MODULE, ECG/SPO2/NIBP	PHILIPS	M3001A	DE632F7989	I.C.U	PASS	MODULE OF ID Code :PTP00307
198	PTP00384	24PTP_0104240141	24PTP_01PM04240142	MONITORS, PATIENT TRANSPORT	PHILIPS	INTELLIVUE X2(M3002A)	DE575M1674	I.C.U	PASS	จอภาพมีลายเส้นสีดำ
199	PTP00385	24PTP_0104240138	24PTP_01PM04240139	MONITORS, PATIENT TRANSPORT	PHILIPS	INTELLIVUE X2(M3002A)	DE315C9782	I.C.U	PASS	
200	PTP00388	24PTP_0104240049	24PTP_01PM04240048	INFUSION PUMPS	TOP	TOP-2200	HL63570	I.C.U	PASS	
201	PTP00392	24PTP_0104240117	24PTP_01PM04240117	INFUSION PUMPS, SYRINGE	B BRAUN	PERFUSOR SPACE	311472	I.C.U	PASS	
202	PTP00393	24PTP_0105240002	24PTP_01PM05240002	VENTILATORS, INTENSIVE CARE	CAREFUSION	VELA	BDT03317	I.C.U	PASS	O2 Sensor failed

No.	ID CODE	Cer.No	PM.No	MEDICAL EQUIPMENT	BRAND	MODEL	S/N	DEPARTMENT	STATUS	REMARK
203	PTP00395	24PTP_0104240144	24PTP_01PM04240145	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	INTELLIVUE MP20(M8001A)	DE72876247	I.C.U	PASS	
204	PTP00396	24PTP_0104240146	24PTP_01PM04240146	MODULE, ECG/SPO2/NIBP	PHILIPS	M3001A	DE9070C8LL	I.C.U	PASS	MODULE OF ID Code :PTP00395
205	PTP00403	24PTP_0104240126	24PTP_01PM04240127	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	INTELLIVUE MP20(M8001A)	35108	I.C.U	PASS	
206	PTP00404	24PTP_0104240191	24PTP_01PM04240191	MODULE, ECG/SPO2/NIBP	PHILIPS	M3001A	DE9070C8GG	I.C.U	PASS	MODULE OF ID Code :PTP02510
207	PTP00454	24PTP_0104240124	24PTP_01PM04240124	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	INTELLIVUE MP20(M8001A)	DE50406333	I.C.U	PASS	ปุ่ม Silence ขำรุุด และตัวถือค module ขำรุุด
208	PTP00455	-	-	MODULE, ECG/SPO2/NIBP	PHILIPS	M3001A	DE632F8005	I.C.U	DEFECTIVE	ค่า IBP ไม่ผ่าน
209	PTP00457	-	-	INFUSION PUMPS, SYRINGE	TERUMO	TE-331	1004000133	I.C.U	DEFECTIVE	เครื่องไม่มีอะไหล่ทดแทน รอส่งคืนทรัพย์สิน
210	PTP00471	24PTP_0104240200	24PTP_01PM04240200	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	INTELLIVUE MX450	DE35148456	I.C.U	PASS	
211	PTP00472	24PTP_0104240157	24PTP_01PM04240158	MODULE, ECG/SPO2/NIBP	PHILIPS	M3001A	DE5630FGR8	I.C.U	PASS	MODULE OF ID Code : PTP00380
212	PTP00473	24PTP_0104240178	24PTP_01PM04240179	MODULE, ECG/SPO2/NIBP/IBP/TEMP	PHILIPS	M3012A	DE83748187	I.C.U	PASS	MODULE OF ID Code : PTP03684
213	PTP00755	24PTP_0104240055	24PTP_01PM04240054	INFUSION PUMPS, SYRINGE	TERUMO	TE-331	1208000519	I.C.U	PASS	
214	PTP01785	-	-	VENTILATORS, INTENSIVE CARE	CAREFUSION	VELA	BDT03256	I.C.U	DEFECTIVE	ส่งซ่อม
215	PTP02475	24PTP_0104240176	24PTP_01PM04240176	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	INTELLIVUE MX450	DE35114679	I.C.U	PASS	
216	PTP02476	-	-	MODULE, ECG/SPO2/NIBP/IBP/TEMP	PHILIPS	M3001A	DE9070C8KF	I.C.U	DEFECTIVE	ค่า IBP ไม่ผ่าน
217	PTP02485	24PTP_0104240115	24PTP_01PM04240115	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	INTELLIVUE MP20(M8001A)	DE72876228	I.C.U	PASS	ปุ่ม Silence ขำรุุด
218	PTP02486	24PTP_0104240181	24PTP_01PM04240181	MODULE, ECG/SPO2/NIBP/IBP/TEMP	PHILIPS	M3001A	DE9070C8LT	I.C.U	PASS	MODULE OF ID Code : PTP00311
219	PTP02488	24PTP_0104240052	24PTP_01PM04240051	INFUSION PUMPS	TOP	TOP-2300	15A0045	I.C.U	PASS	
220	PTP02497	24PTP_0104240155	24PTP_01PM04240155	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	INTELLIVUE MP20(M8001A)	DE72876204	I.C.U	PASS	
221	PTP02498	24PTP_0104240150	24PTP_01PM04240150	MODULE, ECG/SPO2/NIBP/IBP/TEMP	PHILIPS	M3001A	DE632F7324	I.C.U	PASS	MODULE OF ID Code : PTP00323
222	PTP02504	24PTP_0104240351	24PTP_01PM04240355	INFUSION PUMPS	TOP	TOP-2200	HL63575	I.C.U	PASS	
223	PTP02508	24PTP_0104240120	24PTP_01PM04240118	VENTILATORS, INTENSIVE CARE	CAREFUSION	VELA	BFT01839	I.C.U	PASS	O2 sensor failed
224	PTP02510	24PTP_0104240190	24PTP_01PM04240190	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	INTELLIVUE MX450	DE35148457	I.C.U	PASS	
225	PTP02511	24PTP_0104240179	24PTP_01PM04240178	MODULE, ECG/SPO2/NIBP	PHILIPS	M3001A	DE632F7991	I.C.U	PASS	MODULE OF ID Code : PTP3684
226	PTP02521	-	-	VENTILATORS, INTENSIVE CARE	PURITAN BENNETT	840	3512123686	I.C.U	DEFECTIVE	

No.	ID CODE	Cer.No	PM.No	MEDICAL EQUIPMENT	BRAND	MODEL	S/N	DEPARTMENT	STATUS	REMARK
227	PTP02529	24PTP_0104240340	24PTP_01PM04240343	VENTILATORS, INTENSIVE CARE	PURITAN BENNETT	840	3512110639	I.C.U	PASS	O2 Sensor failed
228	PTP02531	24PTP_0104240314	24PTP_01PM04240317	WARMING/COOLING UNITS, PATIENT, CIRCULATING-LIQUID	GAYMAR	MEDI -THERM III (MTA7912)	G21004	I.C.U	PASS	
229	PTP02532	24PTP_0104240364	24PTP_01PM04240367	WARMING/COOLING UNITS, PATIENT, CIRCULATING-LIQUID	CSZ	BLANKETROL III	083-19368	I.C.U	PASS	
230	PTP02534	24PTP_0104240044	24PTP_01PM04240043	INFUSION PUMPS	TOP	TOP-2200	HL63567S	I.C.U	PASS	
231	PTP02535	24PTP_0104240132	24PTP_01PM04240132	INFUSION PUMPS	TOP	TOP-2300	15A0036	I.C.U	PASS	
232	PTP02536	24PTP_0104240051	24PTP_01PM04240050	INFUSION PUMPS	TOP	TOP-2300	15A0164	I.C.U	PASS	
233	PTP02538	24PTP_0104240353	24PTP_01PM04240357	PACEMAKERS, CARDIAC, EXTERNAL	ST. JUDE MEDICAL	3077	1322206	I.C.U	PASS	
234	PTP02557	24PTP_0104240163	24PTP_01PM04240165	RESPIROMETER	FERRARIS	HALOSCALE	HS29303	I.C.U	PASS	
235	PTP02558	24PTP_0104240318	24PTP_01PM04240323	VENTILATORS, INTENSIVE CARE	PURITAN BENNETT	840	BDU 3510070818	I.C.U	PASS	
236	PTP02717	24PTP_0104240186	24PTP_01PM04240186	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	INTELLIVUE MX450	DE35148459	I.C.U	PASS	
237	PTP02718	24PTP_0104240195	24PTP_01PM04240197	MODULE, ECG/SPO2/NIBP	PHILIPS	M3001A	DE9070C8LW	I.C.U	PASS	MODULE OF ID Code :PTP00368
238	PTP02719	24PTP_0104240130	24PTP_01PM04240130	MODULE, ECG/SPO2/NIBP/IBP/TEMP	PHILIPS	M3012A	DE83753516	I.C.U	PASS	MODULE OF ID Code :PTP00403
239	PTP02721	24PTP_0104240168	24PTP_01PM04240170	INFUSION PUMPS	TOP	TOP-2200	GLY2352S	I.C.U	PASS	battery เสื่อม
240	PTP02728	24PTP_0104240329	24PTP_01PM04240331	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	INTELLIVUE MP20(M8001A)	DE72876200	I.C.U	PASS	
241	PTP02729	24PTP_0104240154	24PTP_01PM04240154	MODULE, ECG/SPO2/NIBP	PHILIPS	M3001A	DE717M0553	I.C.U	PASS	MODULE OF ID Code : PTP00370
242	PTP02737	24PTP_0104240123	24PTP_01PM04240122	INFUSION PUMPS	B BRAUN	INFUSOMAT SPACE P	370066	I.C.U	PASS	
243	PTP03289	24PTP_0104240205	24PTP_01PM04240205	DETECTORS, FETAL HEART, ULTRASONIC	NATUS	ELITE 200R	ECO1519	I.C.U	PASS	
244	PTP03371	24PTP_0104240175	24PTP_01PM04240175	MODULE, ECG/SPO2/NIBP/IBP/TEMP	PHILIPS	M3001A	DE9070C8KD	I.C.U	PASS	MODULE OF ID Code : PTP02475
245	PTP03465	24PTP_0104240308	24PTP_01PM04240309	VENTILATORS, INTENSIVE CARE	PURITAN BENNETT	840	3121125670	I.C.U	PASS	
246	PTP03684	24PTP_0104240177	24PTP_01PM04240177	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	INTELLIVUE MP20(M8001A)	DE62221469	I.C.U	PASS	
247	PTP03690	24PTP_0104240202	24PTP_01PM04240202	MODULE, ECG/SPO2/NIBP/IBP/TEMP	PHILIPS	M3012A	DE34712035	I.C.U	PASS	MODULE OF ID Code :PTP00471
248	PTP03798	24PTP_0104240145	24PTP_01PM04240144	OXYGEN HIGH FLOW	FISHER & PAYKEL HEALTHCARE 	AIRVO 2	210417257845	I.C.U	PASS	




No.	ID CODE	Cer.No	PM.No	MEDICAL EQUIPMENT	BRAND	MODEL	S/N	DEPARTMENT	STATUS	REMARK
249	PTP03799	24PTP_0104240143	24PTP_01PM04240143	OXYGEN HIGH FLOW	FISHER & PAYKEL HEALTHCARE 	AIRVO 2	210417257936	I.C.U	PASS	
250	PTP03869	24PTP_0104240106	24PTP_01PM04240106	OXYGEN HIGH FLOW	COMEN	NF5	F5210607105C	I.C.U	PASS	
251	PTP03870	24PTP_0104240324	24PTP_01PM04240328	OXYGEN HIGH FLOW	COMEN	NF5	F5210615003C	I.C.U	PASS	
252	PTP03871	24PTP_0104240206	24PTP_01PM04240206	OXYGEN HIGH FLOW	COMEN	NF5	F5210615071C	I.C.U	PASS	
253	PTP03872	24PTP_0104240315	24PTP_01PM04240318	OXYGEN HIGH FLOW	COMEN	NF5	F5210609110C	I.C.U	PASS	
254	PTP03873	24PTP_0104240107	24PTP_01PM04240107	OXYGEN HIGH FLOW	COMEN	NF5	F5210615001C	I.C.U	PASS	
255	PTP03874	24PTP_0104240108	24PTP_01PM04240108	OXYGEN HIGH FLOW	COMEN	NF5	F5210609092C	I.C.U	PASS	
256	PTP03875	-	-	OXYGEN HIGH FLOW	COMEN	NF5	F5210607048C	I.C.U	หาเครื่องไม่พบ	
257	PTP03876	24PTP_0104240109	24PTP_01PM04240109	OXYGEN HIGH FLOW	COMEN	NF5	F5210615065C	I.C.U	PASS	
258	PTP03921	24PTP_0104240164	24PTP_01PM04240166	RESPIROMETER	FERRARIS	HALOSCALE	HS29329	I.C.U	PASS	
259	PTP04529	24PTP_0104240137	24PTP_01PM04240137	INFUSION PUMPS, ENTERAL FEEDING	HAWKMED	HK-300	01163068	I.C.U	PASS	
260	PTP04530	24PTP_0104240136	24PTP_01PM04240136	INFUSION PUMPS, ENTERAL FEEDING	HAWKMED	HK-300	01163095	I.C.U	PASS	
261	PTP04539	24PTP_0104240204	24PTP_01PM04240204	PACEMAKERS, CARDIAC, EXTERNAL	MEDTRONIC	5392	DJH047741P	I.C.U	PASS	
262	PTP04575	24PTP_0104240189	24PTP_01PM04240189	MODULE, CO2	PHILIPS	M3014A	-	I.C.U	PASS	Carbon Dioxide Concentration 5% (36.8 mmHg) ±2.6 mmHg Carbon Dioxide Concentration 10% (73.6 mmHg) ±5.2 mmHg, MODULE OF ID Code :PTP02717
263	PTP04598	24PTP_0104240140	24PTP_01PM04240140	INFUSION PUMPS, ENTERAL FEEDING	HAWKMED	HK-300	01163197	I.C.U	PASS	
264	PTP04599	-	-	INFUSION PUMPS, ENTERAL FEEDING	HAWKMED	HK-300	01163184	I.C.U	หาเครื่องไม่พบ	
265	PTP04600	24PTP_0104240270	24PTP_01PM04240270	INFUSION PUMPS, ENTERAL FEEDING	HAWKMED	HK-300	01163180	I.C.U	PASS	
266	PTP04601	24PTP_0104240169	24PTP_01PM04240171	INFUSION PUMPS, ENTERAL FEEDING	HAWKMED	HK-300	01163176	I.C.U	PASS	
267	PTP04602	24PTP_0104240400	24PTP_01PM04240403	INFUSION PUMPS, ENTERAL FEEDING	HAWKMED	HK-300	01163190	I.C.U	PASS	
268	PTP04603	-	-	INFUSION PUMPS, ENTERAL FEEDING	HAWKMED	HK-300	01163231	I.C.U	หาเครื่องไม่พบ	
269	PTP04604	24PTP_0104240172	24PTP_01PM04240174	INFUSION PUMPS, ENTERAL FEEDING	HAWKMED	HK-300	01163233	I.C.U	PASS	

No.	ID CODE	Cer.No	PM.No	MEDICAL EQUIPMENT	BRAND	MODEL	S/N	DEPARTMENT	STATUS	REMARK
270	PTP04605	24PTP_0104240139	24PTP_01PM04240138	INFUSION PUMPS, ENTERAL FEEDING	HAWKMED	HK-300	01163226	I.C.U	PASS	
271	PTP04606	24PTP_0104240388	24PTP_01PM04240391	INFUSION PUMPS, ENTERAL FEEDING	HAWKMED	HK-300	01163252	I.C.U	PASS	
272	PTP04643	24PTP_0104240135	24PTP_01PM04240135	WARMING UNITS, PATIENT, FORCED-AIR	BAIR HUGGER	775	208845	I.C.U	PASS	
273	PTP04688	-	-	MODULE, CO2	PHILIPS	M3015A	DE43518151	I.C.U	DEFECTIVE	เสียแล้วไม่ขึ้นจอ
274	PTP00944	24PTP_0104240083	24PTP_01PM04240083	WARMING UNITS, PATIENT, RADIANT, INFANT	FISHER & PAYKEL HEALTHCARE	COSYCOT	141106001001	Labour Room	PASS	
275	PTP00950	24PTP_0104240103	24PTP_01PM04240103	VACUUM EXTRACTOR, OBSTETRIC	ATMOS	S 351 NATAL	200014010-124628-2014-11	Labour Room	PASS	
276	PTP00951	24PTP_0104240077	24PTP_01PM04240078	DETECTORS, FETAL HEART, ULTRASONIC	EDAN	F9	560154-M15202290001	Labour Room	PASS	
277	PTP00952	24PTP_0104240045	24PTP_01PM04240044	INFUSION PUMPS	TOP	TOP-2200	ELZ8606S	Labour Room	PASS	
278	PTP00954	24PTP_0104240102	24PTP_01PM04240102	MONITORS, PHYSIOLOGIC, VITAL SIGNS	COLIN	DUXEO BX-10	511224	Labour Room	PASS	
279	PTP00965	24PTP_0104240082	24PTP_01PM04240082	DETECTORS, FETAL HEART, ULTRASONIC	EDAN	F9	460475-M16B0256007	Labour Room	PASS	
280	PTP00966	-	-	DETECTORS, FETAL HEART, ULTRASONIC	NATUS	ELITE 200R	ECF0379	Labour Room	ยกเลิกการใช้งาน	
281	PTP03792	24PTP_0104240337	24PTP_01PM04240340	MONITORS, PHYSIOLOGIC, VITAL SIGNS	WELCH ALLYN	CONNEX SPOT MONITOR	100073792020	Let's Talk	PASS	
282	PTP03793	24PTP_0104240344	24PTP_01PM04240347	MONITORS, PHYSIOLOGIC, VITAL SIGNS	WELCH ALLYN	CONNEX SPOT MONITOR	100073782020	Let's Talk	PASS	
283	PTP01186	24PTP_0104240346	24PTP_01PM04240348	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	INTELLIVUE MP20(M8001A)	DE72832649	Neurology	PASS	ไม่มีสาย EKG
284	PTP01187	24PTP_0104240347	24PTP_01PM04240349	MODULE, ECG/SPO2/NIBP	PHILIPS	M3001A	DE632F7981	Neurology	PASS	MODULE OF ID Code :PTP01186
285	PTP01188	24PTP_0104240229	24PTP_01PM04240230	MONITORS, PHYSIOLOGIC, VITAL SIGNS	CASMED	740 SELECT	1526311	Neurology	PASS	
286	PTP01345	24PTP_0104240338	24PTP_01PM04240341	POSITIVE AIRWAY PRESSURE UNITS, CONTINUOUS	PHILIPS	OMNILAB ADVANCED+	L20642396994B	Neurology	PASS	
287	PTP01346	24PTP_0104240391	24PTP_01PM04240394	MONITORS, PHYSIOLOGIC, RESPIRATON/EXHALED CARBON DIOXIDE/PULSE OXIMETRY	NONIN MEDICAL	RESPSENSE	501667944	Neurology	PASS	Carbon Dioxide Concentration 5% (36.8 mmHg) ±2.6 mmHg Carbon Dioxide Concentration 10% (73.6 mmHg) ±5.2 mmHg
288	PTP00482	24PTP_0104240147	24PTP_01PM04240147	INCUBATORS, INFANT	ATOM	RABEE INCU I	2521052	Nursery	PASS	Replace Filter
289	PTP00483	24PTP_0105240001	24PTP_01PM05240001	INCUBATORS, INFANT	ATOM	RABEE INCU I	2520527	Nursery	PASS	

No.	ID CODE	Cer.No	PM.No	MEDICAL EQUIPMENT	BRAND	MODEL	S/N	DEPARTMENT	STATUS	REMARK
290	PTP00484	24PTP_0104240161	24PTP_01PM04240163	VENTILATORS, HIGH FREQUENCY OSCILLATORY INFANT	SLE	SLE5000	52363(2008)	Nursery	PASS	
291	PTP00486	24PTP_0104240093	24PTP_01PM04240093	INFUSION PUMPS, SYRINGE	B BRAUN	PERFUSOR SPACE	305937	Nursery	PASS	
292	PTP00487	24PTP_0104240074	24PTP_01PM04240075	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	INTELLIVUE MP5(M8105A)	DE57198579	Nursery	PASS	
293	PTP00488	24PTP_0104240099	24PTP_01PM04240099	OXIMETERS, PULSE	MASIMO	RADICAL-7	228092	Nursery	PASS	
294	PTP00489	24PTP_0104240080	24PTP_01PM04240077	INCUBATORS, INFANT	ATOM	RABEE INCU I	2521051	Nursery	PASS	Replace Filter
295	PTP00490	24PTP_0104240094	24PTP_01PM04240094	INFUSION PUMPS, SYRINGE	JYM	JZB-1800	11017232	Nursery	PASS	
296	PTP00491	24PTP_0104240076	24PTP_01PM04240076	OXIMETERS, PULSE	MASIMO	RADICAL-7	186598	Nursery	PASS	
297	PTP00492	24PTP_0104240100	24PTP_01PM04240100	OXIMETERS, PULSE	MASIMO	RADICAL-7	241129	Nursery	PASS	
298	PTP01050	24PTP_0104240087	24PTP_01PM04240087	INCUBATORS, INFANT, TRANSPORT	ATOM	V-707	25Y0690	Nursery	PASS	Replace Filter
299	PTP01051	24PTP_0104240075	24PTP_01PM04240074	RESUSCITATORS, PULMONARY	ATOM	RESUSCI FLOW	2560309	Nursery	PASS	
300	PTP01066	24PTP_0104240086	24PTP_01PM04240086	INCUBATORS, INFANT, TRANSPORT	ATOM	V-707	24Y0066	Nursery	PASS	Replace Filter
301	PTP01067	24PTP_0104240078	24PTP_01PM04240079	RESUSCITATORS, PULMONARY	FISHER & PAYKEL HEALTHCARE	NEOPUFF	120730003878	Nursery	PASS	
302	PTP01071	24PTP_0104240101	24PTP_01PM04240101	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	INTELLIVUE MP5(M8105A)	DE580A0596	Nursery	PASS	
303	PTP01072	24PTP_0104240079	24PTP_01PM04240081	WARMING UNITS, PATIENT, RADIANT, INFANT	SUTINDA	-	-	Nursery	PASS	
304	PTP01074	24PTP_0104240081	24PTP_01PM04240080	WARMING UNITS, PATIENT, RADIANT, INFANT	FISHER & PAYKEL HEALTHCARE	COSYCOT	151208000753	Nursery	PASS	
305	PTP01085	24PTP_0104240088	24PTP_01PM04240088	INCUBATORS, INFANT	ATOM	RABEE INCU I	2520528	Nursery	PASS	Replace Filter
306	PTP03588	24PTP_0103240001	24PTP_01PM03240001	VENTILATORS, HIGH FREQUENCY OSCILLATORY INFANT	ACUTRONIC	FABIAN HFO	AH18BD-01043	Nursery	PASS	
307	PTP00004	24PTP_0104240069	24PTP_01PM04240069	DETECTORS, FETAL HEART, ULTRASONIC	EDAN	F9	560154-M15902850001	Obstetric & Gynecology Center	PASS	
308	PTP00019	24PTP_0104240070	24PTP_01PM04240070	DETECTORS, FETAL HEART, ULTRASONIC	TOITU	FD-380	9821R41	Obstetric & Gynecology Center	PASS	
309	PTP00020	24PTP_0104240073	24PTP_01PM04240073	DETECTORS, FETAL HEART, ULTRASONIC	TOITU	FD-380	9520B64	Obstetric & Gynecology Center	PASS	
310	PTP00021	24PTP_0104240097	24PTP_01PM04240097	DETECTORS, FETAL HEART, ULTRASONIC	TOITU	FD-380	9520B62	Obstetric & Gynecology Center	PASS	

No.	ID CODE	Cer.No	PM.No	MEDICAL EQUIPMENT	BRAND	MODEL	S/N	DEPARTMENT	STATUS	REMARK
311	PTP00022	24PTP_0104240071	24PTP_01PM04240071	DETECTORS, FETAL HEART, ULTRASONIC	TOITU	FD-380	G010274	Obstetric & Gynecology Center	PASS	
312	PTP01740	-	24PTP_01PM04240312	SCANNING SYSTEMS, ULTRASONIC, GENERAL-PURPOSE	GE HEALTHCARE	LOGIQ C5 PREMIUM	290139WX5	Obstetric & Gynecology Center	PASS	
313	PTP03568	24PTP_0104240098	24PTP_01PM04240098	DETECTORS, FETAL HEART, ULTRASONIC	NICOLET	200R	ECH0988	Obstetric & Gynecology Center	PASS	
314	PTP00534	-	-	ASPIRATORS, EMERGENCY	Cheiron	VICTORIA	5071103	Operating Room	DEFECTIVE	ค่าสูงกว่าเกณฑ์
315	PTP00535	24PTP_0104240277	24PTP_01PM04240277	ELECTROSURGICAL UNITS	RICHARD WOLF	ELLMAN SURGITRON	1080652006	Operating Room	PASS	
316	PTP00548	24PTP_0104240259	24PTP_01PM04240259	ELECTROSURGICAL UNITS	ERBE	ICC 200	D-2235	Operating Room	PASS	
317	PTP00549	24PTP_0104240276	24PTP_01PM04240276	ASPIRATORS, SURGICAL	FOLEE	H001	-	Operating Room	PASS	
318	PTP00551	24PTP_0104240282	24PTP_01PM04240282	ELECTROSURGICAL UNITS	COVIDIEN	FORCE TRIAD	T5B44980EX	Operating Room	PASS	
319	PTP00571	24PTP_0104240379	24PTP_01PM04240382	ELECTROSURGICAL UNITS	VALLEYLAB	FORCE 2	1080147002	Operating Room	PASS	
320	PTP00585	24PTP_0104240294	24PTP_01PM04240293	MONITORS, BEDSIDE, PHYSIOLOGIC	NIHON KOHDEN	BSM-2303K	1366	Operating Room	PASS	
321	PTP00598	24PTP_0104240267	24PTP_01PM04240268	ANESTHESIA UNITS	DATEX-OHMEDA	AESPIRE VIEW	APHU01011	Operating Room	PASS	
322	PTP00598(VEN)	24PTP_0104240268	24PTP_01PM04240267	VENTILATORS, ANESTHESIA	DATEX-OHMEDA	AESPIRE VIEW	APHU01011	Operating Room	PASS	
323	PTP00599	24PTP_0104240295	24PTP_01PM04240295	MONITORS, BEDSIDE, PHYSIOLOGIC	NIHON KOHDEN	BSM-6301K	3172	Operating Room	PASS	
324	PTP00600	24PTP_0104240281	24PTP_01PM04240281	ELECTROSURGICAL UNITS	COVIDIEN	FORCE FX-8CS	S4L16224AX	Operating Room	PASS	
325	PTP00616	24PTP_0104240292	24PTP_01PM04240291	MODULE, ECG/SPO2/NIBP/IBP/TEMP	NIHON KOHDEN	AY-663P	6326	Operating Room	PASS	MODULE OF ID Code :PTP00664
326	PTP00618	24PTP_0104240278	24PTP_01PM04240279	DEFIBRILLATORS, EXTERNAL, MANUAL	PHILIPS	HeartStart XL (M4735A)	US00584077	Operating Room	PASS	
327	PTP00625	24PTP_0104240286	24PTP_01PM04240286	MONITORS, BEDSIDE, PHYSIOLOGIC	NIHON KOHDEN	BSM-6301K	3217	Operating Room	PASS	
328	PTP00626	24PTP_0104240288	24PTP_01PM04240288	MODULE, ECG/SPO2/NIBP/IBP/TEMP	NIHON KOHDEN	AY-663P	6390	Operating Room	PASS	MODULE OF ID Code :PTP00625
329	PTP00627	24PTP_0104240390	24PTP_01PM04240392	ANESTHESIA UNITS	DATEX-OHMEDA	S/5 Aespire	AMXJ01257 (VEN:144A0R3)	Operating Room	PASS	
330	PTP00627(VEN)	24PTP_0104240389	24PTP_01PM04240393	VENTILATORS, ANESTHESIA	DATEX-OHMEDA	S/5 Aespire	AMXJ01257 (VEN:144A0R3)	Operating Room	PASS	
331	PTP00644	24PTP_0104240302	24PTP_01PM04240302	MONITORS, BEDSIDE, PHYSIOLOGIC	NIHON KOHDEN	LIFE SCOPE TR(MU- 631RK)	3121	Operating Room	PASS	
332	PTP00645	24PTP_0104240303	24PTP_01PM04240303	MODULE, ECG/SPO2/NIBP/IBP/TEMP	NIHON KOHDEN	AY-663P	6384	Operating Room	PASS	MODULE OF ID Code :PTP00644

No.	ID CODE	Cer.No	PM.No	MEDICAL EQUIPMENT	BRAND	MODEL	S/N	DEPARTMENT	STATUS	REMARK
333	PTP00646	24PTP_0104240262	24PTP_01PM04240263	ANESTHESIA UNITS	DATEX-OHMEDA	AESPIRE VIEW	APHU01010 (VEN: AQBUBEI00109)	Operating Room	PASS	
334	PTP00646(VEN)	24PTP_0104240263	24PTP_01PM04240262	VENTILATORS, ANESTHESIA	DATEX-OHMEDA	AESPIRE VIEW	APHU01010 (VEN: AQBUBEI00109)	Operating Room	PASS	
335	PTP00647	24PTP_0104240279	24PTP_01PM04240278	ELECTROSURGICAL UNITS	COVIDIEN	FORCE FX	S4L16218AX	Operating Room	PASS	
336	PTP00663	24PTP_0104240260	24PTP_01PM04240260	ANESTHESIA UNITS	DATEX-OHMEDA	AESPIRE 7100	AMXQ00285	Operating Room	PASS	
337	PTP00663(VEN)	24PTP_0104240261	24PTP_01PM04240261	VENTILATORS, ANESTHESIA	DATEX-OHMEDA	AESPIRE 7100	AMXQ00285	Operating Room	PASS	
338	PTP00664	24PTP_0104240290	24PTP_01PM04240290	MONITORS, BEDSIDE, PHYSIOLOGIC	NIHON KOHDEN	BSM-6301K	3152	Operating Room	PASS	
339	PTP00665	24PTP_0104240296	24PTP_01PM04240296	MODULE, ECG/SPO2/NIBP/IBP/TEMP	NIHON KOHDEN	AY-663P	6388	Operating Room	PASS	MODULE OF ID Code :PTP00599
340	PTP00668	24PTP_0104240285	24PTP_01PM04240285	ELECTROSURGICAL UNITS	COVIDIEN	FORCE FX	S4L16231AX	Operating Room	PASS	
341	PTP00712	24PTP_0104240298	24PTP_01PM04240298	TOURNIQUETS, PNEUMATIC	ZIMMER	A.T.S. 1200	1211AAAB	Operating Room	PASS	
342	PTP00728	24PTP_0104240350	24PTP_01PM04240353	MONITORS, BEDSIDE, PHYSIOLOGIC	NIHON KOHDEN	PVM-2701	6897	Operating Room	PASS	cuff เสื่อมสภาพ, ไม่มีสาย SpO2 กับ EKG ซิม เครื่องอื่นสอบเทียบ
343	PTP02950	24PTP_0104240376	24PTP_01PM04240379	DETECTORS, FETAL HEART, ULTRASONIC	NICOLET	200R	ECK1059	Operating Room	PASS	
344	PTP03318	24PTP_0104240297	24PTP_01PM04240297	ASPIRATORS, EMERGENCY	Cheiron	VICTORIA	D5071102	Operating Room	PASS	
345	PTP04805	24PTP_0104240398	24PTP_01PM04240401	MODULE, IBP	PHILIPS 	M1006B	3604G12985	Operating Room	PASS	MODULE OF ID Code :PTP00740
346	PTP01328	24PTP_0104240343	24PTP_01PM04240346	INFUSION PUMPS	TOP	TOP-2200	JL64618	Patient Wards 15	OUT OF RANGE	
347	PTP01350	24PTP_0104240272	24PTP_01PM04240272	MONITORS, PHYSIOLOGIC, VITAL SIGNS	CRITICARE	506DN	113054821	Patient Wards 15	PASS	
348	PTP01351	24PTP_0104240225	24PTP_01PM04240226	MONITORS, PHYSIOLOGIC, VITAL SIGNS	CRITICARE	506DN	113054811	Patient Wards 15	PASS	
349	PTP01469	24PTP_0104240091	24PTP_01PM04240091	INFUSION PUMPS	TOP	TOP-2200	ELZ8641S	Patient Wards 15	PASS	
350	PTP02164	24PTP_0104240035	24PTP_01PM04240034	INFUSION PUMPS	TOP	TOP-2200	ELZ8629S	Patient Wards 15	PASS	
351	PTP02939	24PTP_0104240032	24PTP_01PM04240031	INFUSION PUMPS	TOP	TOP-2200	ELZ8613S	Patient Wards 15	PASS	
352	PTP02943	24PTP_0104240047	24PTP_01PM04240046	INFUSION PUMPS	TOP	TOP-2200	ELZ8611S	Patient Wards 15	PASS	Battery เสื่อมสภาพ
353	PTP03790	24PTP_0104240226	24PTP_01PM04240227	MONITORS, PHYSIOLOGIC, VITAL SIGNS	WELCH ALLYN	CONNEX SPOT MONITOR	100073762020	Patient Wards 15	PASS	
354	PTP03794	24PTP_0104240348	24PTP_01PM04240351	MONITORS, PHYSIOLOGIC, VITAL SIGNS	WELCH ALLYN	CONNEX SPOT MONITOR	100073842020	Patient Wards 15	PASS	
355	PTP01276	24PTP_0104240227	24PTP_01PM04240228	INFUSION PUMPS	TOP	TOP-2200	EL27058S	Patient Wards 16	PASS	
356	PTP01304	24PTP_0104240254	24PTP_01PM04240254	MONITORS, PHYSIOLOGIC, VITAL SIGNS	KTMED	KTPM-1000	ZD1100130	Patient Wards 16	PASS	

No.	ID CODE	Cer.No	PM.No	MEDICAL EQUIPMENT	BRAND	MODEL	S/N	DEPARTMENT	STATUS	REMARK
357	PTP01305	24PTP_0104240275	24PTP_01PM04240274	MONITORS, PHYSIOLOGIC, VITAL SIGNS	KTMED	KTPM-1000	ZC1100113	Patient Wards 16	PASS	
358	PTP01445	24PTP_0104240048	24PTP_01PM04240047	INFUSION PUMPS	TOP	TOP-2200	ELZ8610S	Patient Wards 16	PASS	
359	PTP01449	24PTP_0104240387	24PTP_01PM04240390	INFUSION PUMPS	TOP	TOP-2200	HL63568S	Patient Wards 16	PASS	
360	PTP01453	24PTP_0104240212	24PTP_01PM04240212	INFUSION PUMPS	TOP	TOP-2200	ELY8526S	Patient Wards 16	PASS	
361	PTP01458	24PTP_0104240269	24PTP_01PM04240269	INFUSION PUMPS	TOP	TOP-2200	ELZ8620S	Patient Wards 16	PASS	
362	PTP02357	24PTP_0104240250	24PTP_01PM04240251	INFUSION PUMPS	TOP	TOP-2200	ELZ8643S	Patient Wards 16	PASS	
363	PTP02907	24PTP_0104240399	24PTP_01PM04240402	INFUSION PUMPS	TOP	TOP-2200	JL64607S	Patient Wards 16	PASS	
364	PTP03476	24PTP_0104240223	24PTP_01PM04240224	MONITORS, PHYSIOLOGIC, VITAL SIGNS	WELCH ALLYN	CONNEX SPOT MONITOR	10001962317	Patient Wards 16	PASS	
365	PTP00109	24PTP_0104240036	24PTP_01PM04240035	INFUSION PUMPS	TOP	TOP-2200	JL64621	Patient Wards 17	PASS	Battery เสื่อมสภาพ
366	PTP00112	24PTP_0104240131	24PTP_01PM04240131	INFUSION PUMPS	TOP	TOP-2200	ELZ8619S	Patient Wards 17	PASS	
367	PTP00120	24PTP_0104240024	24PTP_01PM04240024	INFUSION PUMPS	TOP	TOP-2200	ELZ8624S	Patient Wards 17	PASS	
368	PTP00140	24PTP_0104240040	24PTP_01PM04240039	INFUSION PUMPS	TOP	TOP-2200	ELY8539S	Patient Wards 17	PASS	
369	PTP00148	24PTP_0104240316	24PTP_01PM04240319	MONITORS, PHYSIOLOGIC, VITAL SIGNS	CASMED	740 SELECT	1526307	Patient Wards 17	PASS	
370	PTP00149	-	-	MONITORS, PHYSIOLOGIC, VITAL SIGNS	KTMED	KTPM-1000	ZB1200216	Patient Wards 17	หาเครื่องไม่พบ	
371	PTP00184	24PTP_0104240192	24PTP_01PM04240193	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	INTELLIVUE MP20(M8001A)	DE72876221	Patient Wards 17	PASS	
372	PTP00185	24PTP_0104240016	24PTP_01PM04240016	MODULE, ECG/SPO2/NIBP	PHILIPS	M3001A	DE632F7309	Patient Wards 17	PASS	MODULE OF ID Code :PTP02330
373	PTP01256	24PTP_0104240059	24PTP_01PM04240058	INFUSION PUMPS	TOP	TOP-2200	ELZ8646S	Patient Wards 17	PASS	
374	PTP01437	24PTP_0104240252	24PTP_01PM04240253	INFUSION PUMPS	TOP	TOP-2200	ELZ8601S	Patient Wards 17	PASS	
375	PTP00050	24PTP_0104240363	24PTP_01PM04240366	INFUSION PUMPS	TOP	TOP-2200	JL74777	Patient Wards 18	PASS	
376	PTP00078	24PTP_0104240156	24PTP_01PM04240156	MODULE, ECG/SPO2/NIBP	PHILIPS	M3001A	DE717L9004	Patient Wards 18	PASS	MODULE OF ID Code : PTP02497
377	PTP00079	24PTP_0104240142	24PTP_01PM04240141	OXYGEN HIGH FLOW	FISHER & PAYKEL HEALTHCARE	AIRVO 2	1150119010150	Patient Wards 18	PASS	
378	PTP00080	24PTP_0104240328	24PTP_01PM04240332	VENTILATORS, INTENSIVE CARE	MAQUET	SERVO 1	82025	Patient Wards 18	PASS	
379	PTP00091	24PTP_0104240037	24PTP_01PM04240036	INFUSION PUMPS	TOP	TOP-2200	JLX4929	Patient Wards 18	PASS	Battery เสื่อมสภาพ
380	PTP00094	24PTP_0104240053	24PTP_01PM04240052	INFUSION PUMPS	TOP	TOP-2300	15A0138	Patient Wards 18	PASS	
381	PTP00097	24PTP_0104240166	24PTP_01PM04240168	INFUSION PUMPS	TOP	TOP-2300	15A0025	Patient Wards 18	PASS	
382	PTP00100	-	-	INFUSION PUMPS	TOP	TOP-2200	JLY5061	Patient Wards 18	หาเครื่องไม่พบ	
383	PTP00103	24PTP_0104240220	24PTP_01PM04240221	MONITORS, PHYSIOLOGIC, VITAL SIGNS	COLIN	BX-10NE	11049	Patient Wards 18	PASS	knob ปิด Alarm กับ ปิด/เปิด NIBP ขำรุด
384	PTP00153	-	-	INFUSION PUMPS	TOP	TOP-2300	15A0153	Patient Wards 18	หาเครื่องไม่พบ	

No.	ID CODE	Cer.No	PM.No	MEDICAL EQUIPMENT	BRAND	MODEL	S/N	DEPARTMENT	STATUS	REMARK
385	PTP01415	24PTP_0104240133	24PTP_01PM04240133	INFUSION PUMPS	TOP	TOP-2300	15A0012	Patient Wards 18	PASS	
386	PTP01428	24PTP_0104240134	24PTP_01PM04240134	INFUSION PUMPS	TOP	TOP-2300	15A0165	Patient Wards 18	PASS	
387	PTP02878	-	-	INFUSION PUMPS	TOP	TOP-2300	15A0120	Patient Wards 18	DEFECTIVE	ค่า flow rate สูงกว่าเกณฑ์
388	PTP03475	24PTP_0104240392	24PTP_01PM04240395	MONITORS, PHYSIOLOGIC, VITAL SIGNS	WELCH ALLYN	CONNEX SPOT MONITOR	100019772317	Patient Wards 18	PASS	
389	PTP03787	24PTP_0104240224	24PTP_01PM04240225	MONITORS, PHYSIOLOGIC, VITAL SIGNS	WELCH ALLYN	CONNEX SPOT MONITOR	100073752020	Patient Wards 18	PASS	
390	PTP04494	24PTP_0104240396	24PTP_01PM04240399	MONITORS, PHYSIOLOGIC, VITAL SIGNS	WELCH ALLYN	CONNEX SPOT MONITOR	100073852020	Patient Wards 18	PASS	
391	PTP01522	24PTP_0104240326	24PTP_01PM04240329	MONITORS, PHYSIOLOGIC, VITAL SIGNS	CASMED	740 SELECT	1526309	Patient Wards 19	PASS	ไม่มีสาย SpO2
392	PTP03795	24PTP_0104240208	24PTP_01PM04240208	MONITORS, PHYSIOLOGIC, VITAL SIGNS	WELCH ALLYN	CONNEX SPOT MONITOR	100073802020	Patient Wards 19	PASS	
393	PTP01518	24PTP_0104240210	24PTP_01PM04240210	DEFIBRILLATORS, EXTERNAL, MANUAL	PHILIPS	HeartStart XL+ (861290)	USO1518016	Patient Wards 404	PASS	
394	PTP01644	24PTP_0104240042	24PTP_01PM04240041	INFUSION PUMPS	TOP	TOP-2200	ELZ8614S	Patient Wards 404	PASS	Battery เสื่อมสภาพ
395	PTP04585	24PTP_0104240273	24PTP_01PM04240273	MONITORS, PHYSIOLOGIC, VITAL SIGNS	WELCH ALLYN	CONNEX SPOT MONITOR	21100073942020	Patient Wards 404	PASS	
396	PTP01497	24PTP_0104240034	24PTP_01PM04240033	INFUSION PUMPS	TOP	TOP-2200	EL27065S	Patient Wards 406	PASS	
397	PTP01498	24PTP_0104240251	24PTP_01PM04240252	MONITORS, PHYSIOLOGIC, VITAL SIGNS	CASMED	740 SELECT	1547134	Patient Wards 406	PASS	
398	PTP02641	24PTP_0104240031	24PTP_01PM04240030	INFUSION PUMPS	TOP	TOP-2200	GLY2386S	Patient Wards 406	PASS	
399	PTP02649	24PTP_0104240043	24PTP_01PM04240042	INFUSION PUMPS	TOP	TOP-2200	EL27062S	Patient Wards 406	PASS	Battery เสื่อมสภาพ
400	PTP02653	24PTP_0104240021	24PTP_01PM04240021	INFUSION PUMPS	TOP	TOP-2200	ELZ8607S	Patient Wards 406	PASS	Battery เสื่อมสภาพ
401	PTP02673	24PTP_0104240050	24PTP_01PM04240049	INFUSION PUMPS	TOP	TOP-2200	GLY2382S	Patient Wards 406	PASS	
402	PTP02681	24PTP_0104240041	24PTP_01PM04240040	INFUSION PUMPS	TOP	TOP-2200	ELZ8650S	Patient Wards 406	PASS	
403	PTP02700	24PTP_0104240064	24PTP_01PM04240063	INFUSION PUMPS	TOP	TOP-2200	GLY2383S	Patient Wards 406	PASS	
404	PTP02704	24PTP_0104240089	24PTP_01PM04240089	INFUSION PUMPS	TOP	TOP-2200	ELZ8615S	Patient Wards 406	PASS	
405	PTP03621	24PTP_0104240244	24PTP_01PM04240244	MONITORS, PHYSIOLOGIC, ELECTROCARDIOGRAPHY, TELEMETRIC	PHILIPS	INTELLIVUE MX40	DE60300017	Patient Wards 406	PASS	
406	PTP03622	24PTP_0104240245	24PTP_01PM04240246	MONITORS, PHYSIOLOGIC, ELECTROCARDIOGRAPHY, TELEMETRIC	PHILIPS	INTELLIVUE MX40	DE60300019	Patient Wards 406	PASS	
407	PTP03800	24PTP_0104240380	24PTP_01PM04240383	OXIMETERS, PULSE	JUMPER	JPD-500E	8823500E408002	Patient Wards 406	PASS	
408	PTP03803	24PTP_0104240072	24PTP_01PM04240072	OXIMETERS, PULSE	JUMPER	JPD-500E	8823500E408006	Patient Wards 406	PASS	
409	PTP03805	-	-	OXIMETERS, PULSE	JUMPER	JPD-500E	8823500E408011	Patient Wards 406	หาตัวเครื่องไม่พบ	

No.	ID CODE	Cer.No	PM.No	MEDICAL EQUIPMENT	BRAND	MODEL	S/N	DEPARTMENT	STATUS	REMARK
410	PTP03809	24PTP_0104240001	24PTP_01PM04240001	OXIMETERS, PULSE	JUMPER	JPD-500E	8823500E408015	Patient Wards 406	PASS	
411	PTP03813	-	-	OXIMETERS, PULSE	JUMPER	JPD-500E	8823500E408021	Patient Wards 406	หาเครื่องมือพบ	
412	PTP04493	24PTP_0104240241	24PTP_01PM04240242	MONITORS, PHYSIOLOGIC, VITAL SIGNS	WELCH ALLYN	CONNEX SPOT MONITOR	100073862020	Patient Wards 406	PASS	
413	PTP04618	24PTP_0104240104	24PTP_01PM04240104	MONITORS, PHYSIOLOGIC, VITAL SIGNS	WELCH ALLYN	CONNEX SPOT MONITOR	100073952020	Patient Wards 406	PASS	
414	PTP01697	24PTP_0104240039	24PTP_01PM04240038	INFUSION PUMPS	TOP	TOP-2200	ELZ8617S	Patient Wards 407	PASS	
415	PTP02360	24PTP_0104240023	24PTP_01PM04240022	INFUSION PUMPS	TOP	TOP-2200	ELZ8639S	Patient Wards 408	PASS	
416	PTP02361	24PTP_0104240019	24PTP_01PM04240019	INFUSION PUMPS	TOP	TOP-2200	GLY2402S	Patient Wards 408	PASS	
417	PTP02377	24PTP_0104240237	24PTP_01PM04240238	MONITORS, PHYSIOLOGIC, VITAL SIGNS	CRITICARE	506DN	113054814	Patient Wards 408	PASS	ไม่มีสาย SpO2
418	PTP03789	24PTP_0104240236	24PTP_01PM04240237	MONITORS, PHYSIOLOGIC, VITAL SIGNS	WELCH ALLYN	CONNEX SPOT MONITOR	100073772020	Patient Wards 408	PASS	
419	PTP01971	24PTP_0104240148	24PTP_01PM04240148	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	INTELLIVUE MP20(M8001A)	DE62221511	Pediatrics Center	PASS	
420	PTP01972	24PTP_0104240174	24PTP_01PM04240161	MODULE, ECG/SPO2/NIBP	PHILIPS	M3001A	DE5630FGTO	Pediatrics Center	PASS	MODULE OF ID Code : PTP00321
421	PTP01974	24PTP_0104240215	24PTP_01PM04240215	MONITORS, PHYSIOLOGIC, VITAL SIGNS	KTMED	KTPM-1000	ZL1000101	Pediatrics Center	PASS	Battery เสื่อมสภาพ
422	PTP01993	24PTP_0104240228	24PTP_01PM04240229	MONITORS, PHYSIOLOGIC, VITAL SIGNS	ZOE MEDICAL	740 SELECT	CFD01593	Pediatrics Center	PASS	
423	PTP01994	24PTP_0104240213	24PTP_01PM04240213	OXIMETERS, PULSE	NONIN	2500	501117846	Pediatrics Center	PASS	
424	PTP01995	24PTP_0104240214	24PTP_01PM04240214	OXIMETERS, PULSE	Bitmos	SAT 801+	68151123	Pediatrics Center	PASS	
425	PTP03844	24PTP_0104240360	24PTP_01PM04240364	THERMOMETERS, ELECTRONIC, INFRARED, SKIN	ROSSMAX	-	2090520955	Pediatrics Center	PASS	
426	PLP00850	-	-	LASERS, PHYSICAL THERAPY	REIMERS&JANSSEN	PHYSIOLASER OLYMPIC	14172-102	Physiotherapy	DEFECTIVE	ค่าต่ำกว่าเกณฑ์
427	PLP00893	24PTP_0104240311	24PTP_01PM04240314	LASERS, PHYSICAL THERAPY	REIMERS&JANSSEN	PHYSIOLASER OLYMPIC	18172-60	Physiotherapy	PASS	ใช้หัวเลเซอร์ SN : 14511A-012 ในการทดสอบ
428	PLP03109	24PTP_0104240310	24PTP_01PM04240313	LASERS, PHYSICAL THERAPY	REIMERS&JANSSEN	PHYSIOLASER OLYMPIC	19172-07	Physiotherapy	PASS	ใช้หัวเลเซอร์ SN : 14511A-012 ในการทดสอบ
429	PLP03866	24PTP_0104240084	24PTP_01PM04240084	OXIMETERS, PULSE	STRONG	703F	703F-8007008	Physiotherapy	PASS	
430	PTP00847	-	-	BATHS, PARAFFIN, PHYSICAL THERAPY	CONSTANTEMP	112	22-72034	Physiotherapy	ยกเลิกออกจากแผนชั่วคราว	CAL/PM OCT
431	PTP00862	24PTP_0104240238	24PTP_01PM04240239	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	INTELLIVUE MP20(M8001A)	DE72876245	Physiotherapy	PASS	ไม่มีสาย EKG
432	PTP00863	24PTP_0104240239	24PTP_01PM04240240	MODULE, ECG/SPO2/NIBP	PHILIPS	M3001A	DE632F7987	Physiotherapy	PASS	MODULE OF ID Code :PTP00862
433	PTP00884	24PTP_0104240253	24PTP_01PM04240306	LASERS, PHYSICAL THERAPY	REIMERS&JANSSEN	PHYSIOLASER OLYMPIC	14172-23	Physiotherapy	PASS	ใช้หัวเลเซอร์ SN : 14511A-012 ในการทดสอบ
434	PTP00899	24PTP_0104240240	24PTP_01PM04240241	OXIMETERS, PULSE	STRONG	703F	703F-8006966	Physiotherapy	PASS	



No.	ID CODE	Cer.No	PM.No	MEDICAL EQUIPMENT	BRAND	MODEL	S/N	DEPARTMENT	STATUS	REMARK
435	PTP01934	24PTP_0104240356	24PTP_01PM04240359	MONITORS, PHYSIOLOGIC, VITAL SIGNS	PHILIPS	SURESIGNS VS3	US42754220	Physiotherapy	PASS	
436	PTP03867	24PTP_0104240257	24PTP_01PM04240257	OXIMETERS, PULSE	STRONG	703F	703F8GA00833	Physiotherapy	PASS	
437	PTP04500	24PTP_0104240247	24PTP_01PM04240248	OXIMETERS, PULSE	-	703F	703F8GA00738	Physiotherapy	PASS	
438	PTP04502	24PTP_0104240249	24PTP_01PM04240249	OXIMETERS, PULSE	-	703F	703F8GA00845	Physiotherapy	PASS	
439	PTP03474	24PTP_0104240207	24PTP_01PM04240207	MONITORS, PHYSIOLOGIC, VITAL SIGNS	WELCH ALLYN	CONNEX SPOT MONITOR	100019072317	Skin	PASS	
440	PTP01826	24PTP_0104240255	24PTP_01PM04240255	DEFIBRILLATORS, EXTERNAL, MANUAL	PHILIPS	HeartStart XL (M4735A)	US00577901	X-Ray	PASS	สาย EKG เสื่อมสภาพ
441	PTP01827	24PTP_0104240246	24PTP_01PM04240247	MONITORS, PHYSIOLOGIC, VITAL SIGNS	COLIN	DUXEO BX-10	511244	X-Ray	PASS	ปุ่มวัด NIBP และปุ่มปิด Alarm ข้างวัด
442	PTP01840	24PTP_0104240256	24PTP_01PM04240256	INJECTORS, CONTRAST MEDIA	MEDRAD	STELLANT	3014426 38017	X-Ray	PASS	Test : VOLUME 50 ml FLOW RAT 2.5 ml/sec Test : VOLUME 100 ml FLOW RAT 4 ml/sec Test : VOLUME 150 ml FLOW RAT 5 ml/sec
443	PTP01841	24PTP_0104240242	24PTP_01PM04240243	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	INTELLIVUE MP20(M8001A)	DE72847424	X-Ray	PASS	ไม่มีสาย EKG
444	PTP01842	24PTP_0104240243	24PTP_01PM04240245	MODULE, ECG/SPO2/NIBP	PHILIPS	M3001A	DE907T6796	X-Ray	PASS	MODULE OF ID Code :PTP01841
445	PTP01843	24PTP_0104240248	24PTP_01PM04240250	VENTILATORS, TRANSPORT	PNEUPAC	S	S2280	X-Ray	PASS	
446	PTP02891	-	-	INJECTORS, CONTRAST MEDIA	MEDRAD	SPECTRIS SOLARIS EP	3012014 44010	X-Ray	DEFECTIVE	Battery เสื่อมสภาพ รอซื้อเครื่องทดแทน



No.	ID CODE	Cer.No	PM.No	MEDICAL EQUIPMENT	BRAND	MODEL	S/N	DEPARTMENT	STATUS	REMARK
1	PTP01328	24PTP_0104240343	24PTP_01PM04240346	INFUSION PUMPS	TOP	TOP-2200	JL64618	Patient Wards 15	OUT OF RANGE	

No.	ID CODE	Cer.No	PM.No	MEDICAL EQUIPMENT	BRAND	MODEL	S/N	DEPARTMENT	STATUS	REMARK
1	PTP00748	-	-	MONITORS, PATIENT TRANSPORT	PHILIPS	INTELLIVUE X2(M3002A)	DE037A3403	Anesthesia	หาเครื่องไม่พบ	
2	PTP02945	-	-	INFUSION PUMPS, ANALGESIC, PATIENT-CONTROLLED	AITECS	SP-14S	7907	Anesthesia	ยกเลิกการใช้งาน	
3	PTP03459	-	-	MODULE, CO2/TEMP	PHILIPS	M3014A	DE61414205	Anesthesia	หาเครื่องไม่พบ	
4	PTP03563	-	-	MONITORS, PHYSIOLOGIC, VITAL SIGNS	CRITICARE	506DN	113054816	BME-PTP	หาเครื่องไม่พบ	
5	PTP04209	-	-	OXIMETERS, PULSE	-	-	-	BME-PTP	หาเครื่องไม่พบ	
6	PTP04211	-	-	OXIMETERS, PULSE	-	-	-	BME-PTP	หาเครื่องไม่พบ	
7	PTP04228	-	-	OXIMETERS, PULSE	-	-	-	BME-PTP	หาเครื่องไม่พบ	
8	PTP03868	-	-	OXIMETERS, PULSE	STRONG	703F	703F-8007008	Bone & Joint	หาเครื่องไม่พบ	
9	PTP01795	-	-	ANESTHESIA UNITS	DATEX-OHMEDA	AESPIRE	AMX10110153WA	Cardio-Neuro Vascular Intervention	DEFECTIVE	ค่า PEEP ที่ตั้งกับค่าที่เครื่องจ่ายต่างกันเกิน 10%
10	PTP01798	-	-	INJECTORS, CONTRAST MEDIA	LIEBEL-FLARSHEIM	LF	CI0111C011	Cardio-Neuro Vascular Intervention	ยกเลิกการใช้งาน	
11	PTP03490	-	-	MONITORS, PHYSIOLOGIC, VITAL SIGNS	KTMED	KTPM-1000	-	Check Up Center	หาเครื่องไม่พบ	
12	PTP03851	-	-	MONITORS, PHYSIOLOGIC, VITAL SIGNS	EDAN	M3A	360125-M21505660012	Check Up Center	หาเครื่องไม่พบ	
13	PTP02196	-	-	MONITORS, PHYSIOLOGIC, VITAL SIGNS	CRITICARE	506DN	113054331	Emergency & Ambulance	DEFECTIVE	ส่งซ่อม
14	PTP02323	-	-	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	INTELLIVUE MP20(M8001A)	DE62221474	Emergency & Ambulance	DEFECTIVE	ส่งซ่อมกับทางบริษัท
15	PTP01123	-	-	ELECTROSURGICAL UNITS	ERBE	ICC 200	D-2193	Gastrointestinal & Liver Center	DEFECTIVE	ค่า HF Leakage สูงกว่าเกณฑ์, Mode Bipolar ตั้งแต่ค่า 50 ลงมาต่ำกว่าเกณฑ์
16	PTP01163	-	-	MODULE, ECG/SPO2/NIBP	PHILIPS	M3001A	DE632F7960	Gastrointestinal & Liver Center	หาเครื่องไม่พบ	
17	PTP00305	-	-	DEFIBRILLATORS, EXTERNAL, MANUAL	PHILIPS	HeartStart XL+ (861290)	US71514172	I.C.U	DEFECTIVE	ส่งซ่อมกับทางบริษัท

No.	ID CODE	Cer.No	PM.No	MEDICAL EQUIPMENT	BRAND	MODEL	S/N	DEPARTMENT	STATUS	REMARK
18	PTP00455	-	-	MODULE, ECG/SPO2/NIBP	PHILIPS	M3001A	DE632F8005	I.C.U	DEFECTIVE	ค่า IBP ไม่ผ่าน
19	PTP00457	-	-	INFUSION PUMPS, SYRINGE	TERUMO	TE-331	1004000133	I.C.U	DEFECTIVE	เครื่องมือไม่มีอะไหล่ทดแทน รอส่งคืนทรัพย์สิน
20	PTP01785	-	-	VENTILATORS, INTENSIVE CARE	CAREFUSION	VELA	BDT03256	I.C.U	DEFECTIVE	ส่งซ่อม
21	PTP02476	-	-	MODULE, ECG/SPO2/NIBP/IBP/TEMP	PHILIPS	M3001A	DE9070C8KF	I.C.U	DEFECTIVE	ค่า IBP ไม่ผ่าน
22	PTP02521	-	-	VENTILATORS, INTENSIVE CARE	PURITAN BENNETT	840	3512123686	I.C.U	DEFECTIVE	
23	PTP03875	-	-	OXYGEN HIGH FLOW	COMEN	NF5	F5210607048C	I.C.U	หาเครื่องไม่พบ	
24	PTP04599	-	-	INFUSION PUMPS, ENTERAL FEEDING	HAWKMED	HK-300	01163184	I.C.U	หาเครื่องไม่พบ	
25	PTP04603	-	-	INFUSION PUMPS, ENTERAL FEEDING	HAWKMED	HK-300	01163231	I.C.U	หาเครื่องไม่พบ	
26	PTP04688	-	-	MODULE, CO2	PHILIPS	M3015A	DE43518151	I.C.U	DEFECTIVE	เสียบแล้วไม่ขึ้นจอ
27	PTP00966	-	-	DETECTORS, FETAL HEART, ULTRASONIC	NATUS	ELITE 200R	ECF0379	Labour Room	ยกเลิกการใช้งาน	
28	PTP00534	-	-	ASPIRATORS, EMERGENCY	Cheiron	VICTORIA	5071103	Operating Room	DEFECTIVE	ค่าสูงกว่าเกณฑ์
29	PTP00149	-	-	MONITORS, PHYSIOLOGIC, VITAL SIGNS	KTMED	KTPM-1000	ZB1200216	Patient Wards 17	หาเครื่องไม่พบ	
30	PTP00100	-	-	INFUSION PUMPS	TOP	TOP-2200	JLY5061	Patient Wards 18	หาเครื่องไม่พบ	
31	PTP00153	-	-	INFUSION PUMPS	TOP	TOP-2300	15A0153	Patient Wards 18	หาเครื่องไม่พบ	
32	PTP02878	-	-	INFUSION PUMPS	TOP	TOP-2300	15A0120	Patient Wards 18	DEFECTIVE	ค่า flow rate สูงกว่าเกณฑ์
33	PTP03805	-	-	OXIMETERS, PULSE	JUMPER	JPD-500E	8823500E408011	Patient Wards 406	หาเครื่องไม่พบ	
34	PTP03813	-	-	OXIMETERS, PULSE	JUMPER	JPD-500E	8823500E408021	Patient Wards 406	หาเครื่องไม่พบ	

No.	ID CODE	Cer.No	PM.No	MEDICAL EQUIPMENT	BRAND	MODEL	S/N	DEPARTMENT	STATUS	REMARK
35	PLP00850	-	-	LASERS, PHYSICAL THERAPY	REIMERS&JANSSEN	PHYSIOLASER OLYMPIC	14172-102	Physiotherapy	DEFECTIVE	ค่าต่ำกว่าเกณฑ์
36	PTP00847	-	-	BATHS, PARAFFIN, PHYSICAL THERAPY	CONSTANTEMP	112	22-72034	Physiotherapy	ขกเลิกออกจากแผนชั่วคราว	CAL/PM OCT
37	PTP02891	-	-	INJECTORS, CONTRAST MEDIA	MEDRAD	SPECTRIS SOLARIS EP	3012014 44010	X-Ray	DEFECTIVE	Battery เสื่อมสภาพ รอซื้อเครื่องทดแทน