

รายงานผลการดำเนินการ


บำรุงรักษาเชิงป้องกันและสอบเทียบเครื่องมือแพทย์

โรงพยาบาลเปาโลเกษตร

รอบเดือน มิถุนายน 2567


สรุปผลการดำเนินการ

ลำดับ	รายละเอียด	จำนวน (เครื่อง)	หมายเหตุ
1	จำนวนเครื่องมือทั้งหมด	384	ตามเอกสารแนบ 1
2	ผลการสอบเทียบ		
	PASS	332	ตามเอกสารแนบ 1
	OUT OF RANGE	10	ตามเอกสารแนบ 2
3	ไม่สามารถดำเนินการ		ตามเอกสารแนบ 3
	DEFECTIVE	18	
	BME	1	
	บริษัทภายนอกดำเนินการ	2	
	ยกเลิกการใช้งาน	15	
	หาเครื่องไม่พบ	4	
	ยกเลิกออกจากแผนชั่วคราว	2	
ดำเนินการแล้วทั้งหมด		384	

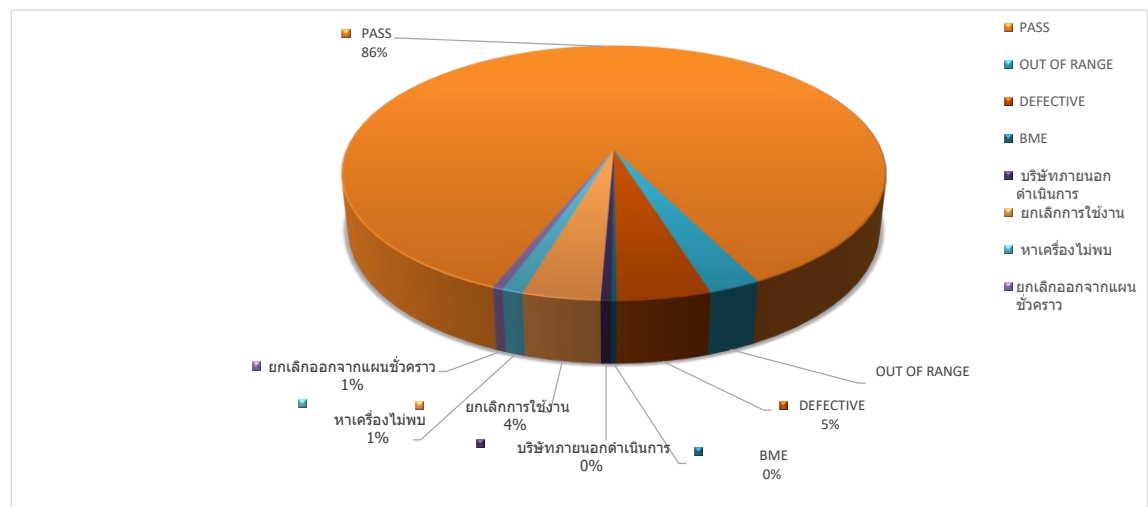


สรุปผลเครื่องมือที่ไม่ผ่านเกณฑ์การสอบเทียบ จำแนกตามเครื่องมือ

ชื่อเครื่องมือ	จำนวน
ELECTROSURGICAL UNITS, MONOPOLAR/BIPOLAR	2
INFUSION PUMPS	6
OXIMETERS, PULSE	2
Grand Total	10

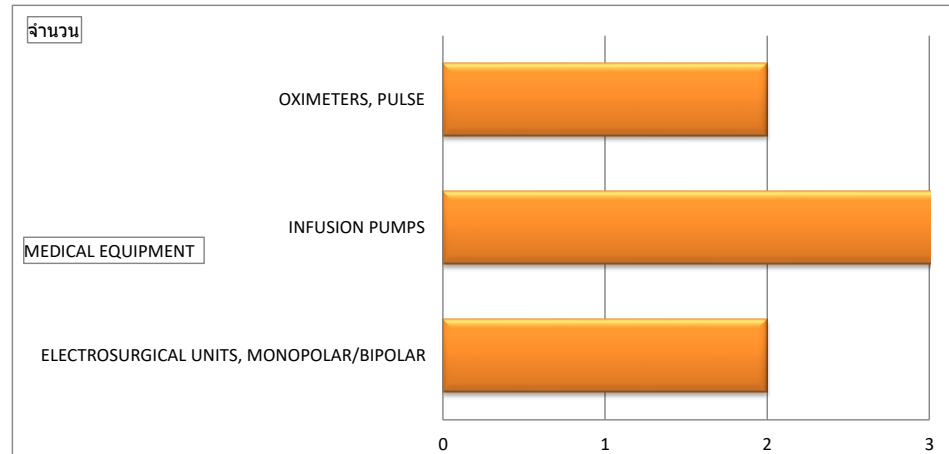


สรุปผลเครื่องมือที่ไม่ผ่านเกณฑ์การสอบเทียบ จำแนกตามแผนก

ชื่อแผนก	จำนวน
Emergency Room	1
Intensive Care Unit	1
Skin	1
Social Security	2
Ward B5	2
Ward B6	3
Grand Total	10

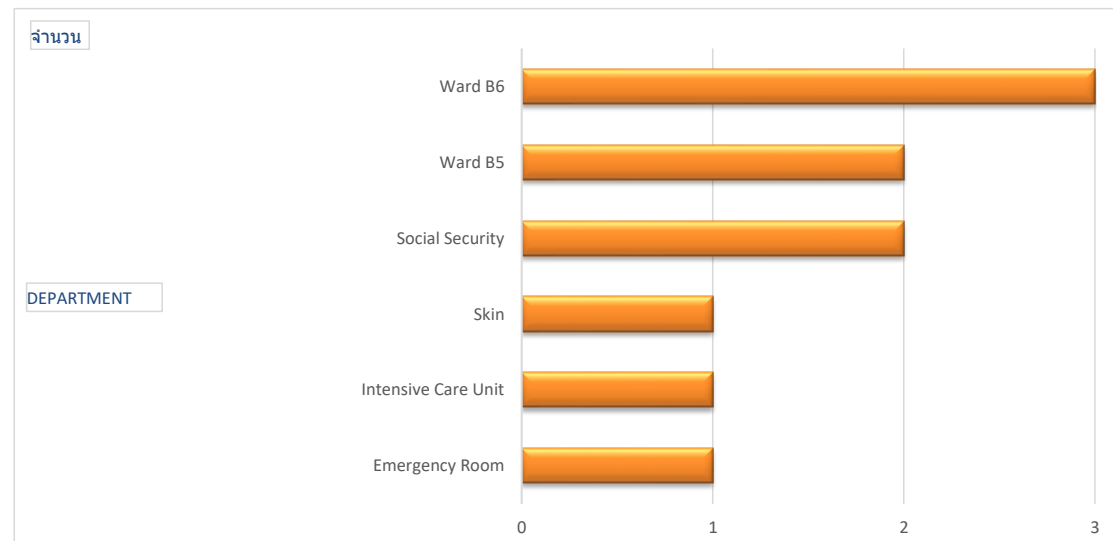

สรุปผลเครื่องที่ไม่สามารถดำเนินการ จำแนกตามสถานะ

ชื่อสถานะ	จำนวน
DEFECTIVE	18
บริษัทภายนอกดำเนินการ	2
หาเครื่องไม่พบ	4
ยกเลิกการใช้งาน	15
BME	1
ยกเลิกออกจากแผนชั่วคราว	2
Grand Total	42

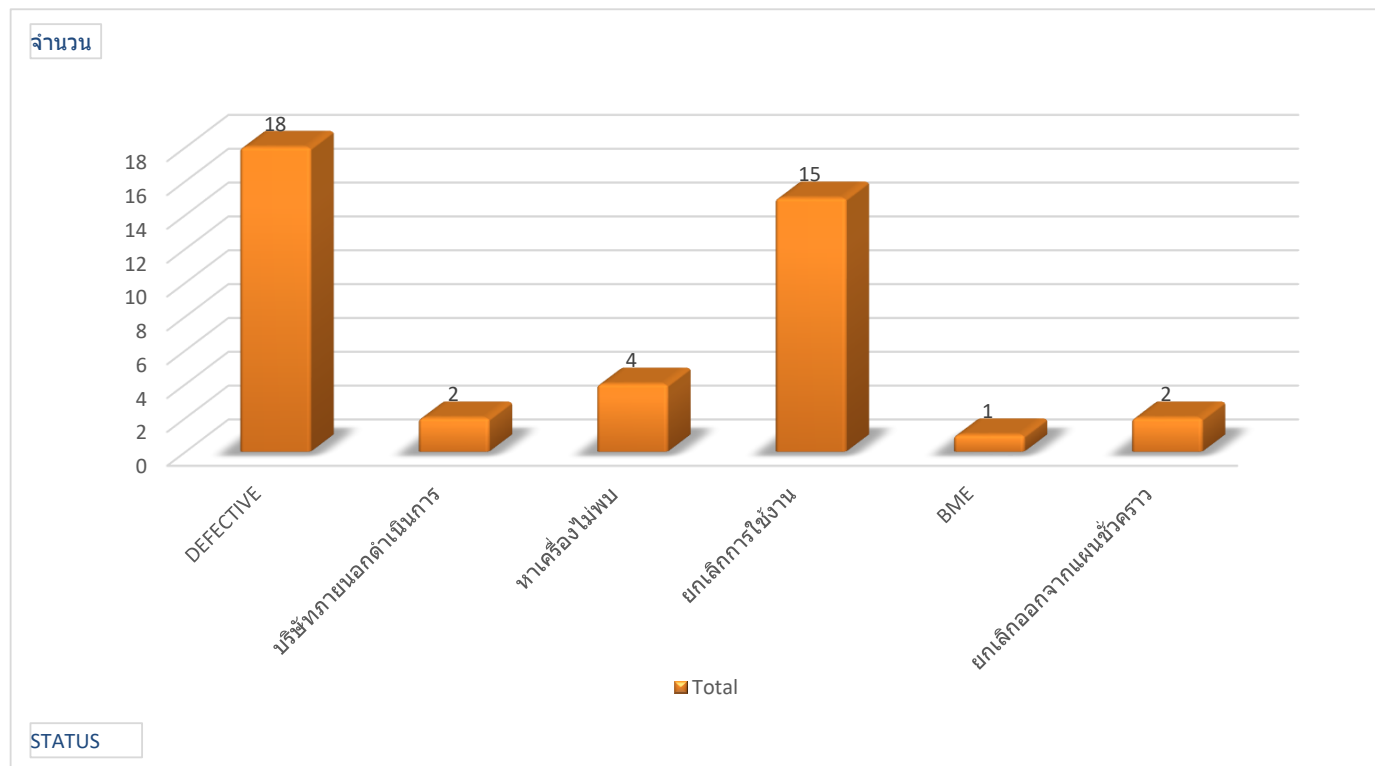

NO	ID CODE	Cer.No	PM.No	MEDICAL EQUIPMENT	BRAND	MODEL	S/N	DEPARTMENT	STATUS	REMARK
1	PLK00367	24PLK_0106240334	24PLK_01PM06240334	THERMO-HYGRO METER	VICTOR	VC230A	-	BME-PLK	PASS	
2	PLK00444	24PLK_0106240176	24PLK_01PM06240176	OXIMETERS, PULSE	-	-	-	BME-PLK	PASS	
3	PLK00689	-	-	INFUSION PUMPS	TOP	TOP-2300	GU26818B	BME-PLK	ยกเลิกการใช้งาน	24JUN24
4	PLK00735	24PLK_0106240294	24PLK_01PM06240294	INFUSION PUMPS	TOP	TOP-2300	GUX8406M	BME-PLK	PASS	Battery เสื่อม
5	PLK00971	24PLK_0106240064	24PLK_01PM06240064	OXIMETERS, PULSE	-	SO811	-	BME-PLK	PASS	
6	PLK00972	24PLK_0106240065	24PLK_01PM06240065	OXIMETERS, PULSE	-	SO811	-	BME-PLK	PASS	
7	PLK00975	24PLK_0106240066	24PLK_01PM06240066	OXIMETERS, PULSE	-	SO811	-	BME-PLK	PASS	
8	PLK00976	24PLK_0106240321	24PLK_01PM06240321	OXIMETERS, PULSE	-	-	-	BME-PLK	PASS	Code พาย
9	PLK00978	24PLK_0106240060	24PLK_01PM06240060	OXIMETERS, PULSE	-	SO811	-	BME-PLK	PASS	
10	PLK00980	24PLK_0106240059	24PLK_01PM06240059	OXIMETERS, PULSE	-	SO811	-	BME-PLK	PASS	
11	PLK00981	24PLK_0106240084	24PLK_01PM06240084	OXIMETERS, PULSE	-	SO811	-	BME-PLK	PASS	
12	PLK00982	24PLK_0106240061	24PLK_01PM06240061	OXIMETERS, PULSE	-	SO811	-	BME-PLK	PASS	
13	PLK00983	24PLK_0106240062	24PLK_01PM06240062	OXIMETERS, PULSE	-	SO811	-	BME-PLK	PASS	
14	PLK00984	24PLK_0106240106	24PLK_01PM06240106	OXIMETERS, PULSE	-	SO811	-	BME-PLK	PASS	
15	PLK00985	24PLK_0106240067	24PLK_01PM06240067	OXIMETERS, PULSE	-	SO811	-	BME-PLK	PASS	
16	PLK00986	24PLK_0106240070	24PLK_01PM06240069	OXIMETERS, PULSE	-	SO811	-	BME-PLK	PASS	
17	PLK00987	24PLK_0106240053	24PLK_01PM06240052	OXIMETERS, PULSE	-	SO811	-	BME-PLK	PASS	
18	PLK00988	24PLK_0106240203	24PLK_01PM06240203	OXIMETERS, PULSE	-	SO811	-	BME-PLK	PASS	
19	PLK00989	24PLK_0106240071	24PLK_01PM06240070	OXIMETERS, PULSE	-	SO811	-	BME-PLK	PASS	
20	PLK00990	24PLK_0106240083	24PLK_01PM06240083	OXIMETERS, PULSE	-	SO811	-	BME-PLK	PASS	
21	PLK00991	24PLK_0106240055	24PLK_01PM06240054	OXIMETERS, PULSE	-	SO811	-	BME-PLK	PASS	
22	PLK00992	24PLK_0106240300	24PLK_01PM06240300	OXIMETERS, PULSE	-	SO811	-	BME-PLK	PASS	
23	PLK00993	24PLK_0106240056	24PLK_01PM06240056	OXIMETERS, PULSE	-	SO811	-	BME-PLK	PASS	
24	PLK00995	24PLK_0106240058	24PLK_01PM06240058	OXIMETERS, PULSE	-	-	-	BME-PLK	PASS	
25	PLK00996	24PLK_0106240322	24PLK_01PM06240322	OXIMETERS, PULSE	-	-	-	BME-PLK	PASS	Code พาย
26	PLK00997	24PLK_0106240068	24PLK_01PM06240068	OXIMETERS, PULSE	-	-	-	BME-PLK	PASS	
27	PLK00998	24PLK_0106240063	24PLK_01PM06240063	OXIMETERS, PULSE	-	-	-	BME-PLK	PASS	
28	PLK00999	24PLK_0106240057	24PLK_01PM06240057	OXIMETERS, PULSE	-	-	-	BME-PLK	PASS	
29	PLK01300	24PLK_0106240054	24PLK_01PM06240053	OXIMETERS, PULSE	-	-	-	BME-PLK	PASS	
30	PLK01302	24PLK_0106240178	24PLK_01PM06240178	OXIMETERS, PULSE	☐	SO811	PLK-CRA-PUO-01	BME-PLK	PASS	
31	PLK01384	24PLK_0106240317	24PLK_01PM06240317	INFUSION PUMPS	MEDCAPTAIN	MP-60A	60190300858	BME-PLK	PASS	
32	PLK01523	24PLK_0106240299	24PLK_01PM06240299	OXIMETERS, PULSE	CHOICEMMED	MD300C1	192009304536	BME-PLK	PASS	
33	PLK01541	24PLK_0106240306	24PLK_01PM06240306	INFUSION PUMPS	ASIAHEALTH	HK-100II	-	BME-PLK	PASS	
34	PLK01543	24PLK_0106240111	24PLK_01PM06240111	INFUSION PUMPS	ASIAHEALTH	HK-100II	-	BME-PLK	PASS	
35	PLK01544	24PLK_0106240218	24PLK_01PM06240218	INFUSION PUMPS	ASIAHEALTH	HK-100II	-	BME-PLK	PASS	
36	PLK01547	24PLK_0106240319	24PLK_01PM06240319	INFUSION PUMPS	ASIAHEALTH	HK-100II	10294	BME-PLK	PASS	
37	PLK01549	24PLK_0106240074	24PLK_01PM06240074	INFUSION PUMPS	ASIAHEALTH	HK-100II	10370	BME-PLK	PASS	
38	PLK01550	24PLK_0106240228	24PLK_01PM06240228	INFUSION PUMPS	ASIAHEALTH	HK-100II	10370	BME-PLK	PASS	
39	PLK01551	24PLK_0106240240	24PLK_01PM06240240	INFUSION PUMPS	ASIAHEALTH	HK-100II	33966	BME-PLK	PASS	
40	PLK01552	24PLK_0106240035	24PLK_01PM06240035	INFUSION PUMPS	ASIAHEALTH	HK-100II	-	BME-PLK	PASS	
41	PLK01553	24PLK_0106240188	24PLK_01PM06240188	INFUSION PUMPS	ASIAHEALTH	HK-100II	22552	BME-PLK	PASS	
42	PLK01554	24PLK_0106240036	24PLK_01PM06240036	INFUSION PUMPS	ASIAHEALTH	HK-100II	10127	BME-PLK	PASS	
43	PLK01555	24PLK_0106240200	24PLK_01PM06240200	INFUSION PUMPS	ASIAHEALTH	HK-100II	10219	BME-PLK	PASS	
44	PLK01617	24PLK_0106240177	24PLK_01PM06240177	INFUSION PUMPS	ASIAHEALTH	HK-100II	20150306	BME-PLK	PASS	
45	PLK00836	24PLK_0106240269	24PLK_01PM06240269	MONITORS, PHYSIOLOGIC, VITAL SIGNS	Heal Force	CLASSIC-90	J2600MH00481	Checkup	PASS	ไม่มีสาย Sat
46	PLK00838	24PLK_0106240303	24PLK_01PM06240303	OXIMETERS, PULSE	☐	-	-	Checkup	PASS	
47	PLK01632	24PLK_0106240272	24PLK_01PM06240272	MONITORS, PHYSIOLOGIC, VITAL SIGNS	PHILIPS	EARLYVUE VS30	DE75144888	Checkup	PASS	
48	PLK01176	24PLK_0106240335	24PLK_01PM06240335	THERMO-HYGRO METER	VICTOR	VC230A	-	Dental	PASS	
49	PLK01183	24PLK_0106240096	24PLK_01PM06240096	ELECTROSURGICAL UNITS	Coltene/Whaledent	PERFECT TCS II	190409952	Dental	PASS	
50	PLK01190	24PLK_0106240277	24PLK_01PM06240277	MONITORS, PHYSIOLOGIC, VITAL SIGNS	NORTHER MEDITEC	AQUARIUS	J0122017	Dental	PASS	
51	PLK01215	24PLK_0106240097	24PLK_01PM06240097	ELECTROSURGICAL UNITS	Coltene/Whaledent	PERFECT TCS II	101019068	Dental	PASS	
52	PLK01516	24PLK_0106240332	24PLK_01PM06240332	FLOWMETERS, GAS OXYGEN	SOLIDA	15 LPM	AA53400	Dental	PASS	

NO	ID CODE	Cer.No	PM.No	MEDICAL EQUIPMENT	BRAND	MODEL	S/N	DEPARTMENT	STATUS	REMARK
53	PLK01609	24PLK_0106240072	24PLK_01PM06240071	ASPIRATORS, EMERGENCY	FLAEM	ASPIRA GO	23A0647 0233	Dental	PASS	
54	PLK00922	24PLK_0106240174	24PLK_01PM06240174	ASPIRATORS, EMERGENCY	BEING	BES-8030A	170680142	Ear Nose Throat Clinic	PASS	เครื่องสามารถปรับค่าได้ถึง 0.04 MPa(40 kPa) จากค่าสูงสุดของเครื่อง 0.1 MPa(100 kPa)
55	PLK00927	24PLK_0106240172	24PLK_01PM06240172	ASPIRATORS, EMERGENCY	SMAF	YX920S	1N2.084	Ear Nose Throat Clinic	PASS	
56	PLK00047	24PLK_0106240261	24PLK_01PM06240261	ASPIRATORS, EMERGENCY	FLAEM	PORT A SUCTION	15A564 0012	Emergency Room	PASS	ไม่สามารถหมุนปรับค่าได้ จึงสอบเทียบ ค่าจุดเดียว
57	PLK00165	24PLK_0106240166	24PLK_01PM06240166	DEFIBRILLATORS, EXTERNAL, MANUAL	MINDRAY	BENEHEART D3	EL-73034671	Emergency Room	PASS	
58	PLK00166	-	-	MONITORS, BEDSIDE, PHYSIOLOGIC	BIONET	BM5	D8S0500097	Emergency Room	DEFECTIVE	21Jun24
59	PLK00167	24PLK_0106240270	24PLK_01PM06240270	VENTILATORS, INTENSIVE CARE	DRAEGER	CARINA	ASKJ-0078	Emergency Room	PASS	
60	PLK00172	24PLK_0106240330	24PLK_01PM06240330	ASPIRATORS, EMERGENCY	FLAEM	PORT A SUCTION	17AD31 0116	Emergency Room	PASS	
61	PLK00179	24PLK_0106240162	24PLK_01PM06240162	DEFIBRILLATORS, EXTERNAL, AUTOMATED	ZOLL	AED PRO	AA16I040291	Emergency Room	PASS	ทดสอบค่าพลังงานได้ค่าเดียวเนื่องจาก แบตเตอรี่ไม่เพียงพอ, Alarm Change Battery : ควรแบตเตอรี่เพื่อความพร้อม ใช้งานของเครื่อง
62	PLK00180	24PLK_0106240271	24PLK_01PM06240271	DEFIBRILLATORS, EXTERNAL, MANUAL	ZOLL	R Series	AF19B093074	Emergency Room	PASS	กระดาดษหมด
63	PLK00188	24PLK_0106240268	24PLK_01PM06240268	MONITORS, PHYSIOLOGIC, VITAL SIGNS	RENCARE	I7000	1806200100100000	Emergency Room	PASS	
64	PLK00189	24PLK_0106240163	24PLK_01PM06240163	MONITORS, PHYSIOLOGIC, VITAL SIGNS	RENCARE	I7000	1809030100150010	Emergency Room	PASS	
65	PLK00190	24PLK_0106240267	24PLK_01PM06240267	MONITORS, PHYSIOLOGIC, VITAL SIGNS	RENCARE	I7000	1907310100100000	Emergency Room	PASS	
66	PLK00192	24PLK_0106240331	24PLK_01PM06240331	FLOWMETERS, GAS OXYGEN	SOLIDA	-	-	Emergency Room	PASS	
67	PLK00194	24PLK_0106240165	24PLK_01PM06240165	MONITORS, BEDSIDE, PHYSIOLOGIC	EDAN	IM70	360080-M21604630004	Emergency Room	PASS	
68	PLK00204	24PLK_0106240164	24PLK_01PM06240164	OXIMETERS, PULSE	EDAN	H100B	360101-M22507370003	Emergency Room	PASS	
69	PLK00205	24PLK_0107240001	24PLK_01PM07240001	OXIMETERS, PULSE	EDAN	H100B	360101-M22507370004	Emergency Room	PASS	
70	PLK00206	24PLK_0106240161	24PLK_01PM06240161	OXIMETERS, PULSE	NONIN	2500	129105504	Emergency Room	PASS	
71	PLK00207	24PLK_0106240219	24PLK_01PM06240219	ELECTROSURGICAL UNITS, MONOPOLAR/BIPOLAR	WEM	HF-120	3337	Emergency Room	OUT OF RANGE	
72	PLK00380	24PLK_0106240017	24PLK_01PM06240017	DEFIBRILLATORS, EXTERNAL, MANUAL	NIHON KOHDEN	TEC-5521K	9163	Emergency Room	PASS	Alarm Replace Battery
73	PLK00954	24PLK_0106240173	24PLK_01PM06240173	ASPIRATORS, EMERGENCY	FLAEM	PORT A SUCTION	17AG80 0036	Emergency Room	PASS	
74	PLK01356	-	-	MONITORS, PHYSIOLOGIC, RESPIRATON/EXHALED CARBON DIOXIDE/PULSE OXIMETRY, BEDSIDE	MASIMO	EMMA	-	Emergency Room	DEFECTIVE	Alarm Sensor
75	PLK01574	-	-	DEFIBRILLATORS, EXTERNAL, AUTOMATED	ZOLL	AED PLUS	AH191067689	Emergency Room	บริษัทภายนอกดำเนินการ	25/06
76	PLK00211	24PLK_0106240001	24PLK_01PM06240001	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	EFFICIA CM12	CN12001731	Intensive Care Unit	PASS	
77	PLK00212	24PLK_0106240208	24PLK_01PM06240208	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	EFFICIA CM12	CN12001725	Intensive Care Unit	PASS	
78	PLK00215	-	-	VENTILATORS, TRANSPORT	PNEUTON	S	S2148	Intensive Care Unit	DEFECTIVE	27JUN24 ไม่มีSet ไม่สามารถ Cal ได้
79	PLK00217	24PLK_0106240139	24PLK_01PM06240139	DEFIBRILLATORS, EXTERNAL, MANUAL	ZOLL	M Series	T05E70549	Intensive Care Unit	PASS	
80	PLK00231	24PLK_0106240011	24PLK_01PM06240013	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	EFFICIA CM12	CN92354006	Intensive Care Unit	PASS	
81	PLK00232	24PLK_0106240207	24PLK_01PM06240207	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	EFFICIA CM12	CN12001726	Intensive Care Unit	PASS	
82	PLK00233	24PLK_0106240002	24PLK_01PM06240002	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	EFFICIA CM12	CN92354004	Intensive Care Unit	PASS	
83	PLK00234	24PLK_0106240005	24PLK_01PM06240005	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	EFFICIA CM12	CN12001730	Intensive Care Unit	PASS	
84	PLK00235	24PLK_0106240209	24PLK_01PM06240209	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	EFFICIA CM12	CN92354003	Intensive Care Unit	PASS	
85	PLK00236	24PLK_0106240032	24PLK_01PM06240032	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	EFFICIA CM12	CN92354005	Intensive Care Unit	PASS	
86	PLK00237	24PLK_0106240023	24PLK_01PM06240024	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	EFFICIA CM12	CN12001723	Intensive Care Unit	PASS	
87	PLK00238	24PLK_0106240019	24PLK_01PM06240020	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	EFFICIA CM12	CN12001728	Intensive Care Unit	PASS	
88	PLK00239	-	-	VENTILATORS, INTENSIVE CARE	EVENT MEDICAL	INSPIRATION 5i	20115120353	Intensive Care Unit	DEFECTIVE	เปิดเครื่องไม่ติด
89	PLK00241	24PLK_0106240314	24PLK_01PM06240314	VENTILATORS, INTENSIVE CARE	PURITAN BENNETT	840	3512212232	Intensive Care Unit	PASS	
90	PLK00242	24PLK_0106240031	24PLK_01PM06240031	VENTILATORS, INTENSIVE CARE	DRAEGER	CARINA	ASKJ-0079	Intensive Care Unit	PASS	AC Plug No Ground
91	PLK00243	24PLK_0106240288	24PLK_01PM06240288	VENTILATORS, INTENSIVE CARE	EVENT	INSPIRATION LS	2004W0030057	Intensive Care Unit	PASS	No O2 Sensor, Compressor ใช้งานไม่ได้
92	PLK00257	24PLK_0106240018	24PLK_01PM06240018	DEFIBRILLATORS, EXTERNAL, MANUAL	NIHON KOHDEN	TEC-5631	5511	Intensive Care Unit	PASS	Alarm Empty Battery
93	PLK00258	24PLK_0106240007	24PLK_01PM06240008	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	EFFICIA CM12	CN92354002	Intensive Care Unit	PASS	
94	PLK00260	24PLK_0106240282	24PLK_01PM06240282	VENTILATORS, INTENSIVE CARE	EVENT MEDICAL	EVOLUTION 3E	EVL50937	Intensive Care Unit	PASS	O2 Sensor failed
95	PLK00265	24PLK_0106240004	24PLK_01PM06240004	RESPIROMETER	NSPIRE	HALOSCALE, STANDARD	H55506S	Intensive Care Unit	PASS	
96	PLK00266	24PLK_0106240003	24PLK_01PM06240003	MONITORS, PHYSIOLOGIC, RESPIRATON/EXHALED CARBON DIOXIDE/PULSE OXIMETRY, BEDSIDE	MASIMO	EMMA	246616	Intensive Care Unit	PASS	Carbon Dioxide Concentration 5% (36.8 mmHg) ±2.6 mmHg Carbon Dioxide Concentration 10% (73.6 mmHg) ±5.2 mmHg

NO	ID CODE	Cer.No	PM.No	MEDICAL EQUIPMENT	BRAND	MODEL	S/N	DEPARTMENT	STATUS	REMARK
97	PLK00271	24PLK_0106240025	24PLK_01PM06240025	OXYGEN HIGH FLOW	FISHER & PAYKEL HEALTHCARE	AIRVO 2	210416257362	Intensive Care Unit	PASS	
98	PLK00272	24PLK_0106240021	24PLK_01PM06240021	OXYGEN HIGH FLOW	FISHER & PAYKEL HEALTHCARE	AIRVO 2	210417257946	Intensive Care Unit	PASS	
99	PLK00273	24PLK_0106240024	24PLK_01PM06240023	OXYGEN HIGH FLOW	FISHER & PAYKEL HEALTHCARE	AIRVO 2	201109201453	Intensive Care Unit	PASS	
100	PLK00274	24PLK_0106240022	24PLK_01PM06240022	OXYGEN HIGH FLOW	FISHER & PAYKEL HEALTHCARE	AIRVO 2	201222237424	Intensive Care Unit	PASS	
101	PLK00275	24PLK_0106240020	24PLK_01PM06240019	OXYGEN HIGH FLOW	FISHER & PAYKEL HEALTHCARE	AIRVO 2	201120208986	Intensive Care Unit	PASS	
102	PLK00276	-	-	OXYGEN HIGH FLOW	COMEN	NF5	F5210615085C	Intensive Care Unit	DEFECTIVE	24JUN24 ส่งซ่อมบริษัท
103	PLK00277	24PLK_0106240026	24PLK_01PM06240026	OXYGEN HIGH FLOW	COMEN	NF5	F5210201171C	Intensive Care Unit	PASS	
104	PLK00279	24PLK_0106240014	24PLK_01PM06240014	INFUSION PUMPS	MEDCAPTAIN	MP-60	60190300878	Intensive Care Unit	PASS	
105	PLK00280	24PLK_0106240033	24PLK_01PM06240033	INFUSION PUMPS	MEDCAPTAIN	MP-60	60180703031	Intensive Care Unit	PASS	
106	PLK00281	24PLK_0106240222	24PLK_01PM06240222	INFUSION PUMPS	MEDCAPTAIN	MP-60	60180703026	Intensive Care Unit	PASS	AC Plug ขา Ground หัก
107	PLK00282	24PLK_0106240013	24PLK_01PM06240012	INFUSION PUMPS	MEDCAPTAIN	MP-60	60180703023	Intensive Care Unit	PASS	
108	PLK00283	24PLK_0106240008	24PLK_01PM06240007	INFUSION PUMPS	MEDCAPTAIN	MP-60	60160700721	Intensive Care Unit	PASS	
109	PLK00284	24PLK_0106240196	24PLK_01PM06240196	INFUSION PUMPS	MEDCAPTAIN	MP-60	60190300881	Intensive Care Unit	PASS	
110	PLK00292	24PLK_0106240221	24PLK_01PM06240221	INFUSION PUMPS	MEDCAPTAIN	MP-60	60190300836	Intensive Care Unit	PASS	
111	PLK00303	-	-	OXYGEN HIGH FLOW	FISHER & PAYKEL HEALTHCARE	AIRVO 2	201222237396	Intensive Care Unit	DEFECTIVE	รอนบริษัทเข้ามาตรวจสอบ
112	PLK00305	24PLK_0106240213	24PLK_01PM06240213	MONITORS, PHYSIOLOGIC, CENTRAL STATION	PHILIPS	-	-	Intensive Care Unit	PASS	
113	PLK00307	-	-	ASPIRATORS, EMERGENCY	KONSUNG	9E-A	MA22040361279	Intensive Care Unit	DEFECTIVE	17JUN24 เช็มน้ไม่หมุนตามค่าที่ปรับ
114	PLK00308	24PLK_0106240175	24PLK_01PM06240175	ASPIRATORS, EMERGENCY	KONSUNG	9E-A	MA22040361280	Intensive Care Unit	PASS	
115	PLK00386	24PLK_0106240210	24PLK_01PM06240210	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	EFFICIA CM12	CN12001724	Intensive Care Unit	PASS	
116	PLK00390	24PLK_0106240192	24PLK_01PM06240192	INFUSION PUMPS	MEDCAPTAIN	MP-60	60180703036	Intensive Care Unit	PASS	
117	PLK00392	24PLK_0106240316	24PLK_01PM06240316	INFUSION PUMPS	MEDCAPTAIN	MP-60	60180703024	Intensive Care Unit	PASS	
118	PLK00394	24PLK_0106240220	24PLK_01PM06240220	ASPIRATORS, EMERGENCY	KONSUNG	9E-A	MA22040361094	Intensive Care Unit	PASS	
119	PLK00601	24PLK_0106240197	24PLK_01PM06240197	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	EFFICIA CM12	CN12001729	Intensive Care Unit	PASS	
120	PLK00688	24PLK_0106240324	24PLK_01PM06240324	INFUSION PUMPS	TOP	TOP-2300	15A0902	Intensive Care Unit	OUT OF RANGE	
121	PLK00773	24PLK_0106240325	24PLK_01PM06240325	INFUSION PUMPS	TOP	TOP-2300	15A0887	Intensive Care Unit	PASS	Alarm Battery
122	PLK01115	24PLK_0106240214	24PLK_01PM06240214	ASPIRATORS, EMERGENCY	KONSUNG	9E-A	Ma22040360148	Intensive Care Unit	PASS	
123	PLK01378	24PLK_0106240333	24PLK_01PM06240333	PACEMAKERS, CARDIAC, EXTERNAL	MEDTRONIC	5375	CE1005627R	Intensive Care Unit	PASS	
124	PLK01380	24PLK_0106240015	24PLK_01PM06240015	INFUSION PUMPS	MEDCAPTAIN	MP-60A	60190300875	Intensive Care Unit	PASS	
125	PLK01381	24PLK_0106240034	24PLK_01PM06240034	INFUSION PUMPS	MEDCAPTAIN	MP-60	60190300859	Intensive Care Unit	PASS	
126	PLK01382	24PLK_0106240012	24PLK_01PM06240011	INFUSION PUMPS	MEDCAPTAIN	MP-60	60190300862	Intensive Care Unit	PASS	
127	PLK01387	-	-	INFUSION PUMPS	MEDCAPTAIN	MP-60	60151100999	Intensive Care Unit	ยกเลิกการใช้งาน	26JUN24
128	PLK01388	24PLK_0106240190	24PLK_01PM06240190	INFUSION PUMPS	MEDCAPTAIN	MP-60	60190300874	Intensive Care Unit	PASS	
129	PLK01418	24PLK_0106240191	24PLK_01PM06240191	INFUSION PUMPS	MEDCAPTAIN	MP-60A	60190300841	Intensive Care Unit	PASS	AC Plug ขา Ground หัก
130	PLK01419	24PLK_0106240280	24PLK_01PM06240280	INFUSION PUMPS	MEDCAPTAIN	MP-60	60190300841	Intensive Care Unit	PASS	
131	PLK01420	24PLK_0106240195	24PLK_01PM06240195	INFUSION PUMPS	MEDCAPTAIN	MP-60	60180703029	Intensive Care Unit	PASS	AC Plug ขา Ground หัก
132	PLK01421	24PLK_0106240009	24PLK_01PM06240009	INFUSION PUMPS	MEDCAPTAIN	MP-60A	60180703034	Intensive Care Unit	PASS	
133	PLK01422	24PLK_0106240010	24PLK_01PM06240010	INFUSION PUMPS	MEDCAPTAIN	MP-60	60180703032	Intensive Care Unit	PASS	
134	PLK01465	24PLK_0106240285	24PLK_01PM06240285	VENTILATORS, INTENSIVE CARE	PURITAN BENNETT	840	3512212233	Intensive Care Unit	PASS	
135	PLK01469	24PLK_0106240286	24PLK_01PM06240286	VENTILATORS, INTENSIVE CARE	PURITAN BENNETT	840	3512221269	Intensive Care Unit	PASS	O2 Sensor failed
136	PLK01485	24PLK_0106240212	24PLK_01PM06240212	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	EFFICIA CM12	CN92354001	Intensive Care Unit	PASS	
137	PLK01556	24PLK_0106240315	24PLK_01PM06240315	VENTILATORS, INTENSIVE CARE	DRAEGER	SAVINA 300	A55C-0286	Intensive Care Unit	PASS	
138	PLK01557	24PLK_0106240134	24PLK_01PM06240134	INFUSION PUMPS	ASIAHEALTH	HK-100II	22558	Intensive Care Unit	PASS	
139	PLK01558	24PLK_0106240243	24PLK_01PM06240243	INFUSION PUMPS	ASIAHEALTH	HK-100II	14129	Intensive Care Unit	PASS	
140	PLK01559	24PLK_0106240006	24PLK_01PM06240006	VENTILATORS, INTENSIVE CARE	PURITAN BENNETT	840	3512230377	Intensive Care Unit	PASS	
141	PLK01560	24PLK_0106240281	24PLK_01PM06240281	VENTILATORS, INTENSIVE CARE	PURITAN BENNETT	840	35122303882	Intensive Care Unit	PASS	
142	PLK01575	24PLK_0106240149	24PLK_01PM06240150	INFUSION PUMPS	ASIAHEALTH	HK-100II	10172	Intensive Care Unit	PASS	
143	PLK01576	24PLK_0106240193	24PLK_01PM06240193	INFUSION PUMPS	ASIAHEALTH	HK-100II	22554	Intensive Care Unit	PASS	AC Plug ขา Ground หัก
144	PLK01579	24PLK_0106240211	24PLK_01PM06240211	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	EFFICIA CM12	CN12001722	Intensive Care Unit	PASS	
145	PLK01604	-	-	INFUSION PUMPS	ASIAHEALTH	HK-100II	10488	Intensive Care Unit	ยกเลิกการใช้งาน	24JUN24
146	PLK01605	24PLK_0106240253	24PLK_01PM06240253	INFUSION PUMPS	ASIAHEALTH	HK-100II	-	Intensive Care Unit	PASS	
147	PLK01634	24PLK_0106240205	24PLK_01PM06240205	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	EFFICIA CM12	CN12021267	Intensive Care Unit	PASS	
148	PLK01635	24PLK_0106240204	24PLK_01PM06240204	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	EFFICIA CM12	CN12021265	Intensive Care Unit	PASS	
149	PLK01636	24PLK_0106240206	24PLK_01PM06240206	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	EFFICIA CM12	CN12001695	Intensive Care Unit	PASS	

NO	ID CODE	Cer.No	PM.No	MEDICAL EQUIPMENT	BRAND	MODEL	S/N	DEPARTMENT	STATUS	REMARK
150	PLK01637	-	-	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	EFFICIA CM12	CN12001693	Intensive Care Unit	DEFECTIVE	17JUN24 ค่าBPไม่ผ่าน
151	PLK01675	24PLK_0106240180	24PLK_01PM06240180	THERMO-HYGRO METER	TEMPERATURE	HTC-2	-	INVENTORY	PASS	
152	PLK01677	24PLK_0106240181	24PLK_01PM06240181	THERMO-HYGRO METER	TEMPERATURE	HTC-2	-	INVENTORY	PASS	
153	PLK01678	24PLK_0106240182	24PLK_01PM06240182	THERMO-HYGRO METER	TEMPERATURE	HTC-2	-	INVENTORY	PASS	
154	PLK00113	24PLK_0106240075	24PLK_01PM06240075	MONITORS, PHYSIOLOGIC, VITAL SIGNS	Heal Force	CLASSIC-90	J2600MH00379	Labour Room	PASS	
155	PLK00121	-	-	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	6010180703592	Labour Room	DEFECTIVE	18JUN24
156	PLK00122	24PLK_0106240047	24PLK_01PM06240046	DETECTORS, FETAL HEART, ULTRASONIC	EDAN	F6	560038-M21810010004	Labour Room	PASS	
157	PLK00123	24PLK_0106240048	24PLK_01PM06240048	DETECTORS, FETAL HEART, ULTRASONIC	BISTOS	BT-350	AFH90162	Labour Room	PASS	
158	PLK00129	24PLK_0106240076	24PLK_01PM06240076	WARMING UNITS, PATIENT, RADIANT, INFANT	ATOM	V-3200N	8112497	Labour Room	PASS	
159	PLK00135	24PLK_0106240049	24PLK_01PM06240049	VACUUM EXTRACTOR, OBSTETRIC	MEDIST	MEVACS	1007101-1	Labour Room	PASS	
160	PLK00136	-	-	VACUUM EXTRACTOR, OBSTETRIC	ATOM	VP-500	1131	Labour Room	ยกเลิกการใช้งาน	18JUN24
161	PLK00137	-	-	DETECTORS, FETAL HEART, ULTRASONIC	OXFORD	SONICAID TEAM	-	Labour Room	ยกเลิกการใช้งาน	18JUN24
162	PLK00138	-	-	DETECTORS, FETAL HEART, ULTRASONIC	HUNTLEIGH HEALTHCARE	SONICAID TEAM CARE	738XL0206125-11	Labour Room	ยกเลิกการใช้งาน	18JUN24
163	PLK00142	-	-	MONITORS, PHYSIOLOGIC, VITAL SIGNS	CRITIKON DINAMAP	8101	8101-J1140	Labour Room	ยกเลิกออกจากแผนชั่วคราว	18JUN24 Cal DEC24
164	PLK00156	24PLK_0106240077	24PLK_01PM06240077	MONITORS, PHYSIOLOGIC, VITAL SIGNS	Heal Force	CLASSIC-90	J2600N00358	Labour Room	PASS	
165	PLK00797	24PLK_0106240171	24PLK_01PM06240171	OXIMETERS, PULSE	BEIJING CHOICE	MD300C1	192009301786	Medicine	PASS	
166	PLK00804	24PLK_0106240323	24PLK_01PM06240323	OXIMETERS, PULSE	-	-	-	Medicine	PASS	Code หาย
167	PLK00817	24PLK_0106240169	24PLK_01PM06240169	OXIMETERS, PULSE	EDAN	H100B	360101-M21900430036	Medicine	PASS	
168	PLK00821	24PLK_0106240308	24PLK_01PM06240308	MONITORING SYSTEMS, PHYSIOLOGIC, STRESS EXERCISE, CARDIAC	GE HEALTHCARE	T2100-ST2	STE194800015A	Medicine	PASS	
169	PLK00860	24PLK_0106240170	24PLK_01PM06240170	OXIMETERS, PULSE	CHOICEMMED	MD300C1	192009304540	Medicine	PASS	
170	PLK01493	24PLK_0106240183	24PLK_01PM06240183	MONITORS, PHYSIOLOGIC, VITAL SIGNS	NORTHER MEDITEC	AQUARIUS	I0305015	Medicine	PASS	
171	PLK01622	24PLK_0106240276	24PLK_01PM06240276	MONITORS, PHYSIOLOGIC, VITAL SIGNS	PHILIPS	EARLYVUE VS30	DF72412895	Medicine	PASS	
172	PLK00979	24PLK_0106240201	24PLK_01PM06240201	OXIMETERS, PULSE	-	SO811	-	Mobile Checkup	PASS	
173	PLK00075	24PLK_0106240043	24PLK_01PM06240042	INCUBATORS, INFANT	ATOM	V-85	5100305	Nursery	PASS	
174	PLK00076	24PLK_0106240042	24PLK_01PM06240041	INCUBATORS, INFANT, TRANSPORT	FANEM	IT-158-TS	CF9582	Nursery	PASS	
175	PLK00080	24PLK_0106240039	24PLK_01PM06240039	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	EFFICIA CM12	CN12001721	Nursery	PASS	
176	PLK00081	24PLK_0106240041	24PLK_01PM06240040	MONITORS, PHYSIOLOGIC, VITAL SIGNS	RENCARE	I7000	1909110111200000	Nursery	PASS	
177	PLK00082	24PLK_0106240226	24PLK_01PM06240226	INCUBATORS, INFANT	ATOM	AIR INCU I	210700649	Nursery	PASS	
178	PLK00083	24PLK_0106240044	24PLK_01PM06240043	INCUBATORS, INFANT	ATOM	RABEE INCU I	26Y1328	Nursery	PASS	
179	PLK00084	24PLK_0106240045	24PLK_01PM06240044	WARMING UNITS, PATIENT, RADIANT, INFANT	ATOM	SUNFLOWER WARMER	200600173	Nursery	PASS	
180	PLK00085	24PLK_0106240046	24PLK_01PM06240045	RESUSCITATORS, PULMONARY	ATOM	RESUSCI FLOW	200600683	Nursery	PASS	
181	PLK00088	24PLK_0106240037	24PLK_01PM06240037	RESUSCITATORS, PULMONARY	FISHER & PAYKEL HEALTHCARE	NEOPUFF	190515019705	Nursery	PASS	
182	PLK00089	24PLK_0106240320	24PLK_01PM06240320	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	6010180703554	Nursery	PASS	
183	PLK00091	24PLK_0106240051	24PLK_01PM06240055	INFUSION PUMPS, SYRINGE	MEDCAPTAIN	SYS-3011	180119080079	Nursery	PASS	
184	PLK00093	24PLK_0106240069	24PLK_01PM06240072	VENTILATORS, INTENSIVE CARE	EVENT	INSPIRATION LS	2009W030454	Nursery	PASS	O2 Sensor เสื่อม
185	PLK00094	24PLK_0106240227	24PLK_01PM06240227	INCUBATORS, INFANT, TRANSPORT	ATOM	V-707	210700894	Nursery	PASS	
186	PLK00844	24PLK_0106240160	24PLK_01PM06240160	MONITORS, PHYSIOLOGIC, VITAL SIGNS	NORTHER MEDITEC	AQUARIUS	1806200100100000	OPD Orthopedics	PASS	
187	PLK01633	24PLK_0106240273	24PLK_01PM06240273	MONITORS, PHYSIOLOGIC, VITAL SIGNS	PHILIPS	EARLYVUE VS30	DE75144889	OPD Orthopedics	PASS	
188	PLK00214	-	-	MONITORS, PHYSIOLOGIC, VITAL SIGNS	CRITIKON DINAMAP	1846 SX	8261 H2111	Operating Room	ยกเลิกการใช้งาน	20JUN24
189	PLK00216	-	-	OXIMETERS, PULSE	OHMEDA	BIOX 3740	FMQW01371	Operating Room	ยกเลิกการใช้งาน	20JUN24
190	PLK00459	24PLK_0106240185	24PLK_01PM06240185	ANESTHESIA UNITS	GE HEALTHCARE	CARESTATION 650	SM721350050MA	Operating Room	PASS	
191	PLK00459(VEN)	24PLK_0106240184	24PLK_01PM06240184	VENTILATORS, ANESTHESIA	GE HEALTHCARE	CARESTATION 650	SM721350050MA	Operating Room	PASS	
192	PLK00461	24PLK_0106240264	24PLK_01PM06240264	ANESTHESIA UNITS, VAPORIZER	DRAGER	VAPOR 2000	02050203EN0000	Operating Room	PASS	
193	PLK00462	24PLK_0106240146	24PLK_01PM06240145	MONITORS, BEDSIDE, PHYSIOLOGIC	MINDRAY	MEC-2000	CV-5B115902	Operating Room	PASS	Carbon Dioxide Concentration 5% (36.8 mmHg) ±2.6 mmHg Carbon Dioxide Concentration 10% (73.6 mmHg) ±5.2 mmHg
194	PLK00463	24PLK_0106240135	24PLK_01PM06240135	ELECTROSURGICAL UNITS, MONOPOLAR/BIPOLAR	COVIDIEN	VALLEYLAB FT10	T9C31406DX	Operating Room	PASS	
195	PLK00469	24PLK_0106240266	24PLK_01PM06240266	TOURNIQUETS, PNEUMATIC	-	-	-	Operating Room	PASS	

NO	ID CODE	Cer.No	PM.No	MEDICAL EQUIPMENT	BRAND	MODEL	S/N	DEPARTMENT	STATUS	REMARK
196	PLK00473	24PLK_0106240029	24PLK_01PM06240030	ANESTHESIA UNITS	DAMECA	SIESTA I WHISPA	AM508 5401	Operating Room	PASS	
197	PLK00473(VEN)	24PLK_0106240030	24PLK_01PM06240029	VENTILATORS, ANESTHESIA	DAMECA	SIESTA I WHISPA	AM508 5401	Operating Room	PASS	
198	PLK00474	24PLK_0106240297	24PLK_01PM06240297	MONITORS, BEDSIDE, PHYSIOLOGIC	MINDRAY	MEC-2000	CV-43112330	Operating Room	PASS	Carbon Dioxide Concentration 5% (36.8 mmHg) ±2.6 mmHg Carbon Dioxide Concentration 10% (73.6 mmHg) ±5.2 mmHg
199	PLK00475	24PLK_0106240028	24PLK_01PM06240028	ANESTHESIA UNITS, VAPORIZER	DATEX-OHMEDA	TEC 7	BEJV07698	Operating Room	PASS	
200	PLK00476	24PLK_0106240133	24PLK_01PM06240133	ELECTROSURGICAL UNITS, MONOPOLAR/BIPOLAR	COVIDIEN	FORCE FX	S7J27429AX	Operating Room	PASS	
201	PLK00481	24PLK_0106240155	24PLK_01PM06240155	TOURNIQUETS, PNEUMATIC	-	-	-	Operating Room	PASS	
202	PLK00482	-	-	ANESTHESIA UNITS, VAPORIZER	DATEX-OHMEDA	TEC 7	BEGR02477	Operating Room	ยกเลิกการใช้งาน	25/06
203	PLK00483	24PLK_0106240027	24PLK_01PM06240027	ANESTHESIA UNITS, VAPORIZER	PENLON	SIGMA DELTA	D12070123	Operating Room	PASS	
204	PLK00497	24PLK_0106240263	24PLK_01PM06240263	WARMING UNITS, PATIENT, RADIANT, INFANT	FISHER & PAYKEL HEALTHCARE	IW703	9503AEA00286	Operating Room	PASS	
205	PLK00498	24PLK_0106240262	24PLK_01PM06240262	RESUSCITATORS, PULMONARY	FISHER & PAYKEL HEALTHCARE	NEOPUFF RD1000	-	Operating Room	PASS	
206	PLK00510	24PLK_0106240156	24PLK_01PM06240156	ASPIRATORS, SURGICAL	-	-	-	Operating Room	PASS	
207	PLK00514	24PLK_0106240140	24PLK_01PM06240140	INFUSION PUMPS, SYRINGE	TOP	TOP-5300	BM40406E	Operating Room	PASS	
208	PLK00515	24PLK_0106240141	24PLK_01PM06240141	INFUSION PUMPS, SYRINGE	TOP	TOP-5300	BM40407E	Operating Room	PASS	
209	PLK00524	24PLK_0106240304	24PLK_01PM06240304	ANESTHESIA UNITS	DAMECA	SIESTA	200750026	Operating Room	PASS	
210	PLK00525	-	-	ANESTHESIA UNITS, VAPORIZER	PENLON	SIGMA DELTA	D10070481	Operating Room	DEFECTIVE	25JUN24 นำยาหมด
211	PLK00526	24PLK_0106240307	24PLK_01PM06240307	ANESTHESIA UNITS, VAPORIZER	DATEX-OHMEDA	TEC 7	BEJS04174	Operating Room	PASS	
212	PLK00527	-	-	VENTILATORS, TRANSPORT	DAMECA	MCM 890-3S	200726001	Operating Room	DEFECTIVE	25/06
213	PLK00534	24PLK_0106240137	24PLK_01PM06240137	ELECTROSURGICAL UNITS, MONOPOLAR/BIPOLAR	ERBE	VIO 300D	11284070	Operating Room	PASS	
214	PLK00541	24PLK_0106240050	24PLK_01PM06240050	ELECTROSURGICAL UNITS	COVIDIEN	FORCE FX	F5J42334A	Operating Room	PASS	
215	PLK00544	24PLK_0106240136	24PLK_01PM06240136	ELECTROSURGICAL UNITS	ELLMAN	SURGITRON F.F.P.F EMC	3428	Operating Room	PASS	ทดสอบค่าพลังงานใน Mode II
216	PLK00556	24PLK_0106240187	24PLK_01PM06240187	ANESTHESIA UNITS	DAMECA	SIESTA I WHISPA	DK43102039	Operating Room	PASS	
217	PLK00556(VEN)	24PLK_0106240186	24PLK_01PM06240186	VENTILATORS, ANESTHESIA	DAMECA	SIESTA I WHISPA	DK43102039	Operating Room	PASS	
218	PLK00557	24PLK_0106240265	24PLK_01PM06240265	ANESTHESIA UNITS, VAPORIZER	PENLON	SIGMA DELTA	D10070502	Operating Room	PASS	
219	PLK00558	24PLK_0106240298	24PLK_01PM06240298	MONITORS, BEDSIDE, PHYSIOLOGIC	MINDRAY	MEC-2000	CV-26108620	Operating Room	PASS	Carbon Dioxide Concentration 5% (36.8 mmHg) ±2.6 mmHg Carbon Dioxide Concentration 10% (73.6 mmHg) ±5.2 mmHg
220	PLK00562	24PLK_0106240138	24PLK_01PM06240138	ELECTROSURGICAL UNITS, MONOPOLAR/BIPOLAR	COVIDIEN	FORCE FX	S4K15598AX	Operating Room	PASS	
221	PLK00568	-	-	ANESTHESIA UNITS	DAMECA	SIESTA	200750027	Operating Room	ยกเลิกการใช้งาน	25/06
222	PLK00569	-	-	ANESTHESIA UNITS, VAPORIZER	PENLON	SIGMA DELTA	D10070484	Operating Room	ยกเลิกการใช้งาน	25/06
223	PLK00570	-	-	VENTILATORS, TRANSPORT	DAMECA	MCM 890-3S	200748003	Operating Room	ยกเลิกการใช้งาน	20JUN24
224	PLK00599	24PLK_0106240198	24PLK_01PM06240198	MONITORS, BEDSIDE, PHYSIOLOGIC	MINDRAY	UMEC12	KQ-8B017901	Operating Room	PASS	
225	PLK00600	24PLK_0106240199	24PLK_01PM06240199	MONITORS, BEDSIDE, PHYSIOLOGIC	MINDRAY	UMEC12	KQ-8B017902	Operating Room	PASS	
226	PLK00602	24PLK_0106240157	24PLK_01PM06240157	WARMING UNITS, PATIENT, FORCED-AIR	3M Health Care	775	10126	Operating Room	PASS	
227	PLK01114	-	-	INFUSION PUMPS	TOP	TOP-2200	BLY0255S	Operating Room	หาเครื่องใหม่	
228	PLK01158	-	-	PHACOEMULSIFICATION UNITS, CATARACT EXTRACTION	Alcon	LEGION	2201910001X	Operating Room	BME	PM By Site
229	PLK01307	24PLK_0106240154	24PLK_01PM06240153	TOURNIQUETS, PNEUMATIC	VBM	TOURNIQUET TOUCH TT20	1280	Operating Room	PASS	
230	PLK01309	24PLK_0106240150	24PLK_01PM06240149	WARMING UNITS, PATIENT, FORCED-AIR	3M Health Care	775	-	Operating Room	PASS	
231	PLK01445	24PLK_0106240152	24PLK_01PM06240151	MONITORS, BEDSIDE, PHYSIOLOGIC	MINDRAY	UMEC12	KQ-18070965	Operating Room	PASS	Carbon Dioxide Concentration 5% (36.8 mmHg) ±2.6 mmHg Carbon Dioxide Concentration 10% (73.6 mmHg) ±5.2 mmHg
232	PLK01446	24PLK_0106240148	24PLK_01PM06240147	MONITORS, BEDSIDE, PHYSIOLOGIC	MINDRAY	UMEC12	KQ-29093966	Operating Room	PASS	Carbon Dioxide Concentration 5% (36.8 mmHg) ±2.6 mmHg Carbon Dioxide Concentration 10% (73.6 mmHg) ±5.2 mmHg
233	PLK01656	-	-	ELECTROSURGICAL UNITS, HIGH FREQUENCY	SUTTER MEDIZINTECHNIK	CURIS RF-GENERATOR	BM17000707232514	Operating Room	บริษัทภายนอกดำเนินการ	เครื่องอยู่ในประกัน
234	PLK00054	24PLK_0106240079	24PLK_01PM06240079	MONITORS, PHYSIOLOGIC, VITAL SIGNS	EDAN	M3	302041-M11A02630003	Pediatrics Clinic	PASS	

NO	ID CODE	Cer.No	PM.No	MEDICAL EQUIPMENT	BRAND	MODEL	S/N	DEPARTMENT	STATUS	REMARK
235	PLK00055	24PLK_0106240081	24PLK_01PM06240081	INFUSION PUMPS	TOP	TOP-2300	GUX8407M	Pediatrics Clinic	PASS	
236	PLK00056	24PLK_0106240080	24PLK_01PM06240080	OXIMETERS, PULSE	EDAN	H100B	360101-M19A06480009	Pediatrics Clinic	PASS	
237	PLK00313	24PLK_0106240085	24PLK_01PM06240085	MONITORS, PHYSIOLOGIC, VITAL SIGNS	NORTHER MEDITEC	AQUARIUS	JH20210809051	Physical Therapy	PASS	
238	PLK00928	24PLK_0106240052	24PLK_01PM06240051	ELECTROSURGICAL UNITS, MONOPOLAR/BIPOLAR	WEM	HF-120	3339	Skin	OUT OF RANGE	
239	PLK00378	24PLK_0106240094	24PLK_01PM06240094	MONITORS, PHYSIOLOGIC, VITAL SIGNS	Heal Force	CLASSIC-90	J2600MH00415	Social Security	PASS	
240	PLK01075	24PLK_0106240278	24PLK_01PM06240278	OXIMETERS, PULSE	EDAN	H100B	113575-M14402030001	Social Security	PASS	
241	PLK01079	24PLK_0106240279	24PLK_01PM06240279	MONITORS, PHYSIOLOGIC, VITAL SIGNS	Heal Force	CLASSIC-90	J2600MH00413	Social Security	PASS	
242	PLK01085	24PLK_0106240305	24PLK_01PM06240305	SPHYGMOMANOMETERS, MERCURY	ALPK2	-	-	Social Security	PASS	
243	PLK01414	24PLK_0106240302	24PLK_01PM06240302	OXIMETERS, PULSE	BLT	M70B	M058E149936	Social Security	OUT OF RANGE	
244	PLK01524	24PLK_0106240301	24PLK_01PM06240301	OXIMETERS, PULSE	-	-	-	Social Security	OUT OF RANGE	
245	PLK01525	24PLK_0106240312	24PLK_01PM06240312	OXIMETERS, PULSE	-	-	-	Social Security	PASS	
246	PLK00024	24PLK_0106240274	24PLK_01PM06240274	ASPIRATORS, EMERGENCY	THOMAS	MEDI-PUMP	-	Transportation	PASS	
247	PLK00031	24PLK_0106240275	24PLK_01PM06240275	ASPIRATORS, EMERGENCY	THOMAS	MEDI-PUMP	31500012932	Transportation	PASS	
248	PLK00040	24PLK_0106240168	24PLK_01PM06240168	ASPIRATORS, EMERGENCY	FLAEM	PORT A SUCTION	18A245 0002	Transportation	PASS	
249	PLK00994	24PLK_0106240202	24PLK_01PM06240202	OXIMETERS, PULSE	-	-	-	TTB สนง.ใหญ่	PASS	
250	PLK00108	-	-	INFUSION PUMPS	SHENZHEN HAWK MEDICAL	HK-100II	10370	Ward A3	หาเครื่องไม่พบ	
251	PLK00112	24PLK_0106240073	24PLK_01PM06240073	INFUSION PUMPS	TOP	TOP-2300	GU26822B	Ward A3	PASS	
252	PLK00114	24PLK_0106240038	24PLK_01PM06240038	MONITORS, PHYSIOLOGIC, VITAL SIGNS	RENCARE	I7000	1906170100100000	Ward A3	PASS	
253	PLK01365	-	-	MONITORS, PHYSIOLOGIC, VITAL SIGNS	GE HEALTHCARE	DINAMAP PROCARE 300	AAW052302005A	Ward A3	DEFECTIVE	18JUN24 Cal ไม่ผ่าน ไม่สามารถซ่อมได้
254	PLK01367	24PLK_0106240040	24PLK_01PM06240047	INFUSION PUMPS, SYRINGE	TERUMO	TE-331	1302000682	Ward A3	PASS	
255	PLK00516	-	-	INFUSION PUMPS	TOP	TOP-2200	BL79019S	Ward B3	ยกเลิกการใช้งาน	24JUN24
256	PLK00690	24PLK_0106240087	24PLK_01PM06240087	MONITORS, PHYSIOLOGIC, VITAL SIGNS	Heal Force	CLASSIC-90	J2600MH00466	Ward B3	PASS	
257	PLK00728	24PLK_0106240117	24PLK_01PM06240117	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	6010180401717	Ward B3	PASS	
258	PLK00730	-	-	OXIMETERS, PULSE	EDAN	H100B	113575-M11A01970005	Ward B3	ยกเลิกการใช้งาน	25/06
259	PLK00741	24PLK_0106240091	24PLK_01PM06240091	OXIMETERS, PULSE	CHOICEMMED	MD300C2	210355410591	Ward B3	PASS	
260	PLK00745	24PLK_0106240090	24PLK_01PM06240090	OXIMETERS, PULSE	CHOICEMMED	MD300C22	210355410403	Ward B3	PASS	
261	PLK00768	24PLK_0106240122	24PLK_01PM06240122	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	6010180401713	Ward B3	PASS	
262	PLK01429	24PLK_0106240093	24PLK_01PM06240093	MONITORS, PHYSIOLOGIC, VITAL SIGNS	RENCARE	I7000	JH20220302027	Ward B3	PASS	AC Plug ขา Ground หัก
263	PLK01449	24PLK_0106240114	24PLK_01PM06240114	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	1410120010018	Ward B3	PASS	
264	PLK01450	24PLK_0106240113	24PLK_01PM06240113	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	1410120010049	Ward B3	PASS	
265	PLK01451	24PLK_0106240116	24PLK_01PM06240116	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	250119100041	Ward B3	PASS	
266	PLK01452	24PLK_0106240238	24PLK_01PM06240238	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	1410120010020	Ward B3	PASS	
267	PLK01453	24PLK_0106240120	24PLK_01PM06240120	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	1410120020090	Ward B3	PASS	
268	PLK01454	24PLK_0106240237	24PLK_01PM06240237	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	1410120010010	Ward B3	PASS	
269	PLK01455	24PLK_0106240234	24PLK_01PM06240234	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	1410120020088	Ward B3	PASS	
270	PLK01456	24PLK_0106240119	24PLK_01PM06240119	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	250119100063	Ward B3	PASS	
271	PLK01457	24PLK_0106240235	24PLK_01PM06240235	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	250119100055	Ward B3	PASS	
272	PLK01458	24PLK_0106240121	24PLK_01PM06240121	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	1410120010034	Ward B3	PASS	
273	PLK01459	24PLK_0106240236	24PLK_01PM06240236	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	1410120010003	Ward B3	PASS	
274	PLK01460	24PLK_0106240118	24PLK_01PM06240118	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	1410120010043	Ward B3	PASS	
275	PLK01461	-	-	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	1410120010004	Ward B3	DEFECTIVE	24JUN24 ส่งซ่อมบริษัท
276	PLK01462	24PLK_0106240112	24PLK_01PM06240112	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	1410120010008	Ward B3	PASS	
277	PLK01463	24PLK_0106240115	24PLK_01PM06240115	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	1410120010014	Ward B3	PASS	
278	PLK01538	24PLK_0106240089	24PLK_01PM06240089	OXIMETERS, PULSE	CHOICEMMED	MD300C22	210355410672	Ward B3	PASS	
279	PLK01583	24PLK_0106240088	24PLK_01PM06240088	OXIMETERS, PULSE	EDAN	H100B	360101-M23414830003	Ward B3	PASS	
280	PLK00655	24PLK_0106240092	24PLK_01PM06240092	MONITORS, PHYSIOLOGIC, VITAL SIGNS	NORTHER MEDITEC	AQUARIUS	J0122016	Ward B4	PASS	
281	PLK00666	24PLK_0106240251	24PLK_01PM06240251	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	1410120010045	Ward B4	PASS	
282	PLK00670	24PLK_0106240123	24PLK_01PM06240123	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	1410120010035	Ward B4	PASS	
283	PLK00692	24PLK_0106240252	24PLK_01PM06240252	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	1410120010009	Ward B4	PASS	
284	PLK00695	24PLK_0106240246	24PLK_01PM06240246	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	250119100057	Ward B4	PASS	
285	PLK00698	24PLK_0106240125	24PLK_01PM06240125	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	1410120010015	Ward B4	PASS	
286	PLK00701	24PLK_0106240254	24PLK_01PM06240254	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	1410120010023	Ward B4	PASS	
287	PLK00704	-	-	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	1410120010025	Ward B4	DEFECTIVE	24JUN24 ส่งซ่อมบริษัท
288	PLK00707	24PLK_0106240127	24PLK_01PM06240127	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	1410120010039	Ward B4	PASS	
289	PLK00710	24PLK_0106240247	24PLK_01PM06240247	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	1410120010022	Ward B4	PASS	

NO	ID CODE	Cer.No	PM.No	MEDICAL EQUIPMENT	BRAND	MODEL	S/N	DEPARTMENT	STATUS	REMARK
290	PLK00712	-	-	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	1410120010041	Ward B4	DEFECTIVE	24JUN24 ส่งซ่อมบริษัท
291	PLK00714	-	-	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	1410120020056	Ward B4	DEFECTIVE	24JUN24 ส่งซ่อมบริษัท
292	PLK00716	24PLK_0106240329	24PLK_01PM06240329	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	250119100035	Ward B4	PASS	
293	PLK00719	24PLK_0106240244	24PLK_01PM06240244	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	1410120010030	Ward B4	PASS	
294	PLK00722	24PLK_0106240245	24PLK_01PM06240245	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	1410120010040	Ward B4	PASS	
295	PLK00977	24PLK_0106240144	24PLK_01PM06240144	OXIMETERS, PULSE	-	SO811	-	Ward B4	PASS	
296	PLK01317	24PLK_0106240124	24PLK_01PM06240124	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	1410120010007	Ward B4	PASS	
297	PLK01323	24PLK_0106240126	24PLK_01PM06240126	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	1410120010016	Ward B4	PASS	
298	PLK00210	-	-	INFUSION PUMPS	TOP	TOP-2300	14A0786	Ward B5	ยกเลิกการใช้งาน	24JUN24
299	PLK00365	24PLK_0106240225	24PLK_01PM06240225	INFUSION PUMPS	TOP	TOP-2300	GU26899B	Ward B5	PASS	
300	PLK00738	24PLK_0106240016	24PLK_01PM06240016	INFUSION PUMPS	TOP	TOP-2300	GU16646B	Ward B5	PASS	
301	PLK00784	24PLK_0106240215	24PLK_01PM06240215	INFUSION PUMPS	TOP	TOP-2300	14A0745	Ward B5	OUT OF RANGE	
302	PLK01113	24PLK_0106240318	24PLK_01PM06240318	INFUSION PUMPS	TOP	TOP-2300	GU26903B	Ward B5	PASS	
303	PLK01119	24PLK_0106240223	24PLK_01PM06240223	INFUSION PUMPS	TOP	TOP-2200	EL67961S	Ward B5	PASS	
304	PLK01139	24PLK_0106240224	24PLK_01PM06240224	INFUSION PUMPS	TOP	TOP-2200	BL79023S	Ward B5	PASS	
305	PLK01142	24PLK_0106240078	24PLK_01PM06240078	INFUSION PUMPS	TOP	TOP-2200	BL79021S	Ward B5	OUT OF RANGE	
306	PLK01151	24PLK_0106240100	24PLK_01PM06240100	MONITORS, PHYSIOLOGIC, VITAL SIGNS	Heal Force	CLASSIC-90	J2600MH00445	Ward B5	PASS	
307	PLK01152	24PLK_0106240086	24PLK_01PM06240086	MONITORS, PHYSIOLOGIC, VITAL SIGNS	RENCARE	I7000	1906170100100000	Ward B5	PASS	
308	PLK01153	24PLK_01PM06240109	24PLK_01PM06240109	OXIMETERS, PULSE	CHOICEMMED	MD300C22	210355410598	Ward B5	PASS	
309	PLK01310	-	-	MONITORS, PHYSIOLOGIC, VITAL SIGNS	CRITIKON DINAMAP	8101	8101-H5858	Ward B5	ยกเลิกออกจากแผนชั่วคราว	25/06 CAL DEC
310	PLK01537	24PLK_0106240110	24PLK_01PM06240110	OXIMETERS, PULSE	CHOICEMMED	MD300C22	2103554 10595	Ward B5	PASS	
311	PLK00353	24PLK_0106240217	24PLK_01PM06240217	INFUSION PUMPS	TOP	TOP-2300	14A078	Ward B6	OUT OF RANGE	
312	PLK00356	24PLK_0106240095	24PLK_01PM06240095	MONITORS, PHYSIOLOGIC, VITAL SIGNS	Heal Force	CLASSIC-90	J2600MH00386	Ward B6	PASS	
313	PLK00357	24PLK_0106240098	24PLK_01PM06240098	OXIMETERS, PULSE	CHOICEMMED	MD300C1	192009304535	Ward B6	PASS	
314	PLK00359	24PLK_0106240099	24PLK_01PM06240099	MONITORS, PHYSIOLOGIC, VITAL SIGNS	NORTHER MEDITEC	AQUARIUS	J0122013	Ward B6	PASS	AC Plug ขา Ground หัก
315	PLK00360	24PLK_0106240230	24PLK_01PM06240230	INFUSION PUMPS	TOP	TOP-2300	FU26279B	Ward B6	PASS	
316	PLK00368	24PLK_0106240231	24PLK_01PM06240231	INFUSION PUMPS	TOP	TOP-2200	EL67929	Ward B6	PASS	
317	PLK00369	24PLK_0106240233	24PLK_01PM06240233	INFUSION PUMPS	TOP	TOP-2300	GUY8672M	Ward B6	PASS	
318	PLK00371	24PLK_0106240293	24PLK_01PM06240293	INFUSION PUMPS	TOP	TOP-2300	GU26900B	Ward B6	PASS	Battery เสื่อม
319	PLK00373	-	-	INFUSION PUMPS	TOP	TOP-2300	GU26897B	Ward B6	หาเครื่องใหม่	
320	PLK00374	24PLK_0106240229	24PLK_01PM06240229	INFUSION PUMPS	TOP	TOP-2200	BLV0252S	Ward B6	PASS	AC Plug ขา Ground หัก
321	PLK00375	24PLK_0106240216	24PLK_01PM06240216	INFUSION PUMPS	TOP	TOP-2200	BL79022S	Ward B6	OUT OF RANGE	
322	PLK00381	24PLK_0106240189	24PLK_01PM06240189	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	EFFICIA CM12	CN12001727	Ward B6	PASS	
323	PLK00388	24PLK_0106240242	24PLK_01PM06240242	INFUSION PUMPS	TOP	TOP-2200	EL67930S	Ward B6	PASS	AC Plug ขา Ground หัก
324	PLK00389	24PLK_0106240194	24PLK_01PM06240194	INFUSION PUMPS	MEDCAPTAIN	MP-60	60190300880	Ward B6	PASS	
325	PLK00395	24PLK_0106240241	24PLK_01PM06240241	INFUSION PUMPS	TOP	TOP-2300	FU26280B	Ward B6	PASS	
326	PLK00397	24PLK_0106240232	24PLK_01PM06240232	INFUSION PUMPS	TOP	TOP-2300	GU26823B	Ward B6	PASS	
327	PLK00399	24PLK_0106240296	24PLK_01PM06240296	INFUSION PUMPS	TOP	TOP-2300	GU26904B	Ward B6	OUT OF RANGE	
328	PLK01498	24PLK_0106240313	24PLK_01PM06240313	ASPIRATORS, EMERGENCY	KONSUNG	9E-A	Ma22040360147	Ward B6	PASS	
329	PLK01000	24PLK_0106240103	24PLK_01PM06240103	MONITORS, PHYSIOLOGIC, VITAL SIGNS	Heal Force	CLASSIC-90	J2600MH00391	Ward B7	PASS	
330	PLK01001	24PLK_0106240104	24PLK_01PM06240104	MONITORS, PHYSIOLOGIC, VITAL SIGNS	NORTHER MEDITEC	AQUARIUS	J0122019	Ward B7	PASS	
331	PLK01002	24PLK_0106240105	24PLK_01PM06240105	OXIMETERS, PULSE	EDAN	H100B	113575-M12400480010	Ward B7	PASS	
332	PLK01014	24PLK_0106240153	24PLK_01PM06240154	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	6010181105874	Ward B7	PASS	
333	PLK01017	24PLK_0106240295	24PLK_01PM06240295	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	6010190301770	Ward B7	PASS	
334	PLK01020	24PLK_0106240131	24PLK_01PM06240131	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	6010190301883	Ward B7	PASS	
335	PLK01023	24PLK_0106240151	24PLK_01PM06240152	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	6010190301834	Ward B7	PASS	AC Plug ขา Ground หัก
336	PLK01026	24PLK_0106240260	24PLK_01PM06240260	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	6010181105897	Ward B7	PASS	AC Plug ขา Ground หัก
337	PLK01029	24PLK_0106240327	24PLK_01PM06240327	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	6010190301788	Ward B7	PASS	
338	PLK01032	24PLK_0106240147	24PLK_01PM06240148	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	6010190301876	Ward B7	PASS	
339	PLK01035	24PLK_0106240129	24PLK_01PM06240129	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	6010181105796	Ward B7	PASS	
340	PLK01038	24PLK_0106240128	24PLK_01PM06240128	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	6010180703556	Ward B7	PASS	
341	PLK01041	24PLK_0106240259	24PLK_01PM06240259	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	6010180703581	Ward B7	PASS	AC Plug ขา Ground หัก
342	PLK01044	24PLK_0106240158	24PLK_01PM06240158	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	6010181105865	Ward B7	PASS	
343	PLK01047	24PLK_0106240239	24PLK_01PM06240239	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	6010190301845	Ward B7	PASS	
344	PLK01050	-	-	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	6010181105762	Ward B7	หาเครื่องใหม่	
345	PLK01053	24PLK_0106240143	24PLK_01PM06240143	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	6010190301807	Ward B7	PASS	

NO	ID CODE	Cer.No	PM.No	MEDICAL EQUIPMENT	BRAND	MODEL	S/N	DEPARTMENT	STATUS	REMARK
346	PLK01056	24PLK_0106240145	24PLK_01PM06240146	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	6010190301838	Ward B7	PASS	
347	PLK01059	24PLK_0106240130	24PLK_01PM06240130	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	6010190301731	Ward B7	PASS	AC Plug ขา Ground หัก
348	PLK01062	24PLK_0106240142	24PLK_01PM06240142	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	6010190301896	Ward B7	PASS	
349	PLK01065	24PLK_0106240132	24PLK_01PM06240132	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	6010190301867	Ward B7	PASS	AC Plug ขา Ground หัก
350	PLK00867	24PLK_0106240107	24PLK_01PM06240107	MONITORS, PHYSIOLOGIC, VITAL SIGNS	Heal Force	CLASSIC-90	J2600MH00459	Ward B8	PASS	ไม่มีสาย Sat
351	PLK00869	24PLK_0106240310	24PLK_01PM06240310	OXIMETERS, PULSE	CHOICEMMED	MD300C1	192009304538	Ward B8	PASS	
352	PLK00882	24PLK_0106240256	24PLK_01PM06240256	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	6010190301890	Ward B8	PASS	AC Plug ขา Ground หัก
353	PLK00890	24PLK_0106240284	24PLK_01PM06240284	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	6010190301784	Ward B8	PASS	
354	PLK00892	24PLK_0106240311	24PLK_01PM06240311	OXIMETERS, PULSE	CHOICEMMED	MD300C1	192009304532	Ward B8	PASS	
355	PLK00894	24PLK_0106240287	24PLK_01PM06240287	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	6010190301851	Ward B8	PASS	
356	PLK00897	24PLK_0106240255	24PLK_01PM06240255	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	6010190301792	Ward B8	PASS	
357	PLK00900	24PLK_0106240283	24PLK_01PM06240283	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	6010190301810	Ward B8	PASS	
358	PLK00902	24PLK_0106240250	24PLK_01PM06240250	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	6010180703562	Ward B8	PASS	
359	PLK00905	24PLK_0106240248	24PLK_01PM06240248	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	6010180703600	Ward B8	PASS	
360	PLK00907	24PLK_0106240291	24PLK_01PM06240291	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	6010180401740	Ward B8	PASS	
361	PLK00909	24PLK_0106240326	24PLK_01PM06240326	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	6010180703540	Ward B8	PASS	
362	PLK00913	24PLK_0106240289	24PLK_01PM06240289	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	6010190301747	Ward B8	PASS	
363	PLK00914	24PLK_0106240159	24PLK_01PM06240159	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	6010170702304	Ward B8	PASS	
364	PLK01304	24PLK_0106240258	24PLK_01PM06240258	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	601017070702306	Ward B8	PASS	
365	PLK01325	24PLK_0106240249	24PLK_01PM06240249	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	6010190301779	Ward B8	PASS	
366	PLK01326	24PLK_0106240290	24PLK_01PM06240290	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	6010190301826	Ward B8	PASS	
367	PLK01327	24PLK_0106240257	24PLK_01PM06240257	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	6010180703575	Ward B8	PASS	
368	PLK01329	24PLK_0106240309	24PLK_01PM06240309	OXIMETERS, PULSE	-	-	-	Ward B8	PASS	
369	PLK01330	24PLK_0106240108	24PLK_01PM06240108	OXIMETERS, PULSE	CHOICEMMED	MD300C22	210355410578	Ward B8	PASS	
370	PLK01331	24PLK_0106240292	24PLK_01PM06240292	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	6010190301827	Ward B8	PASS	
371	PLK01341	24PLK_0106240101	24PLK_01PM06240101	MONITORS, PHYSIOLOGIC, VITAL SIGNS	Heal Force	CLASSIC-90	J2600MH00433	Ward B8	PASS	
372	PLK01423	24PLK_0106240328	24PLK_01PM06240328	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	6010190301766	Ward B8	PASS	
373	PLK01526	-	-	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	6010171206799	Ward B8	DEFECTIVE	24JUN24 ค่าOcclusionไม่ผ่าน
374	PLK01540	24PLK_0106240082	24PLK_01PM06240082	OXIMETERS, PULSE	CHOICEMMED	MD300C29	202508709639	Ward B8	PASS	
375	PLK01542	24PLK_0106240102	24PLK_01PM06240102	OXIMETERS, PULSE	EDAN	H100B	113575-M11A01970036	Ward B8	PASS	
376	PLK00017	-	-	INJECTORS, CONTRAST MEDIA	Apollo	APO 100	APO100Z2161003	X-RAY	DEFECTIVE	25/06
377	PLK00018	24PLK_0106240167	24PLK_01PM06240167	MONITORS, PHYSIOLOGIC, VITAL SIGNS	Heal Force	CLASSIC-90	J2600LG00312	X-RAY	PASS	
378	PLK01682	24PLK_0106240179	24PLK_01PM06240179	OXIMETERS, PULSE	ฐ	-	-	คลินิกเวชกรรมเปาโล อาคาร ชั้นทาวเวอร์	PASS	
379	PLK01427	24PLK_0106240336	24PLK_01PM06240336	MONITORS, PHYSIOLOGIC, VITAL SIGNS	RENCARE	I7000	JH20220302016	ชั้นทาวเวอร์	PASS	
380	PLK01301	24PLK_0106240341	24PLK_01PM06240341	OXIMETERS, PULSE	-	-	-	ถนนเพชรบุรี	PASS	
381	PLK01287	24PLK_0106240338	24PLK_01PM06240338	MONITORS, PHYSIOLOGIC, VITAL SIGNS	NORTHER MEDITEC	AQUARIUS	I0904023	วงศ์สว่าง	PASS	
382	PLK01250	24PLK_0106240337	24PLK_01PM06240337	MONITORS, PHYSIOLOGIC, VITAL SIGNS	NORTHER MEDITEC	AQUARIUS	I0904024	สหคลินิกเปาโล TTB	PASS	ไม่มีสาย Sat
383	PLK01269	24PLK_0106240340	24PLK_01PM06240340	MONITORS, PHYSIOLOGIC, VITAL SIGNS	NORTHER MEDITEC	AQUARIUS	I0904026	อาคาร ธ.ก.ส	PASS	
384	PLK01428	24PLK_0106240339	24PLK_01PM06240339	MONITORS, PHYSIOLOGIC, VITAL SIGNS	RENCARE	I7000	JH20220302024	อาคาร ธ.ก.ส	PASS	

No.	ID CODE	Cer.No	PM.No	MEDICAL EQUIPMENT	BRAND	MODEL	S/N	DEPARTMENT	STATUS	REMARK
1	PLK00207	24PLK_0106240219	24PLK_01PM06240219	ELECTROSURGICAL UNITS, MONOPOLAR/BIPOLAR	WEM	HF-120	3337	Emergency Room	OUT OF RANGE	
2	PLK00688	24PLK_0106240324	24PLK_01PM06240324	INFUSION PUMPS	TOP	TOP-2300	15A0902	Intensive Care Unit	OUT OF RANGE	
3	PLK00928	24PLK_0106240052	24PLK_01PM06240051	ELECTROSURGICAL UNITS, MONOPOLAR/BIPOLAR	WEM	HF-120	3339	Skin	OUT OF RANGE	
4	PLK01414	24PLK_0106240302	24PLK_01PM06240302	OXIMETERS, PULSE	BLT	M70B	M058E149936	Social Security	OUT OF RANGE	
5	PLK01524	24PLK_0106240301	24PLK_01PM06240301	OXIMETERS, PULSE	-	-	-	Social Security	OUT OF RANGE	
6	PLK00784	24PLK_0106240215	24PLK_01PM06240215	INFUSION PUMPS	TOP	TOP-2300	14A0745	Ward B5	OUT OF RANGE	
7	PLK01142	24PLK_0106240078	24PLK_01PM06240078	INFUSION PUMPS	TOP	TOP-2200	BL79021S	Ward B5	OUT OF RANGE	
8	PLK00353	24PLK_0106240217	24PLK_01PM06240217	INFUSION PUMPS	TOP	TOP-2300	14A078	Ward B6	OUT OF RANGE	
9	PLK00375	24PLK_0106240216	24PLK_01PM06240216	INFUSION PUMPS	TOP	TOP-2200	BL79022S	Ward B6	OUT OF RANGE	
10	PLK00399	24PLK_0106240296	24PLK_01PM06240296	INFUSION PUMPS	TOP	TOP-2300	GU26904B	Ward B6	OUT OF RANGE	

No.	ID CODE	Cer.No	PM.No	MEDICAL EQUIPMENT	BRAND	MODEL	S/N	DEPARTMENT	STATUS	REMARK
1	PLK00689	-	-	INFUSION PUMPS	TOP	TOP-2300	GU26818B	BME-PLK	ยกเลิกการใช้งาน	24JUN24
2	PLK00166	-	-	MONITORS, BEDSIDE, PHYSIOLOGIC	BIONET	BM5	D8S0500097	Emergency Room	DEFECTIVE	21Jun24
3	PLK01356	-	-	MONITORS, PHYSIOLOGIC, RESPIRATOR/EXHALED CARBON DIOXIDE/PULSE OXIMETRY, BEDSIDE	MASIMO	EMMA	-	Emergency Room	DEFECTIVE	Alarm Sensor
4	PLK01574	-	-	DEFIBRILLATORS, EXTERNAL, AUTOMATED	ZOLL	AED PLUS	AH191067689	Emergency Room	บริษัทภายนอกดำเนินการ	25/06
5	PLK00215	-	-	VENTILATORS, TRANSPORT	PNEUTON	S	S2148	Intensive Care Unit	DEFECTIVE	27JUN24 ไม่มีSet ไม่สามารถ Cal ได้
6	PLK00239	-	-	VENTILATORS, INTENSIVE CARE	EVENT MEDICAL	INSPIRATION 5i	20115120353	Intensive Care Unit	DEFECTIVE	เปิดเครื่องไม่ติด
7	PLK00276	-	-	OXYGEN HIGH FLOW	COMEN	NF5	F5210615085C	Intensive Care Unit	DEFECTIVE	24JUN24 ส่งซ่อม บริษัท
8	PLK00303	-	-	OXYGEN HIGH FLOW	FISHER & PAYKEL HEALTHCARE	AIRVO 2	201222237396	Intensive Care Unit	DEFECTIVE	รอบริษัทเข้ามา ตรวจสอบ
9	PLK00307	-	-	ASPIRATORS, EMERGENCY	KONSUNG	9E-A	MA22040361279	Intensive Care Unit	DEFECTIVE	17JUN24 เชื่อมไม่ หมดตามค่าที่ปรับ
10	PLK01387	-	-	INFUSION PUMPS	MEDCAPTAIN	MP-60	60151100999	Intensive Care Unit	ยกเลิกการใช้งาน	26JUN24
11	PLK01604	-	-	INFUSION PUMPS	ASIAHEALTH	HK-100II	10488	Intensive Care Unit	ยกเลิกการใช้งาน	24JUN24
12	PLK01637	-	-	MONITORS, BEDSIDE, PHYSIOLOGIC	PHILIPS	EFFICIA CM12	CN12001693	Intensive Care Unit	DEFECTIVE	17JUN24 ค่าBPไม่ ผ่าน
13	PLK00121	-	-	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	6010180703592	Labour Room	DEFECTIVE	18JUN24
14	PLK00136	-	-	VACUUM EXTRACTOR, OBSTETRIC	ATOM	VP-500	1131	Labour Room	ยกเลิกการใช้งาน	18JUN24
15	PLK00137	-	-	DETECTORS, FETAL HEART, ULTRASONIC	OXFORD	SONICAID TEAM	-	Labour Room	ยกเลิกการใช้งาน	18JUN24
16	PLK00138	-	-	DETECTORS, FETAL HEART, ULTRASONIC	HUNTLEIGH HEALTHCARE	SONICAID TEAM CARE	738XL0206125-11	Labour Room	ยกเลิกการใช้งาน	18JUN24
17	PLK00142	-	-	MONITORS, PHYSIOLOGIC, VITAL SIGNS	CRITIKON DINAMAP	8101	8101-J1140	Labour Room	ยกเลิกออกจากแผนชั่วคราว	18JUN24 Cal DEC24
18	PLK00214	-	-	MONITORS, PHYSIOLOGIC, VITAL SIGNS	CRITIKON DINAMAP	1846 SX	8261 H2111	Operating Room	ยกเลิกการใช้งาน	20JUN24
19	PLK00216	-	-	OXIMETERS, PULSE	OHMEDA	BIOX 3740	FMQW01371	Operating Room	ยกเลิกการใช้งาน	20JUN24
20	PLK00482	-	-	ANESTHESIA UNITS, VAPORIZER	DATEX-OHMEDA	TEC 7	BEGR02477	Operating Room	ยกเลิกการใช้งาน	25/06
21	PLK00525	-	-	ANESTHESIA UNITS, VAPORIZER	PENLON	SIGMA DELTA	D10070481	Operating Room	DEFECTIVE	25JUN24 น้ำยาหมด
22	PLK00527	-	-	VENTILATORS, TRANSPORT	DAMECA	MCM 890-3S	200726001	Operating Room	DEFECTIVE	25/06
23	PLK00568	-	-	ANESTHESIA UNITS	DAMECA	SIESTA	200750027	Operating Room	ยกเลิกการใช้งาน	25/06
24	PLK00569	-	-	ANESTHESIA UNITS, VAPORIZER	PENLON	SIGMA DELTA	D10070484	Operating Room	ยกเลิกการใช้งาน	25/06

No.	ID CODE	Cer.No	PM.No	MEDICAL EQUIPMENT	BRAND	MODEL	S/N	DEPARTMENT	STATUS	REMARK
25	PLK00570	-	-	VENTILATORS, TRANSPORT	DAMECA	MCM 890-3S	200748003	Operating Room	ยกเลิกการใช้งาน	20JUN24
26	PLK01114	-	-	INFUSION PUMPS	TOP	TOP-2200	BLY0255S	Operating Room	หาเครื่องไม่พบ	
27	PLK01158	-	-	PHACOEMULSIFICATION UNITS, CATARACT EXTRACTION	Alcon	LEGION	2201910001X	Operating Room	BME	PM By Site
28	PLK01656	-	-	ELECTROSURGICAL UNITS, HIGH FREQUENCY	SUTTER MEDIZINTECHNIK	CURIS RF-GENERATOR	BM17000707232514	Operating Room	บริษัทภายนอกดำเนินการ	เครื่องอยู่ในประกัน
29	PLK00108	-	-	INFUSION PUMPS	SHENZHEN HAWK MEDICAL	HK-100II	10370	Ward A3	หาเครื่องไม่พบ	
30	PLK01365	-	-	MONITORS, PHYSIOLOGIC, VITAL SIGNS	GE HEALTHCARE	DINAMAP PROCARE 300	AAW05230200SA	Ward A3	DEFECTIVE	18JUN24 Cal ไม่ผ่าน ไม่สามารถซ่อมได้
31	PLK00516	-	-	INFUSION PUMPS	TOP	TOP-2200	BL79019S	Ward B3	ยกเลิกการใช้งาน	24JUN24
32	PLK00730	-	-	OXIMETERS, PULSE	EDAN	H100B	113575-M11A01970005	Ward B3	ยกเลิกการใช้งาน	25/06
33	PLK01461	-	-	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	1410120010004	Ward B3	DEFECTIVE	24JUN24 ส่งซ่อมบริษัท
34	PLK00704	-	-	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	1410120010025	Ward B4	DEFECTIVE	24JUN24 ส่งซ่อมบริษัท
35	PLK00712	-	-	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	1410120010041	Ward B4	DEFECTIVE	24JUN24 ส่งซ่อมบริษัท
36	PLK00714	-	-	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	1410120020056	Ward B4	DEFECTIVE	24JUN24 ส่งซ่อมบริษัท
37	PLK00210	-	-	INFUSION PUMPS	TOP	TOP-2300	14A0786	Ward B5	ยกเลิกการใช้งาน	24JUN24
38	PLK01310	-	-	MONITORS, PHYSIOLOGIC, VITAL SIGNS	CRITIKON DINAMAP	8101	8101-H5858	Ward B5	ยกเลิกออกจากแผนชั่วคราว	25/06 CAL DEC
39	PLK00373	-	-	INFUSION PUMPS	TOP	TOP-2300	GU26897B	Ward B6	หาเครื่องไม่พบ	
40	PLK01050	-	-	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	6010181105762	Ward B7	หาเครื่องไม่พบ	
41	PLK01526	-	-	INFUSION PUMPS	MEDCAPTAIN	SYS-6010	6010171206799	Ward B8	DEFECTIVE	24JUN24 ค่า Occlusion ไม่ผ่าน
42	PLK00017	-	-	INJECTORS, CONTRAST MEDIA	Apollo	APO 100	APO1002Z161003	X-RAY	DEFECTIVE	25/06