

IINTS-AF

Learning-Enhanced Clinical Report

Session ID: 20260617_175037

Duration: 23.9 hours

Data points: 288

Report Date: 2026-06-17 17:50

RESEARCH RUN SUMMARY

Time in range reached 82.6% with mean glucose 148 mg/dL.


Glucose variability was 19.6% CV and GMI was 6.8%.

All outputs are for simulation, research review, and education only.

Not a medical device. Not for treatment, diagnosis, or dosing decisions.

ALGORITHMIC PERFORMANCE ANALYSIS


Time in Range Comparison

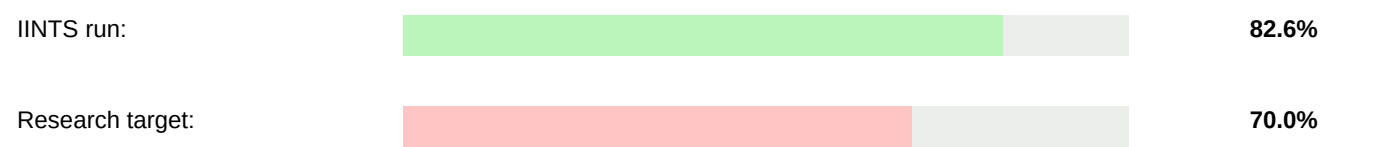

TIR 70-180 82.6% target framing	Mean glucose 148 mg/dL	CV 19.6% variability	Overrides 2 safety
--	---	---	---

Research Interpretation

This report shows whether a simulated glucose-control run stayed within common CGM research targets, how much hypoglycemia/hyperglycemia appeared, and whether the deterministic safety supervisor intervened. It is designed for pre-clinical discussion, not patient care.

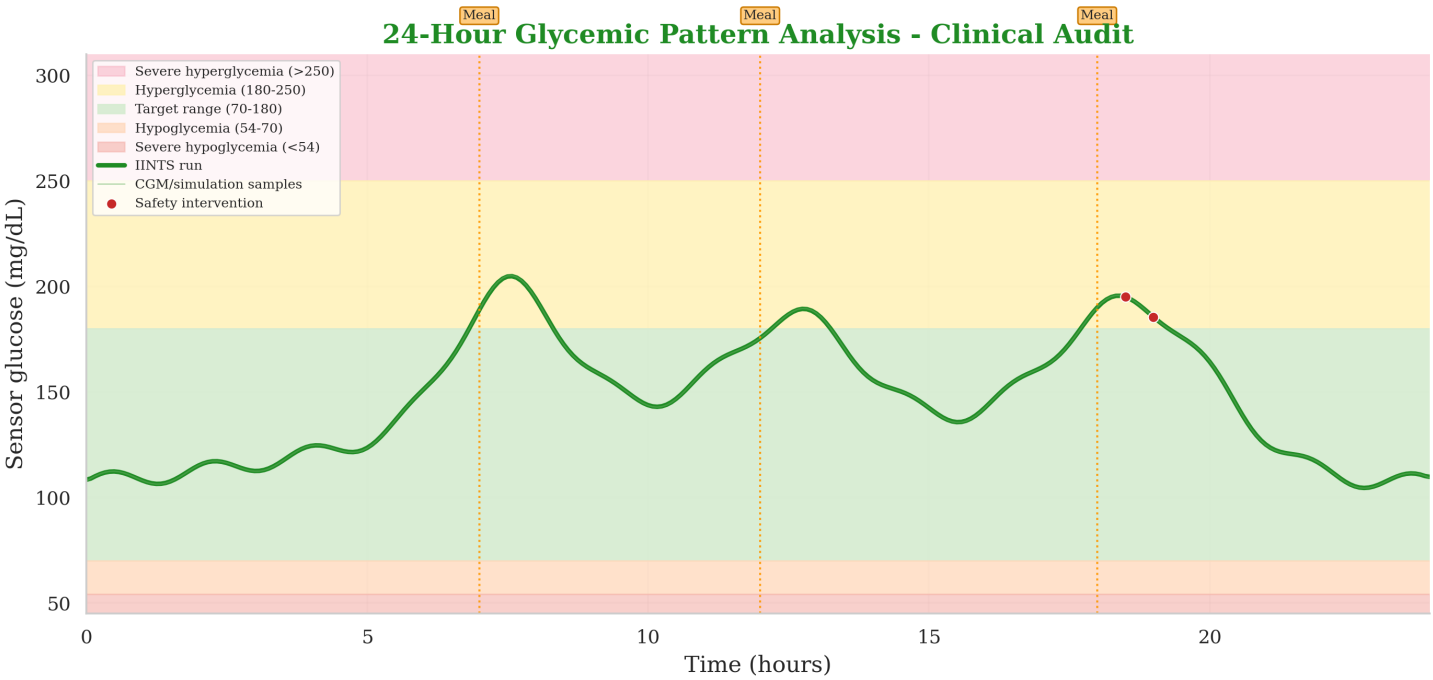

Clinical Metrics Summary


Metric	Result	Reference	Delta	Clinical note
Time in Range	82.6%	>=70%	+12.6	Primary CGM target metric
Mean Glucose	148 mg/dL	research range	-	Average glycemic exposure
Hypoglycemia	0.0%	<4%	+4.0	Low-glucose exposure
Variability (CV)	19.6%	<36%	+16.4	Glycemic stability

SAFETY VALIDATION RESULTS

Deterministic Safety Supervisor

- Total safety violations: 0
- Bolus interventions: 2
- Terminated early: False
- Research boundary: not a medical device and not for treatment decisions.
- Top intervention: Predicted low (2)

Insulin Delivery Trace

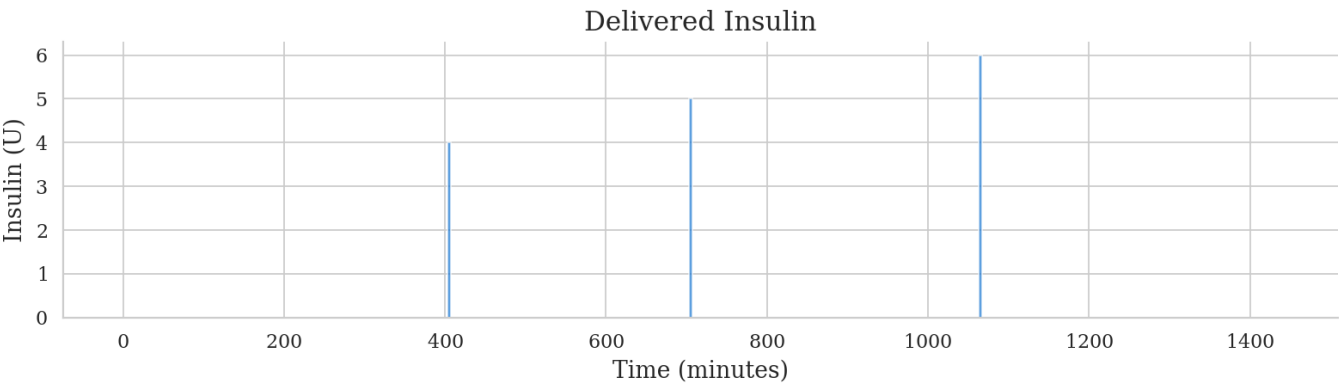

Research-use framing follows ADA 2026 glycemic goals and ATTD Time-in-Range consensus. See docs/EVIDENCE_BASE.md and `iints sources` for full citations.