Corrected ablation outcomes by removed component

Ten problem−metric endpoints are counted for each component removal

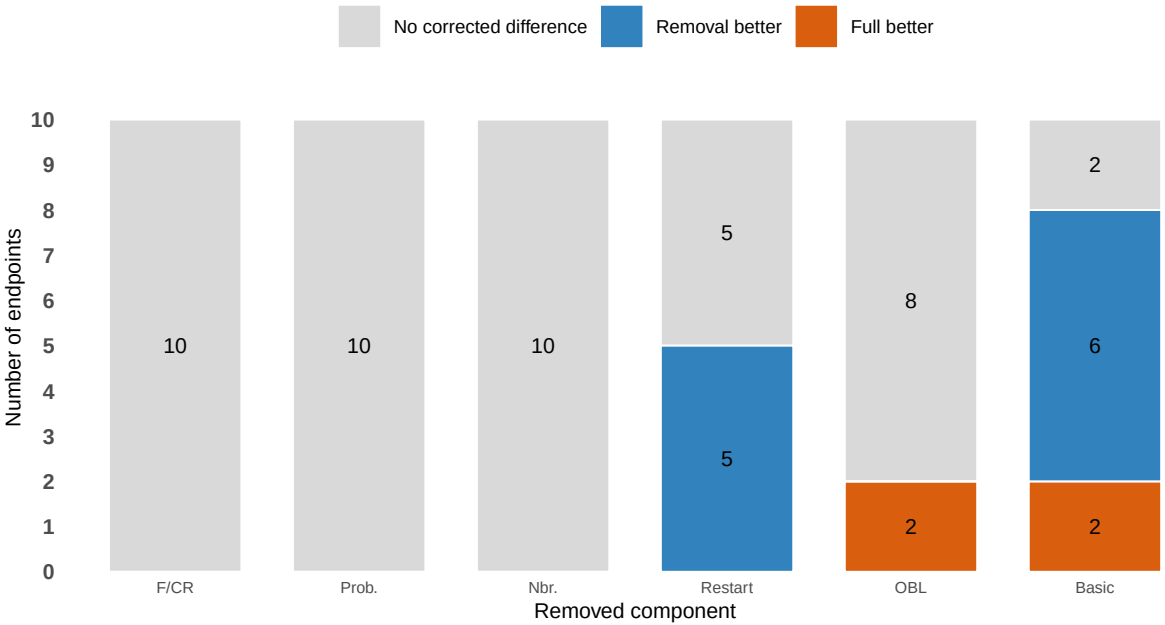

Two−sided paired Wilcoxon tests with Holm adjustment; n = 30 paired runs per endpoint.