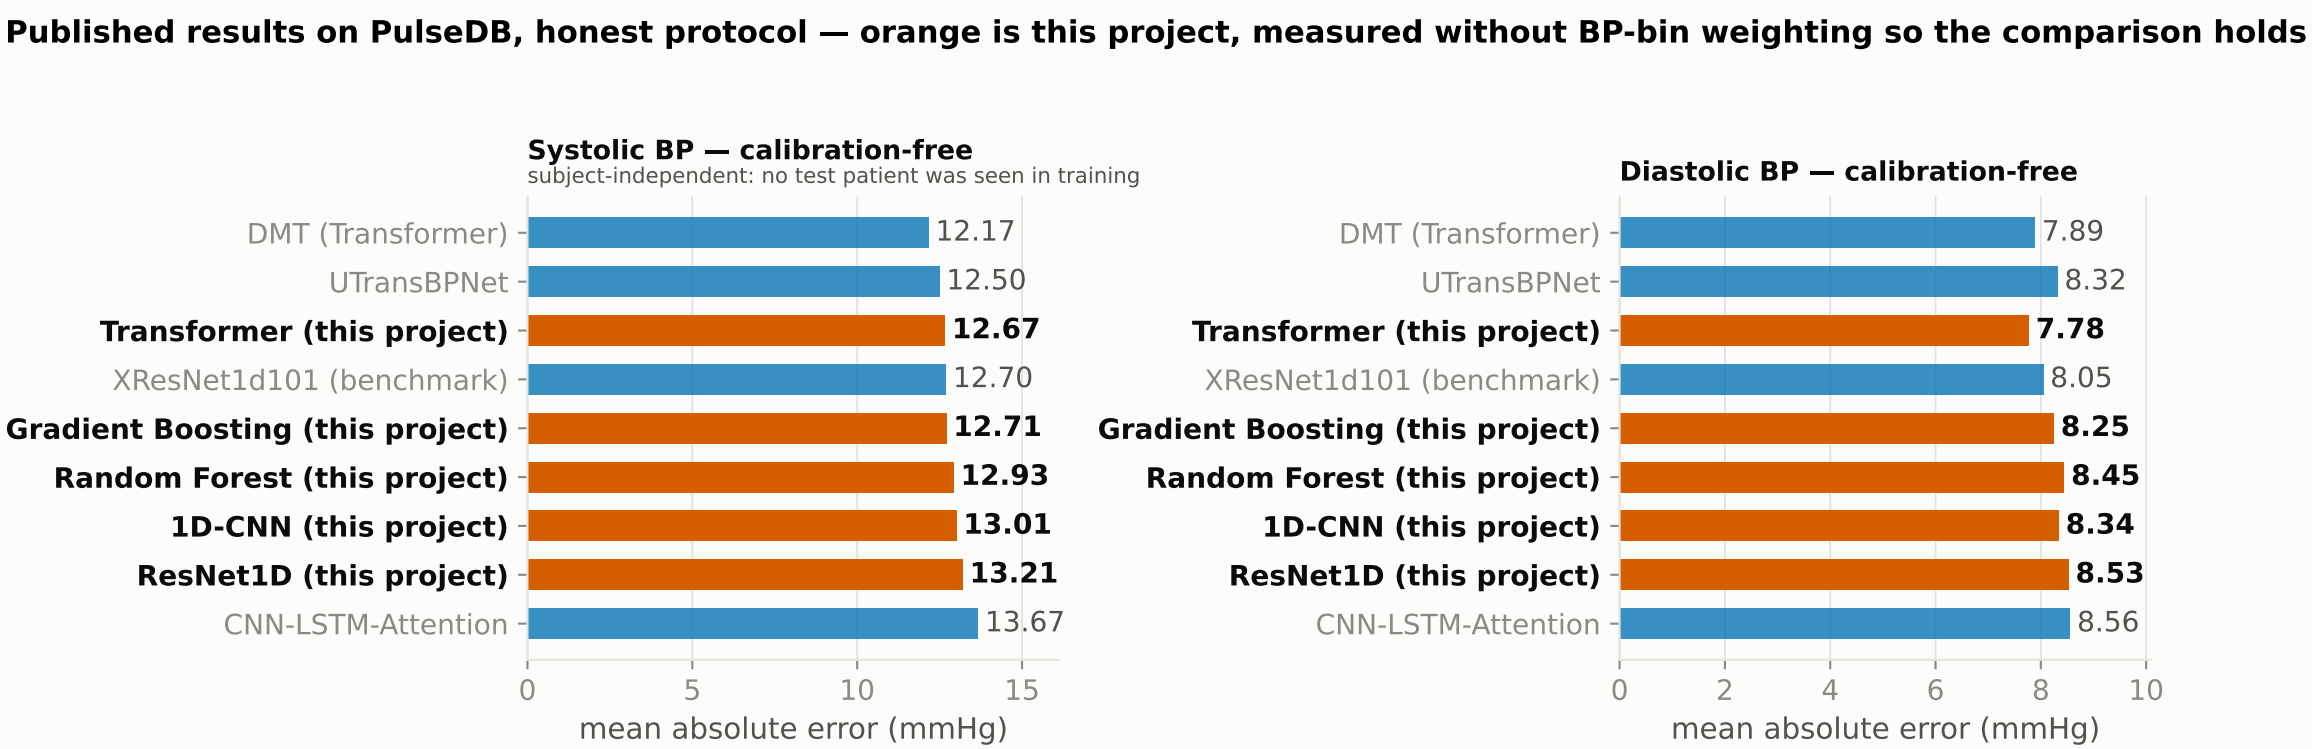
Published results on PulseDB, honest protocol — orange is this project, measured without BP-bin weighting so the comparison holds
Systolic BP — calibration-free
subject-independent: no test patient was seen in training
DMT (Transformer)
12.17
UTransBPNet
12.50
Transformer (this project)
12.67
XResNet1d101 (benchmark)
12.70
Gradient Boosting (this project)
12.71
Random Forest (this project)
12.93
1D-CNN (this project)
13.01
ResNet1D (this project)
13.21
CNN-LSTM-Attention
13.67
0
5
10
15
mean absolute error (mmHg)
Diastolic BP — calibration-free
DMT (Transformer)
7.89
UTransBPNet
8.32
Transformer (this project)
7.78
XResNet1d101 (benchmark)
8.05
Gradient Boosting (this project)
8.25
Random Forest (this project)
8.45
1D-CNN (this project)
8.34
ResNet1D (this project)
8.53
CNN-LSTM-Attention
8.56
0
2
4
6
8
10
mean absolute error (mmHg)