Leaky

random clips, any patient

Calibration-based

held-out clips, same patients

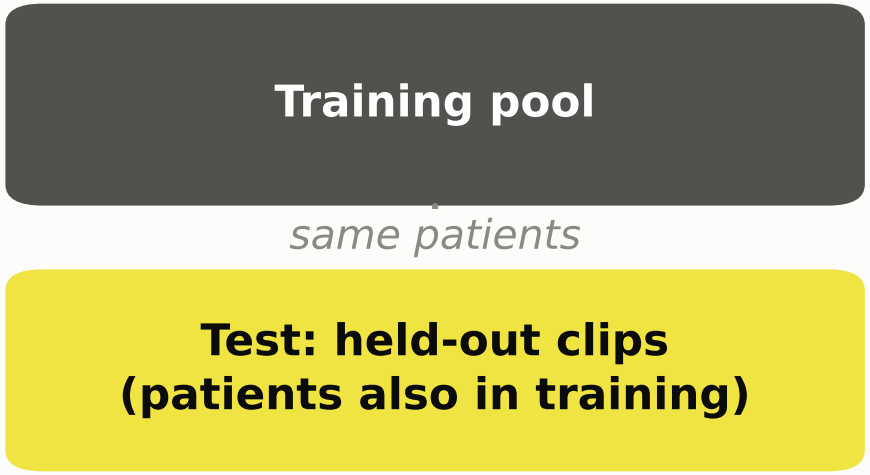

Calibration-free

144 unseen patients

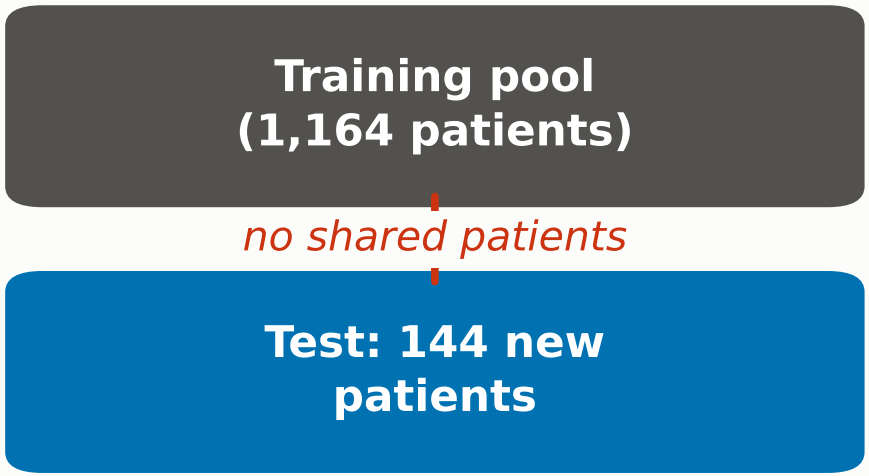

AAMI
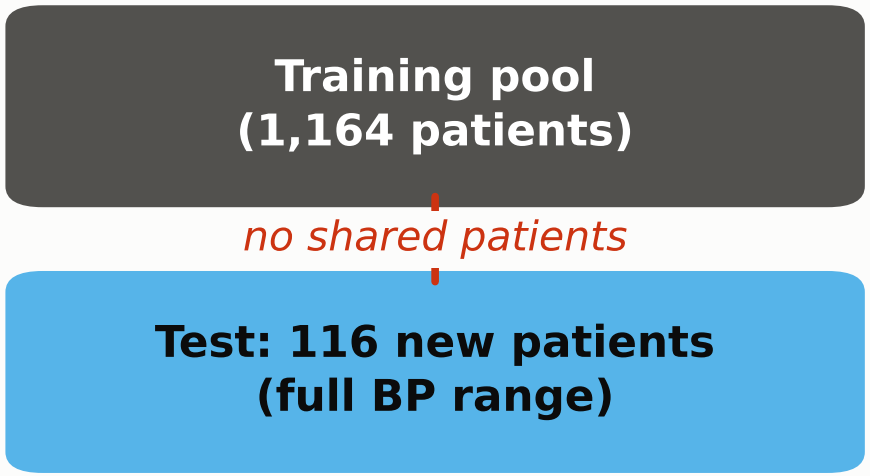
116 unseen patients, full BP range