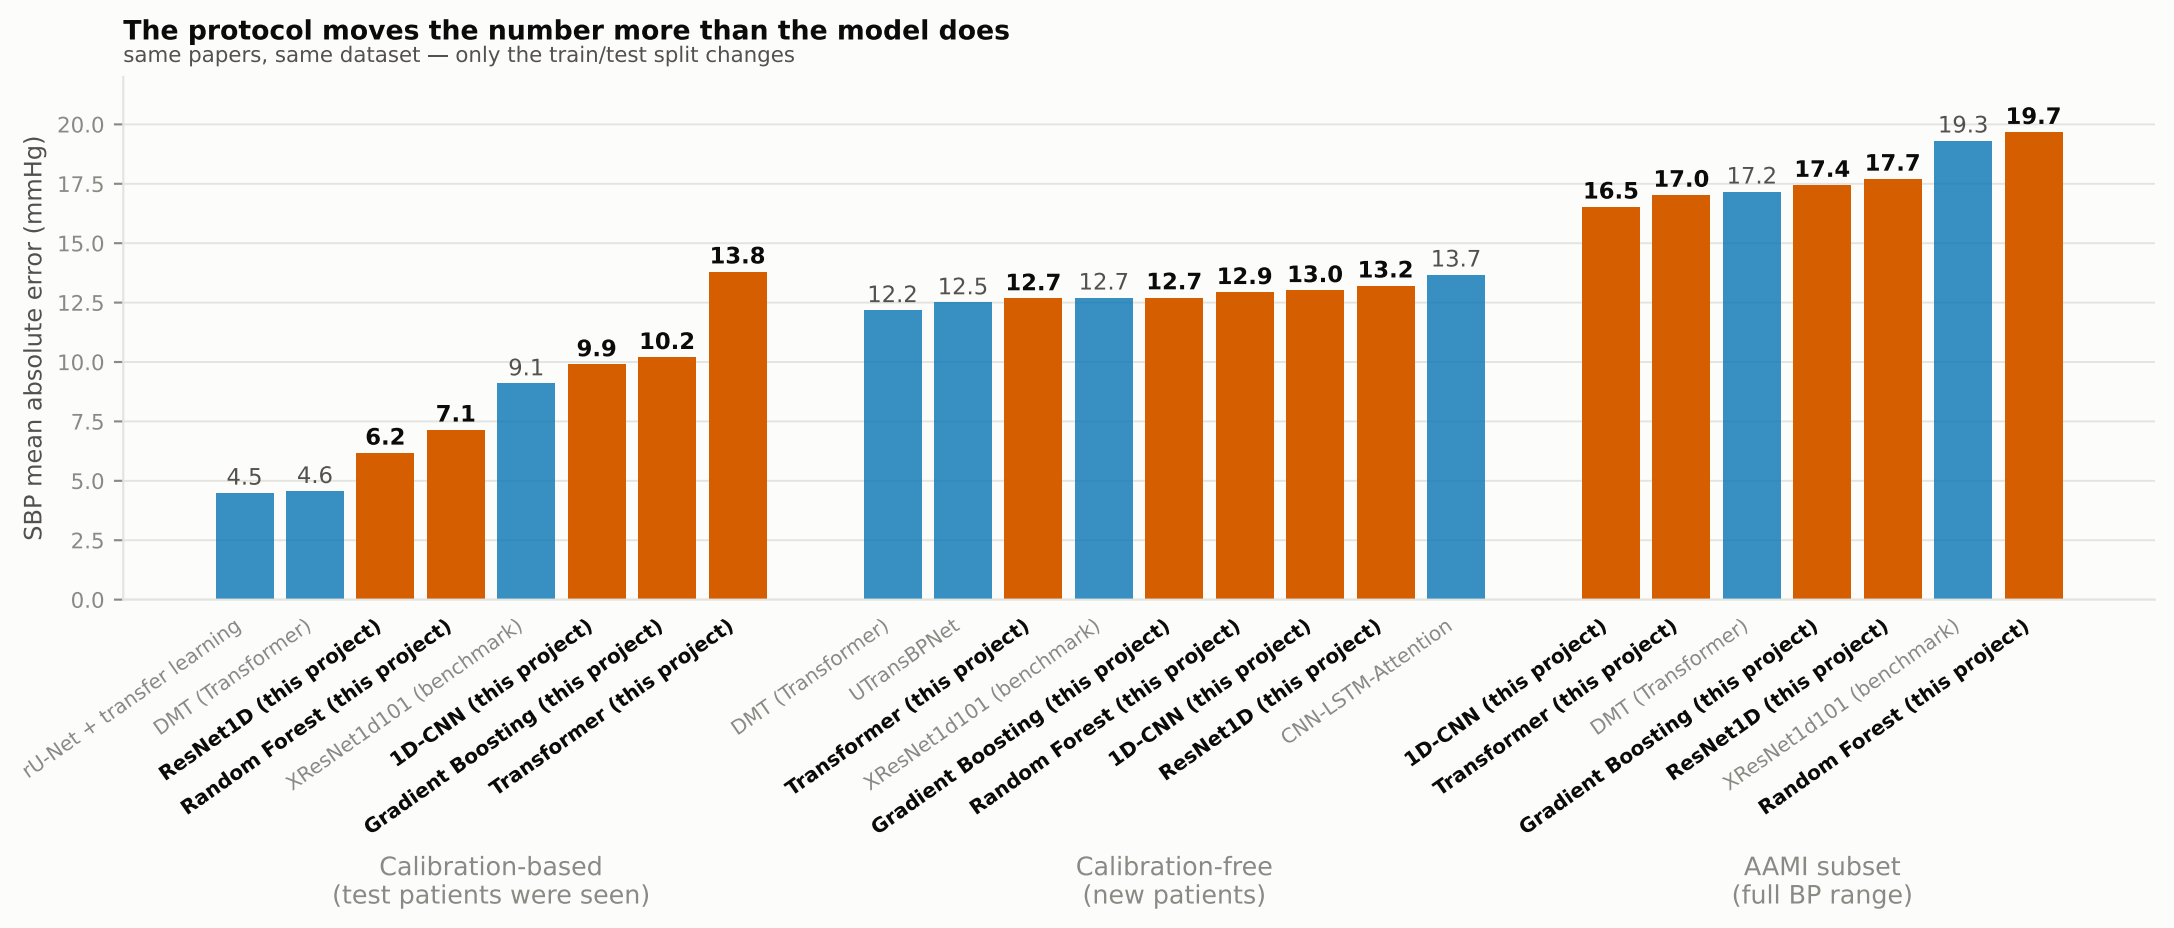
The protocol moves the number more than the model does
same papers, same dataset — only the train/test split changes
SBP mean absolute error (mmHg)
0.0
2.5
5.0
7.5
10.0
12.5
15.0
17.5
20.0
4.5
4.6
6.2
7.1
9.1
9.9
10.2
13.8
12.2
12.5
12.7
12.7
12.7
12.9
13.0
13.2
13.7
16.5
17.0
17.2
17.4
17.7
19.3
19.7
rU-Net + transfer learning
DMT (Transformer)
ResNet1D (this project)
Random Forest (this project)
XResNet1d101 (benchmark)
1D-CNN (this project)
Gradient Boosting (this project)
Transformer (this project)
DMT (Transformer)
UTransBPNet
Transformer (this project)
XResNet1d101 (benchmark)
Gradient Boosting (this project)
Random Forest (this project)
1D-CNN (this project)
ResNet1D (this project)
CNN-LSTM-Attention
1D-CNN (this project)
Transformer (this project)
DMT (Transformer)
Gradient Boosting (this project)
ResNet1D (this project)
XResNet1d101 (benchmark)
Random Forest (this project)
Calibration-based
(test patients were seen)
Calibration-free
(new patients)
AAMI subset
(full BP range)