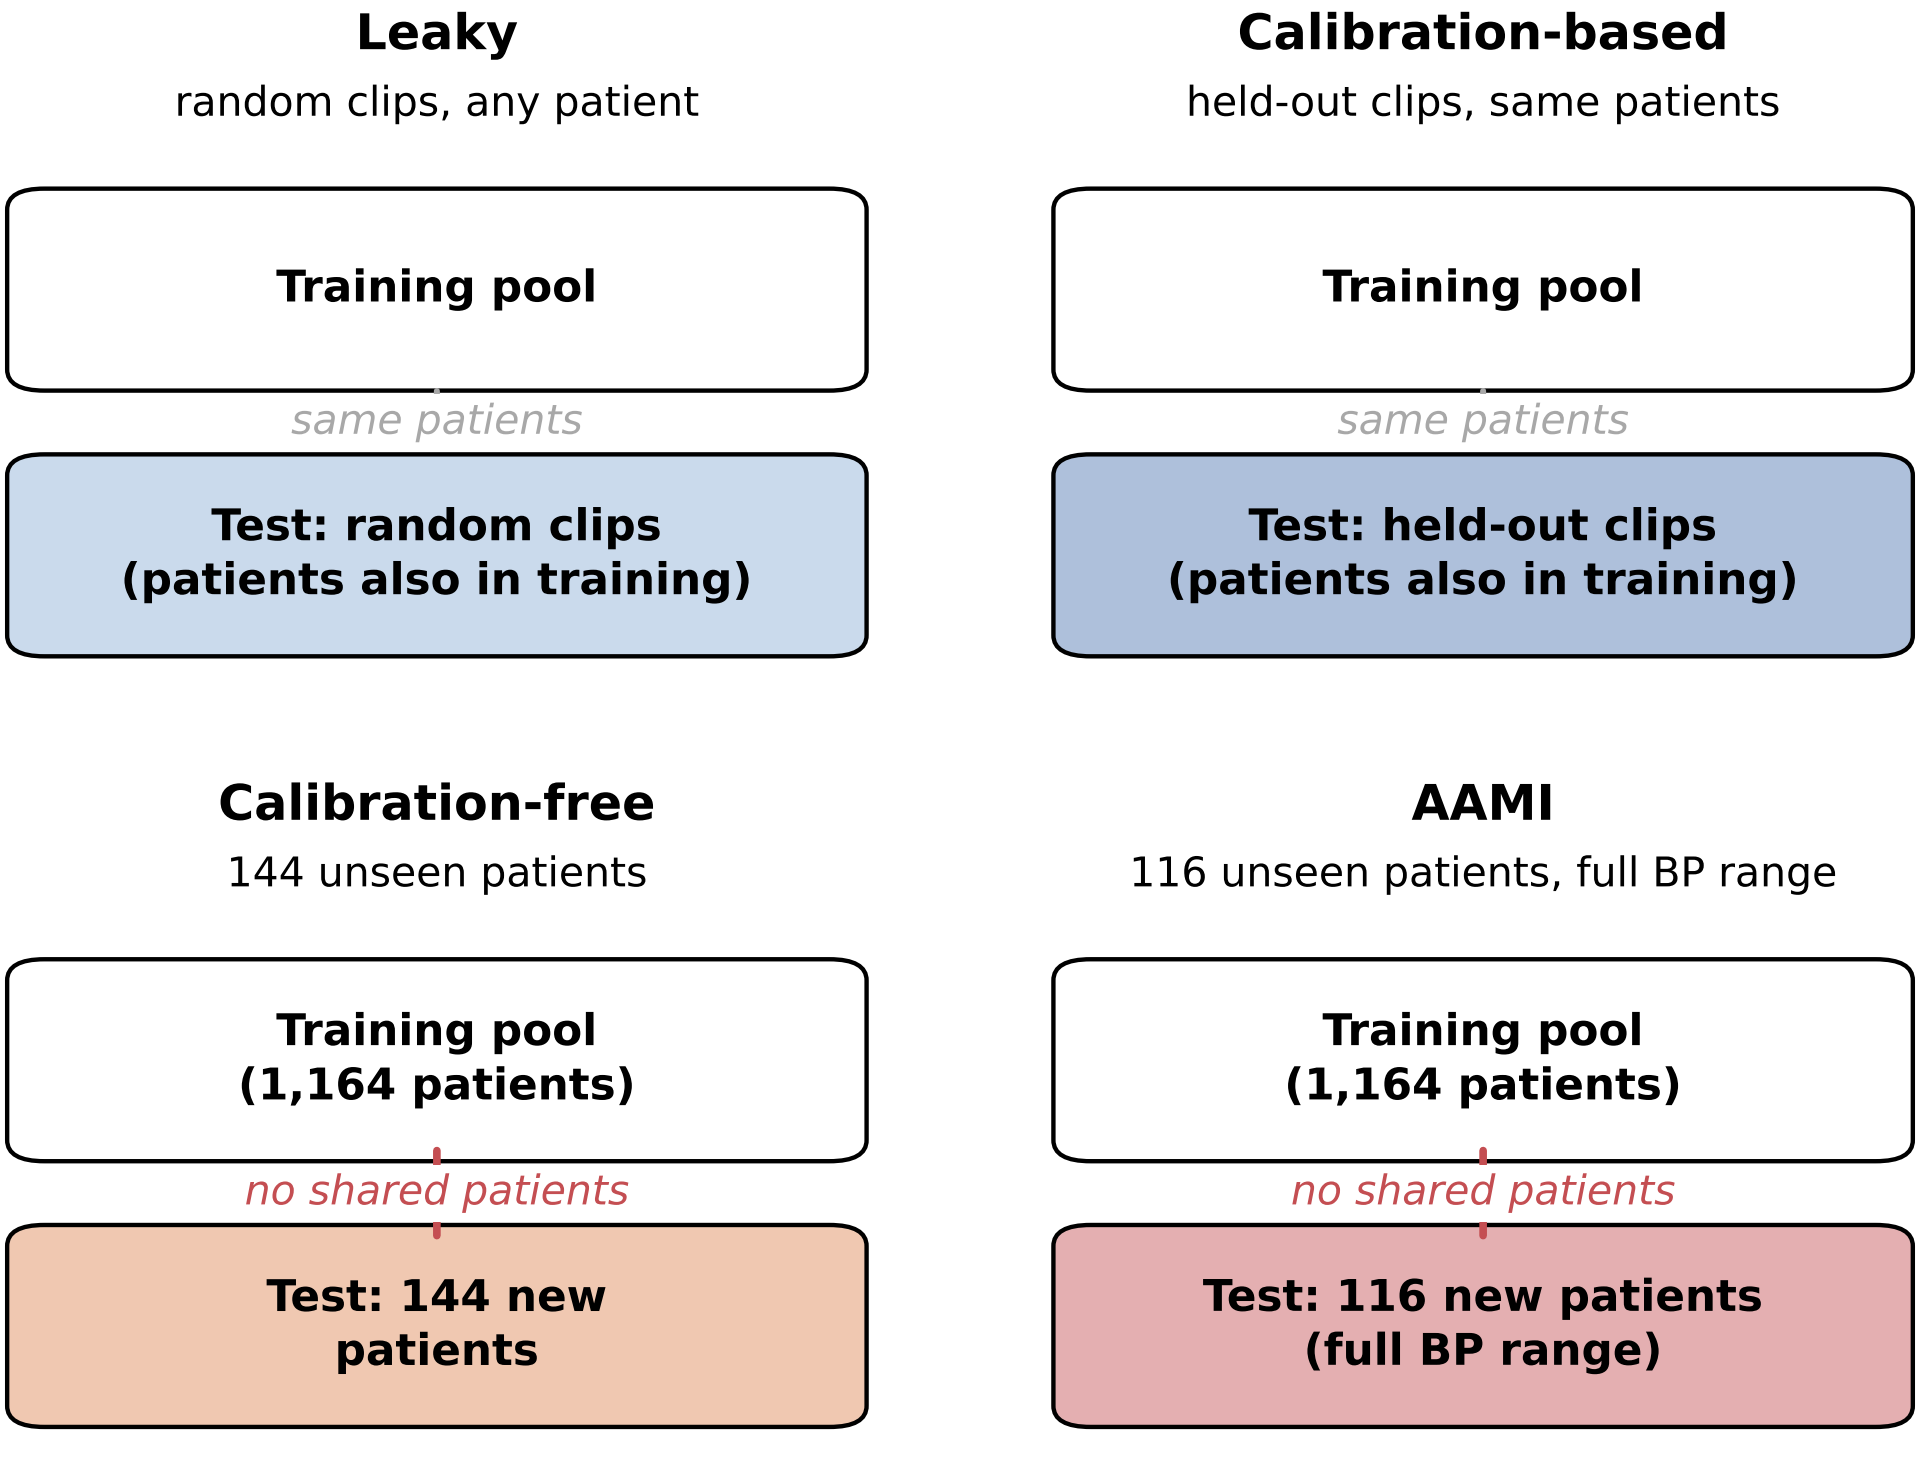
Leaky
random clips, any patient
Training pool
same patients
Test: random clips
(patients also in training)
Calibration-based
held-out clips, same patients
Training pool
same patients
Test: held-out clips
(patients also in training)
Calibration-free
144 unseen patients
Training pool
(1,164 patients)
no shared patients
Test: 144 new
patients
AAMI
116 unseen patients, full BP range
Training pool
(1,164 patients)
no shared patients
Test: 116 new patients
(full BP range)